


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122419\
 Data File : BP001383.D
 Acq On : 24 Dec 2019 13:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 16:04:49 2019

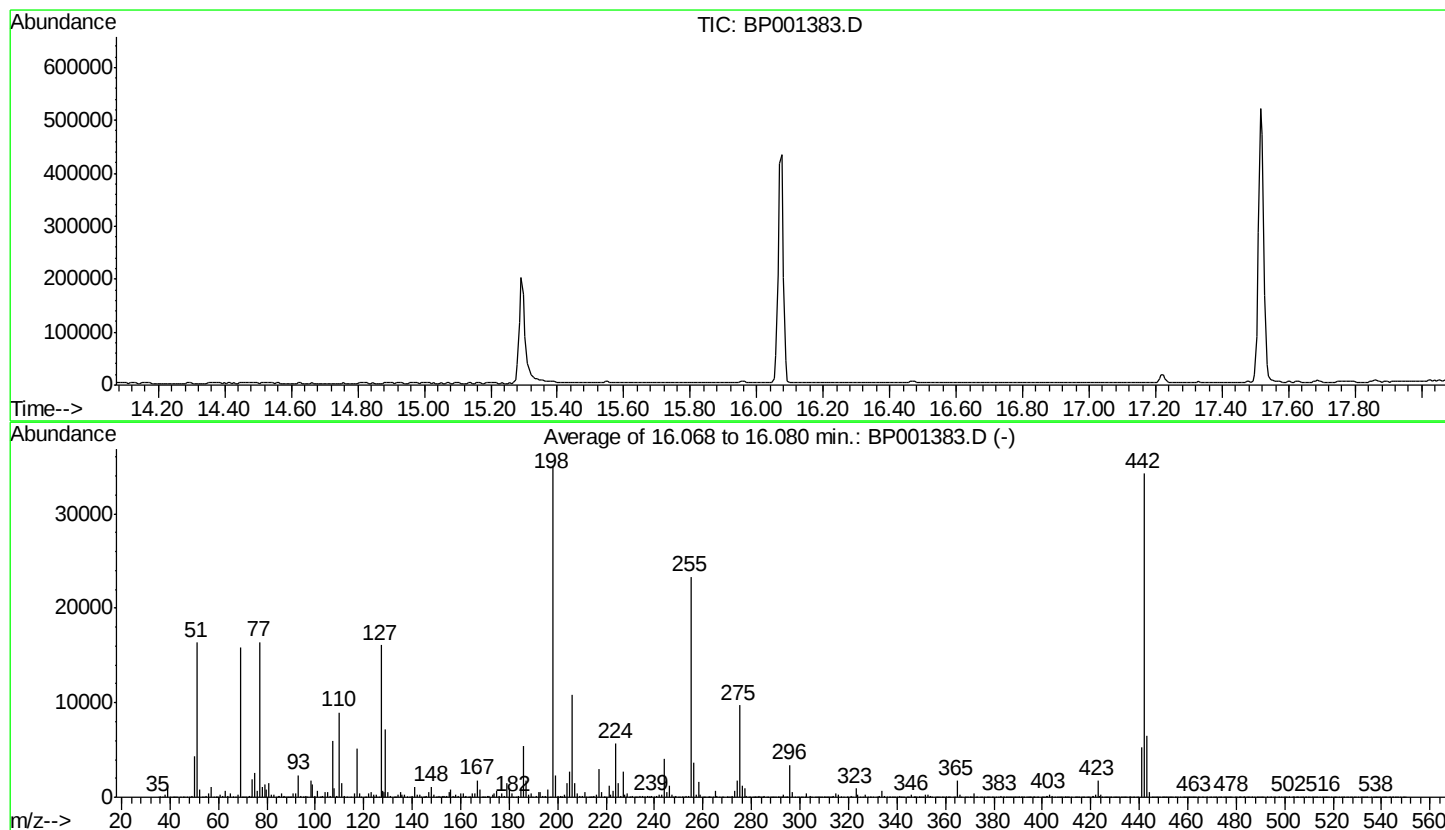

AutoFind: Scans 2377, 2378, 2379; Background Corrected with Scan 2370

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	16336	PASS
68	69	0.00	2	1.9	295	PASS
69	198	0.00	100	45.2	15859	PASS
70	69	0.00	2	0.3	44	PASS
127	198	10	80	45.8	16080	PASS
197	198	0.00	2	0.1	35	PASS
198	198	100	100	100.0	35106	PASS
199	198	5	9	6.7	2359	PASS
275	198	10	60	27.7	9727	PASS
365	198	1	100	5.0	1743	PASS
441	198	0.01	100	15.2	5322	PASS
442	198	50	100	97.7	34296	PASS
443	442	15	24	18.8	6457	PASS