


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122419\
 Data File : BP001407.D
 Acq On : 25 Dec 2019 05:03
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 16:04:49 2019

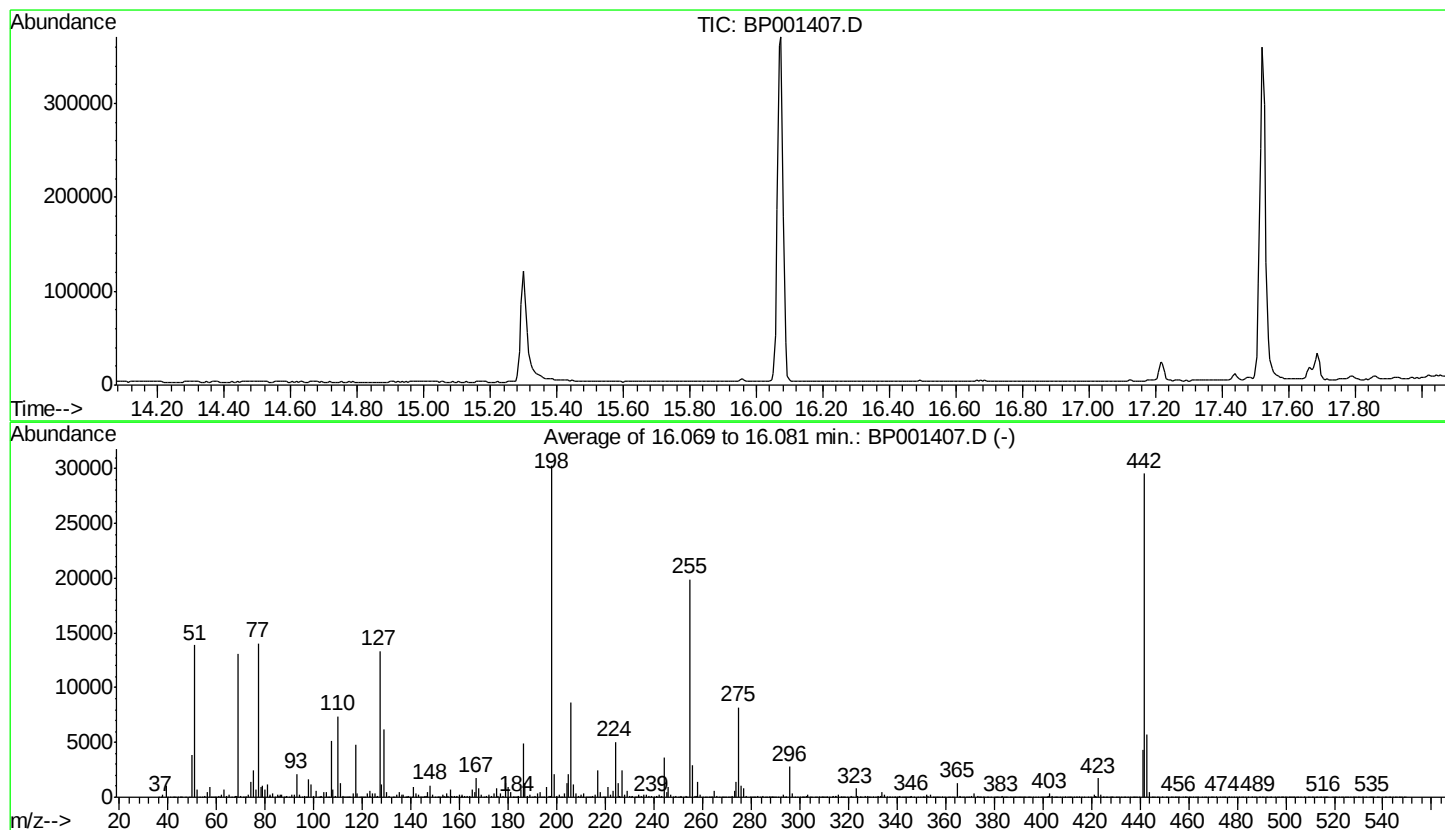

AutoFind: Scans 2377, 2378, 2379; Background Corrected with Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	13875	PASS
68	69	0.00	2	1.0	136	PASS
69	198	0.00	100	43.3	13086	PASS
70	69	0.00	2	0.7	88	PASS
127	198	10	80	44.2	13359	PASS
197	198	0.00	2	0.3	101	PASS
198	198	100	100	100.0	30256	PASS
199	198	5	9	6.9	2099	PASS
275	198	10	60	27.2	8215	PASS
365	198	1	100	4.4	1343	PASS
441	198	0.01	100	14.5	4374	PASS
442	198	50	100	97.7	29562	PASS
443	442	15	24	19.4	5747	PASS