

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
 Data File : BP004430.D
 Acq On : 24 Dec 2020 12:25
 Operator : CG/JU
 Sample : L5132-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.364	198	200	208	rVB	43391	55740	1.14%	0.115%
2	4.952	298	300	308	rVB	28251	45777	0.94%	0.095%
3	6.993	640	647	663	rVB2	692183	1357359	27.85%	2.807%
4	7.158	669	675	687	rVB	568497	905297	18.58%	1.872%
5	7.358	703	709	717	rBV	732800	1171283	24.04%	2.422%
6	7.828	782	789	796	rBV	787109	1299594	26.67%	2.688%
7	8.528	901	908	920	rBV	828954	1347221	27.65%	2.786%
8	8.981	978	985	995	rBV	642682	1076263	22.09%	2.226%
9	9.411	1054	1058	1064	rVB	27465	42509	0.87%	0.088%
10	9.705	1101	1108	1116	rBV	489840	851707	17.48%	1.761%
11	10.240	1192	1199	1212	rBV	809166	1408923	28.91%	2.914%
12	10.622	1255	1264	1275	rBV	1052289	1804445	37.03%	3.732%
13	10.752	1279	1286	1300	rVV	764901	1345010	27.60%	2.782%
14	12.052	1503	1507	1513	rVB7	4996	9045	0.19%	0.019%
15	12.116	1513	1518	1522	rBV7	2637	5155	0.11%	0.011%
16	12.210	1529	1534	1540	rVB2	14307	23612	0.48%	0.049%
17	13.304	1714	1720	1726	rBV6	7780	13693	0.28%	0.028%
18	13.363	1726	1730	1736	rVV3	7854	12973	0.27%	0.027%
19	13.434	1738	1742	1748	rVB8	4110	6887	0.14%	0.014%
20	13.875	1811	1817	1822	rBV	1359285	1946458	39.94%	4.026%
21	13.922	1822	1825	1834	rVB	331077	449028	9.21%	0.929%
22	14.163	1855	1866	1878	rBV	1784686	2648923	54.36%	5.478%
23	14.381	1898	1903	1907	rVB3	6642	9337	0.19%	0.019%
24	14.469	1907	1918	1927	rBV	1471652	2286388	46.92%	4.729%
25	14.675	1944	1953	1975	rBV	467243	783447	16.08%	1.620%
26	14.893	1985	1990	1994	rVB5	6667	11789	0.24%	0.024%
27	15.110	2022	2027	2032	rVB4	5822	9407	0.19%	0.019%
28	15.287	2052	2057	2061	rBV6	3504	7434	0.15%	0.015%
29	15.334	2061	2065	2070	rVB5	6704	8950	0.18%	0.019%
30	15.469	2080	2088	2096	rBV	2184521	3125436	64.14%	6.464%
31	15.593	2103	2109	2123	rBV	426384	624099	12.81%	1.291%
32	15.710	2123	2129	2139	rVB	26103	46959	0.96%	0.097%
33	16.157	2199	2205	2209	rBV6	6238	10410	0.21%	0.022%
34	16.204	2209	2213	2218	rVV8	6261	11261	0.23%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
 Data File : BP004430.D
 Acq On : 24 Dec 2020 12:25
 Operator : CG/JU
 Sample : L5132-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	16.257	2218	2222	2230	rVB5	12731	22179	0.46%	0.046%
36	16.469	2253	2258	2263	rVB2	13618	19402	0.40%	0.040%
37	16.628	2280	2285	2290	rVB9	2716	5430	0.11%	0.011%
38	17.010	2345	2350	2355	rBV2	6045	13807	0.28%	0.029%
39	17.234	2381	2388	2393	rBV	1854149	2711635	55.64%	5.608%
40	17.275	2393	2395	2398	rVV	40394	47076	0.97%	0.097%
41	17.328	2398	2404	2416	rVV	2313669	3420247	70.19%	7.074%
42	17.428	2416	2421	2426	rVV8	4164	7648	0.16%	0.016%
43	17.816	2483	2487	2491	rBV3	7917	8889	0.18%	0.018%
44	18.122	2530	2539	2542	rBV6	31741	62045	1.27%	0.128%
45	18.292	2563	2568	2571	rBV5	12690	21445	0.44%	0.044%
46	18.322	2571	2573	2578	rVB2	7179	9127	0.19%	0.019%
47	18.592	2616	2619	2621	rBV3	5531	7961	0.16%	0.016%
48	18.863	2661	2665	2671	rBV2	21877	29472	0.60%	0.061%
49	18.998	2684	2688	2690	rBV5	5752	8778	0.18%	0.018%
50	19.216	2721	2725	2727	rBV	27907	36515	0.75%	0.076%
51	19.245	2727	2730	2735	rVB	44841	63167	1.30%	0.131%
52	19.463	2764	2767	2769	rBV	20272	25464	0.52%	0.053%
53	19.492	2769	2772	2778	rVB	64186	77424	1.59%	0.160%
54	19.575	2780	2786	2798	rVV	3150557	4390994	90.11%	9.081%
55	21.045	3032	3036	3043	rBV6	63247	147232	3.02%	0.305%
56	21.322	3078	3083	3096	rBV	2586970	3463661	71.08%	7.164%
57	21.439	3099	3103	3107	rBV2	65103	104932	2.15%	0.217%
58	22.957	3358	3361	3367	rVB2	89252	135185	2.77%	0.280%
59	23.533	3451	3459	3474	rVB	2340527	4873170	100.00%	10.079%
60	23.680	3477	3484	3497	rVB2	1759322	3648169	74.86%	7.545%
61	24.269	3581	3584	3592	rVB	123139	228552	4.69%	0.473%


Sum of corrected areas: 48351425

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
Data File : BP004430.D
Acq On : 24 Dec 2020 12:25
Operator : CG/JU
Sample : L5132-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
A54R6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

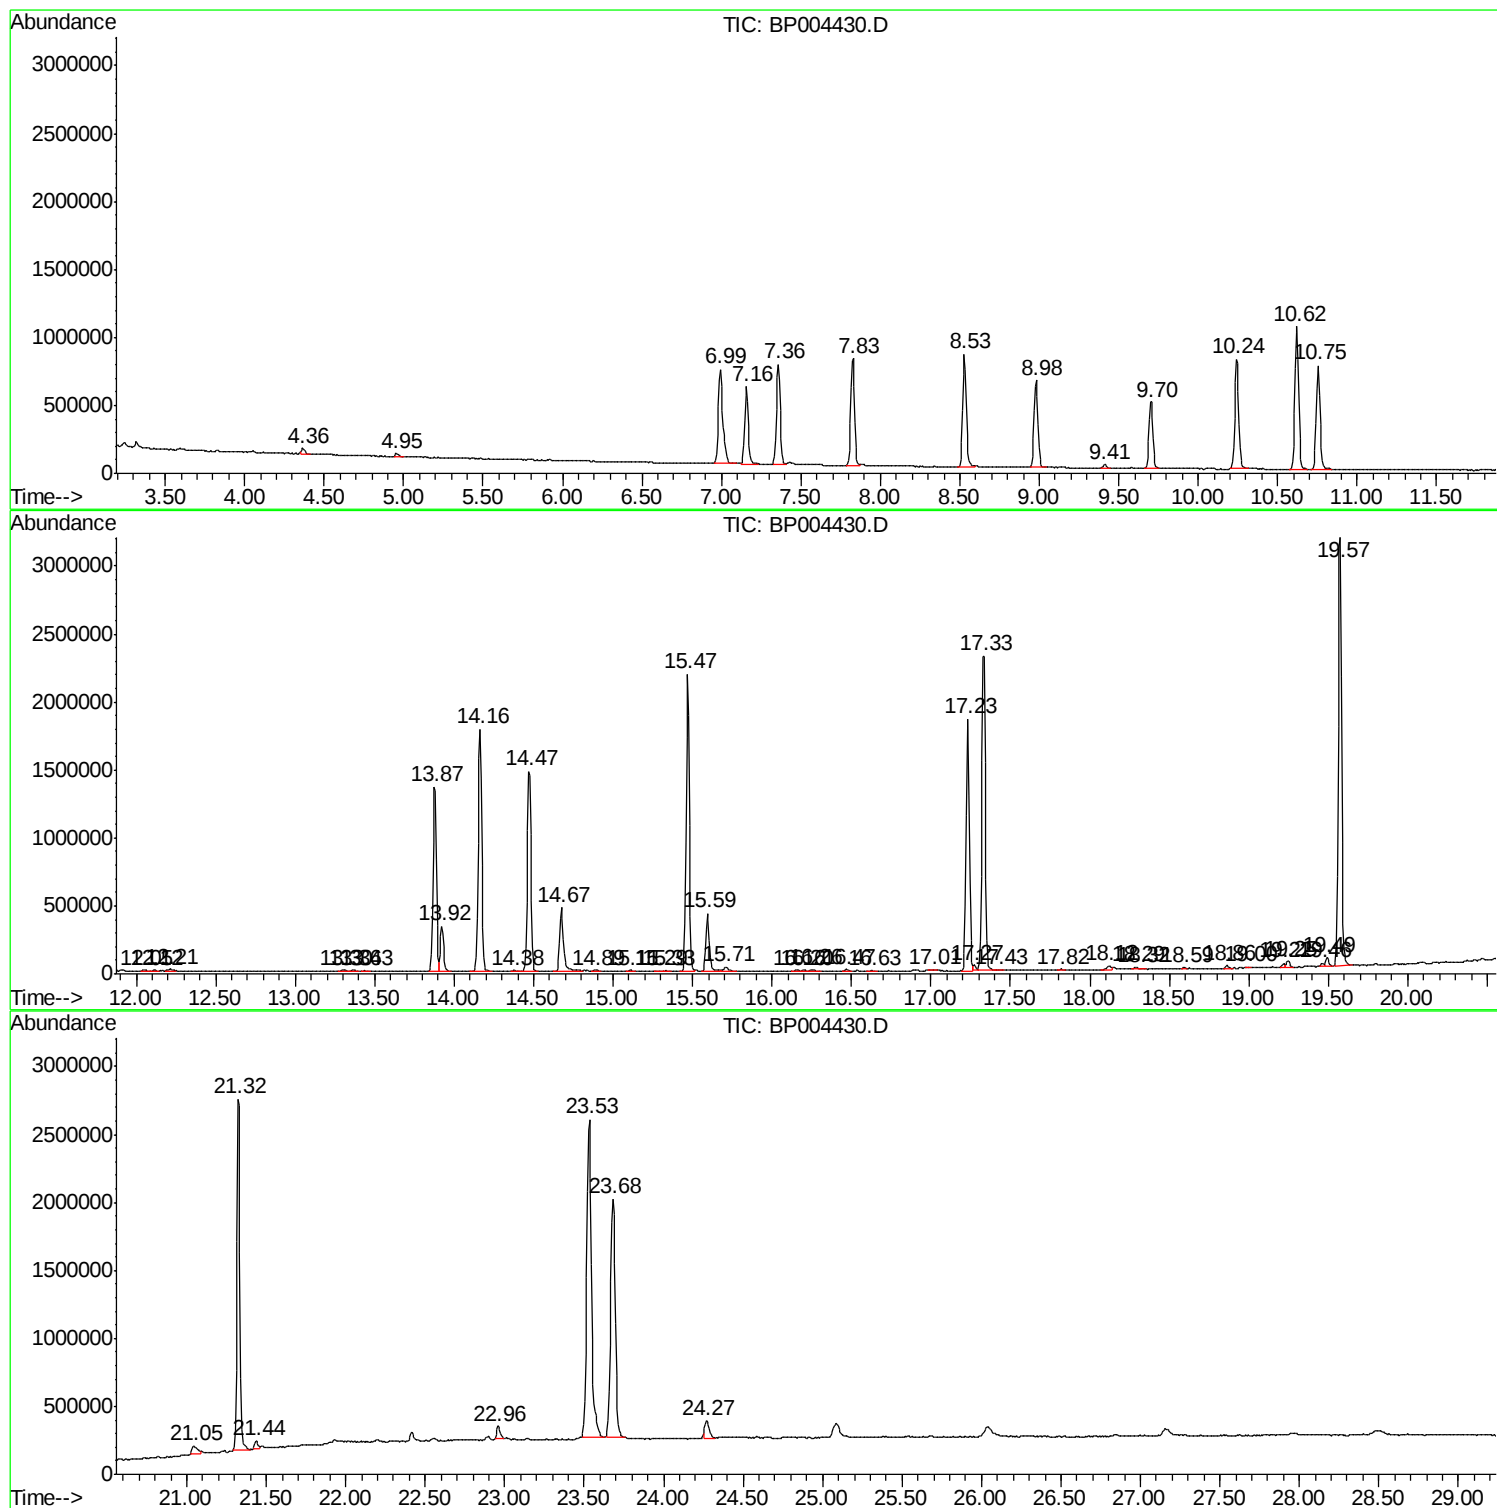

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004430.D
Acq On : 24 Dec 2020 12:25
Operator : CG/JU
Sample : L5132-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004430.D
Acq On : 24 Dec 2020 12:25
Operator : CG/JU
Sample : L5132-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc