

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
 Data File : BP004440.D
 Acq On : 24 Dec 2020 19:26
 Operator : CG/JU
 Sample : L5132-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.987	640	646	660	rVB2	716443	1438047	31.10%	3.128%
2	7.152	668	674	683	rBV	622450	994527	21.51%	2.163%
3	7.352	702	708	717	rBV	779474	1254808	27.13%	2.729%
4	7.822	781	788	795	rBV	739475	1217459	26.33%	2.648%
5	8.522	901	907	918	rBV	715856	1173426	25.37%	2.552%
6	8.975	977	984	994	rBV	714162	1179961	25.52%	2.566%
7	9.405	1052	1057	1065	rVB	56516	92386	2.00%	0.201%
8	9.699	1100	1107	1116	rBV	564748	967877	20.93%	2.105%
9	10.234	1191	1198	1215	rBV	884596	1543808	33.38%	3.358%
10	10.616	1255	1263	1273	rBV	944137	1627848	35.20%	3.540%
11	10.752	1278	1286	1298	rBV	786407	1380853	29.86%	3.003%
12	11.793	1457	1463	1466	rBV8	3590	6276	0.14%	0.014%
13	11.910	1479	1483	1489	rVB5	3484	6091	0.13%	0.013%
14	12.040	1501	1505	1511	rVB6	6331	11996	0.26%	0.026%
15	12.105	1512	1516	1524	rVB5	5679	11067	0.24%	0.024%
16	12.204	1528	1533	1541	rVB3	16102	30502	0.66%	0.066%
17	12.499	1578	1583	1586	rBV6	3112	5163	0.11%	0.011%
18	13.299	1712	1719	1725	rBV2	14328	24371	0.53%	0.053%
19	13.363	1725	1730	1738	rVV3	11184	22599	0.49%	0.049%
20	13.434	1738	1742	1749	rVB6	5872	9309	0.20%	0.020%
21	13.875	1810	1817	1821	rBV	1497729	2158042	46.67%	4.693%
22	13.922	1821	1825	1835	rVV	369509	530761	11.48%	1.154%
23	13.999	1835	1838	1844	rVB6	4275	7580	0.16%	0.016%
24	14.157	1855	1865	1877	rBV	1904312	2825395	61.10%	6.145%
25	14.375	1898	1902	1906	rVB2	9913	13819	0.30%	0.030%
26	14.469	1910	1918	1930	rVV	1361943	2049876	44.33%	4.458%
27	14.669	1945	1952	1967	rBV	415639	694759	15.02%	1.511%
28	14.887	1984	1989	1993	rVB8	5647	10281	0.22%	0.022%
29	15.104	2022	2026	2031	rVB3	8649	13190	0.29%	0.029%
30	15.275	2050	2055	2057	rBV3	5347	7601	0.16%	0.017%
31	15.328	2061	2064	2067	rVB3	8009	10015	0.22%	0.022%
32	15.463	2080	2087	2097	rBV	2318660	3386094	73.22%	7.364%
33	15.593	2102	2109	2124	rBV	432331	635269	13.74%	1.382%
34	15.704	2124	2128	2134	rVV3	25599	38763	0.84%	0.084%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
 Data File : BP004440.D
 Acq On : 24 Dec 2020 19:26
 Operator : CG/JU
 Sample : L5132-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	15.834	2146	2150	2155	rVB8	3825	5845	0.13%	0.013%
36	16.034	2180	2184	2191	rBV10	3171	6286	0.14%	0.014%
37	16.151	2198	2204	2207	rVV3	10477	18918	0.41%	0.041%
38	16.193	2209	2211	2216	rVV6	8889	14212	0.31%	0.031%
39	16.257	2217	2222	2226	rVB5	13470	22299	0.48%	0.048%
40	16.369	2238	2241	2245	rBV6	4104	6067	0.13%	0.013%
41	16.463	2253	2257	2263	rVB	21625	30216	0.65%	0.066%
42	16.540	2266	2270	2273	rBV6	3427	5791	0.13%	0.013%
43	16.616	2278	2283	2287	rBV6	5017	8867	0.19%	0.019%
44	16.704	2293	2298	2303	rBV8	3135	7264	0.16%	0.016%
45	16.769	2305	2309	2313	rBV6	6336	8896	0.19%	0.019%
46	16.904	2329	2332	2336	rVB6	5390	6377	0.14%	0.014%
47	16.975	2340	2344	2345	rBV4	3910	5211	0.11%	0.011%
48	17.228	2380	2387	2397	rBV	1590945	2261183	48.90%	4.918%
49	17.328	2397	2404	2417	rVV	2542167	3574375	77.29%	7.774%
50	17.422	2417	2420	2425	rVB7	5642	9203	0.20%	0.020%
51	17.604	2446	2451	2452	rBV5	5077	8493	0.18%	0.018%
52	18.122	2535	2539	2544	rBV7	14308	24660	0.53%	0.054%
53	18.857	2661	2664	2670	rVB	48003	60484	1.31%	0.132%
54	19.216	2721	2725	2729	rBV	28149	38369	0.83%	0.083%
55	19.463	2763	2767	2771	rBV	24894	32423	0.70%	0.071%
56	19.569	2779	2785	2799	rBV	3230345	4331928	93.67%	9.421%
57	21.039	3031	3035	3039	rBV5	93655	200697	4.34%	0.436%
58	21.322	3078	3083	3092	rVB	1999137	2615286	56.55%	5.688%
59	23.527	3450	3458	3475	rVB	2243956	4624492	100.00%	10.058%
60	23.674	3477	3483	3495	rVB2	1288488	2672435	57.79%	5.812%


Sum of corrected areas: 45980096

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
Data File : BP004440.D
Acq On : 24 Dec 2020 19:26
Operator : CG/JU
Sample : L5132-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

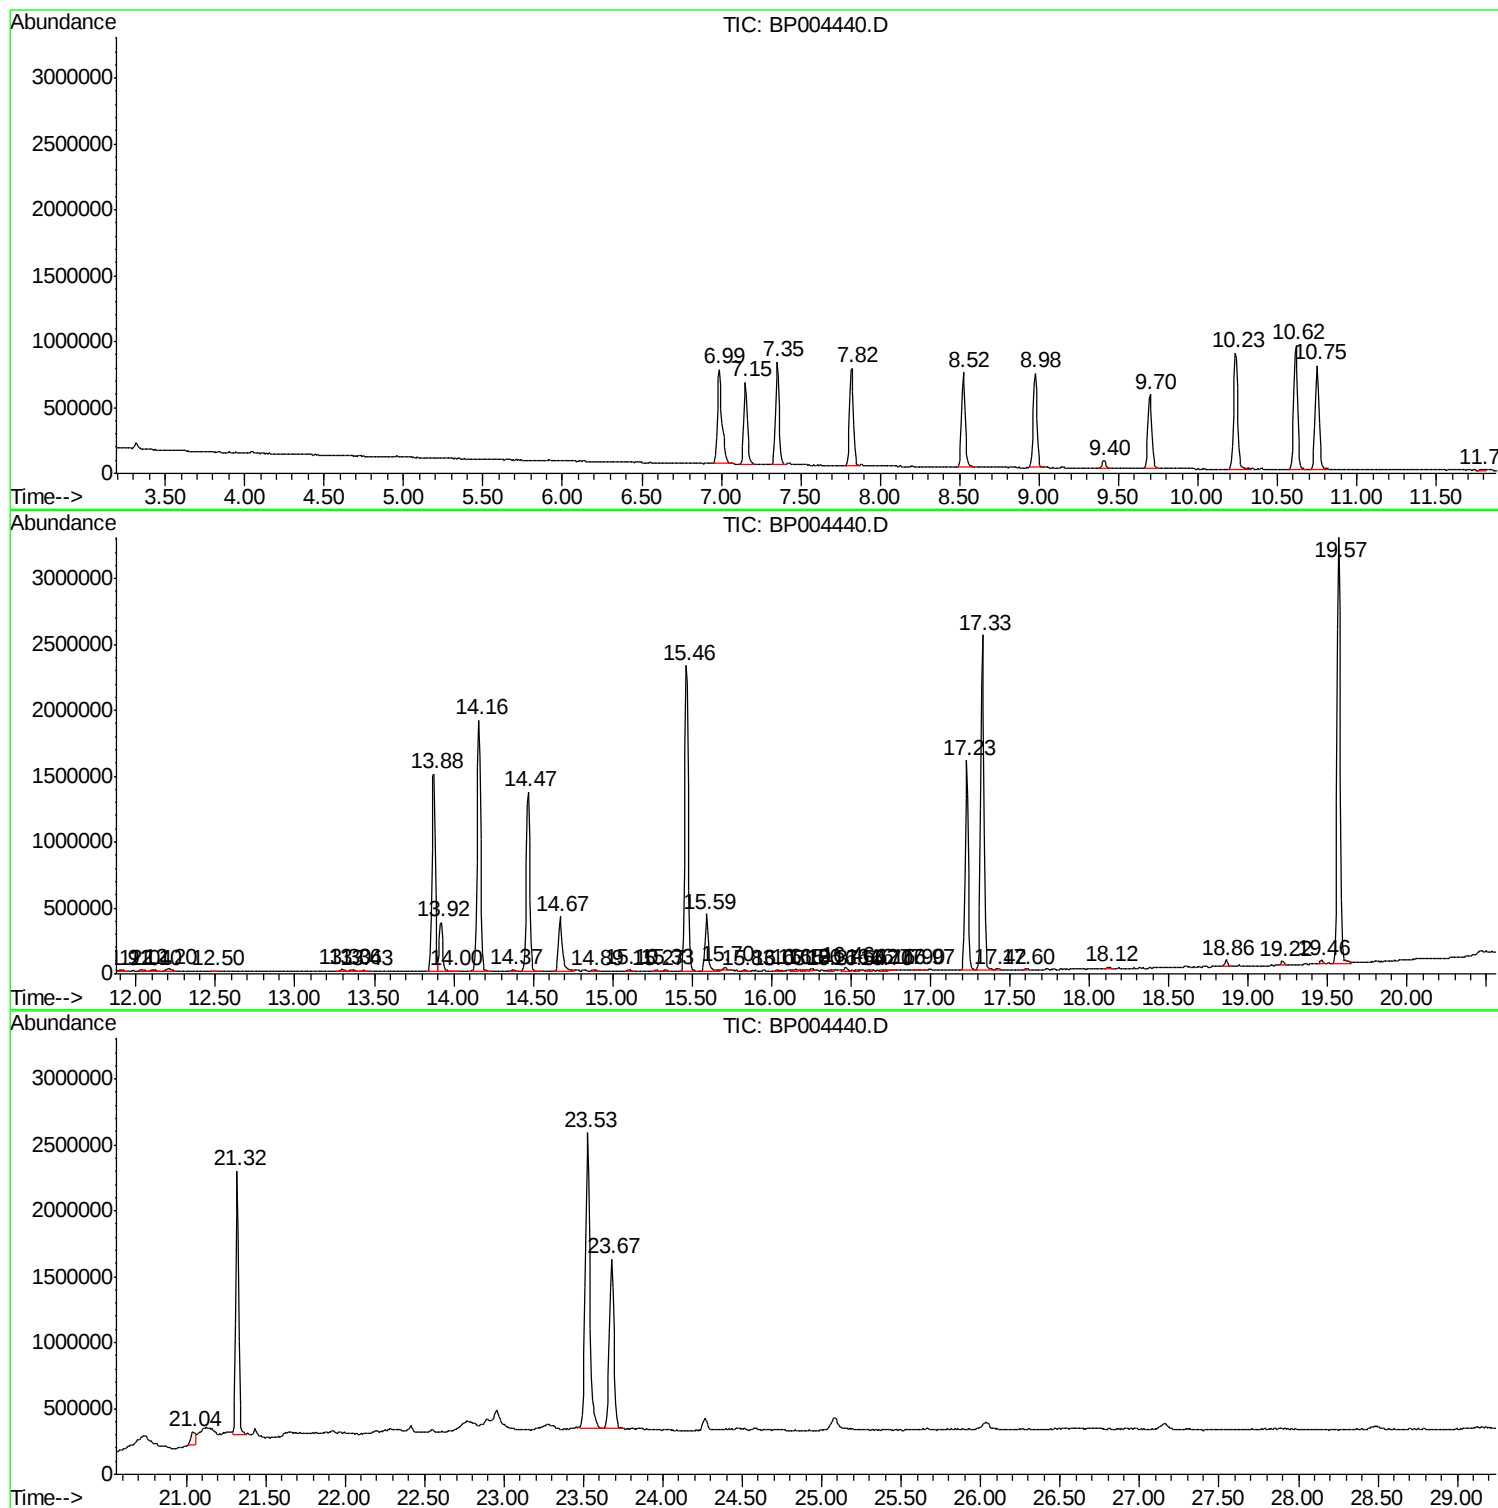

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004440.D
Acq On : 24 Dec 2020 19:26
Operator : CG/JU
Sample : L5132-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004440.D
Acq On : 24 Dec 2020 19:26
Operator : CG/JU
Sample : L5132-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc