

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
 Data File : BP004441.D
 Acq On : 24 Dec 2020 20:00
 Operator : CG/JU
 Sample : L5132-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54S4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	19	22	29	rVB2	50377	67325	1.16%	0.124%
2	6.987	640	646	658	rVB	789775	1373590	23.56%	2.537%
3	7.152	668	674	686	rVB	674884	1084190	18.60%	2.003%
4	7.352	702	708	721	rVB	863264	1395298	23.94%	2.578%
5	7.822	781	788	795	rBV	875846	1411822	24.22%	2.608%
6	8.522	900	907	919	rBV	947843	1582451	27.15%	2.923%
7	8.975	977	984	996	rVB	769013	1289396	22.12%	2.382%
8	9.404	1052	1057	1065	rVB	42627	67802	1.16%	0.125%
9	9.698	1100	1107	1119	rBV	591950	1009381	17.32%	1.865%
10	10.234	1191	1198	1216	rBV	962676	1694436	29.07%	3.130%
11	10.616	1255	1263	1276	rVV	1160196	1940829	33.30%	3.585%
12	10.751	1278	1286	1301	rVB	692308	1227272	21.05%	2.267%
13	12.045	1501	1506	1511	rVB7	4980	7946	0.14%	0.015%
14	12.204	1524	1533	1541	rBV2	17795	35520	0.61%	0.066%
15	13.069	1674	1680	1684	rVB6	7067	9289	0.16%	0.017%
16	13.298	1714	1719	1723	rBV2	12368	18038	0.31%	0.033%
17	13.363	1725	1730	1735	rVV4	11392	19555	0.34%	0.036%
18	13.434	1738	1742	1746	rVB5	4700	6027	0.10%	0.011%
19	13.875	1810	1817	1821	rBV	1593772	2291452	39.31%	4.233%
20	13.922	1821	1825	1833	rVV	256695	368940	6.33%	0.682%
21	13.998	1835	1838	1842	rVB5	4203	6218	0.11%	0.011%
22	14.157	1853	1865	1875	rBV	2086281	3198076	54.87%	5.908%
23	14.375	1897	1902	1906	rVB2	10936	15051	0.26%	0.028%
24	14.469	1911	1918	1931	rVB	1740062	2610452	44.78%	4.822%
25	14.669	1944	1952	1967	rBV	367550	635305	10.90%	1.174%
26	14.828	1974	1979	1984	rVB9	4910	8097	0.14%	0.015%
27	14.886	1984	1989	1995	rVB9	4049	10018	0.17%	0.019%
28	15.104	2022	2026	2030	rVB6	3752	6652	0.11%	0.012%
29	15.328	2061	2064	2069	rVB3	8185	10182	0.17%	0.019%
30	15.463	2080	2087	2102	rBV	2567208	3761355	64.53%	6.948%
31	15.592	2102	2109	2120	rVV	370855	551293	9.46%	1.018%
32	15.704	2123	2128	2137	rVV	32379	60816	1.04%	0.112%
33	15.833	2145	2150	2155	rBV9	3072	5973	0.10%	0.011%
34	15.951	2167	2170	2177	rVB9	2989	6371	0.11%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
 Data File : BP004441.D
 Acq On : 24 Dec 2020 20:00
 Operator : CG/JU
 Sample : L5132-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54S4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	16.033	2180	2184	2192	rBV9	3858	10997	0.19%	0.020%
36	16.157	2200	2205	2208	rBV6	3811	6984	0.12%	0.013%
37	16.198	2208	2212	2215	rVV5	5446	8920	0.15%	0.016%
38	16.251	2218	2221	2229	rVB7	13559	21194	0.36%	0.039%
39	16.463	2252	2257	2262	rVB	12856	18038	0.31%	0.033%
40	16.904	2327	2332	2336	rVB6	5813	7600	0.13%	0.014%
41	17.016	2341	2351	2360	rBV3	10697	33987	0.58%	0.063%
42	17.227	2380	2387	2397	rBV	2115028	3033967	52.05%	5.605%
43	17.327	2397	2404	2415	rVB2	2650653	3901408	66.93%	7.207%
44	17.610	2447	2452	2454	rBV6	4860	7547	0.13%	0.014%
45	18.122	2535	2539	2545	rBV7	9347	16392	0.28%	0.030%
46	18.192	2547	2551	2555	rVB3	3995	5853	0.10%	0.011%
47	19.216	2720	2725	2729	rBV	34433	51485	0.88%	0.095%
48	19.463	2763	2767	2770	rBV	24339	32831	0.56%	0.061%
49	19.569	2779	2785	2799	rBV	3647931	4856425	83.32%	8.971%
50	19.798	2821	2824	2828	rVB3	14693	16550	0.28%	0.031%
51	21.033	3031	3034	3047	rBV2	102513	291182	5.00%	0.538%
52	21.321	3078	3083	3093	rBV	3011554	3751718	64.36%	6.931%
53	23.527	3450	3458	3474	rVV	2842859	5828981	100.00%	10.768%
54	23.680	3476	3484	3496	rVB2	2070209	4206110	72.16%	7.770%
55	24.268	3580	3584	3590	rVB	129151	237736	4.08%	0.439%


Sum of corrected areas: 54132323

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
Data File : BP004441.D
Acq On : 24 Dec 2020 20:00
Operator : CG/JU
Sample : L5132-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

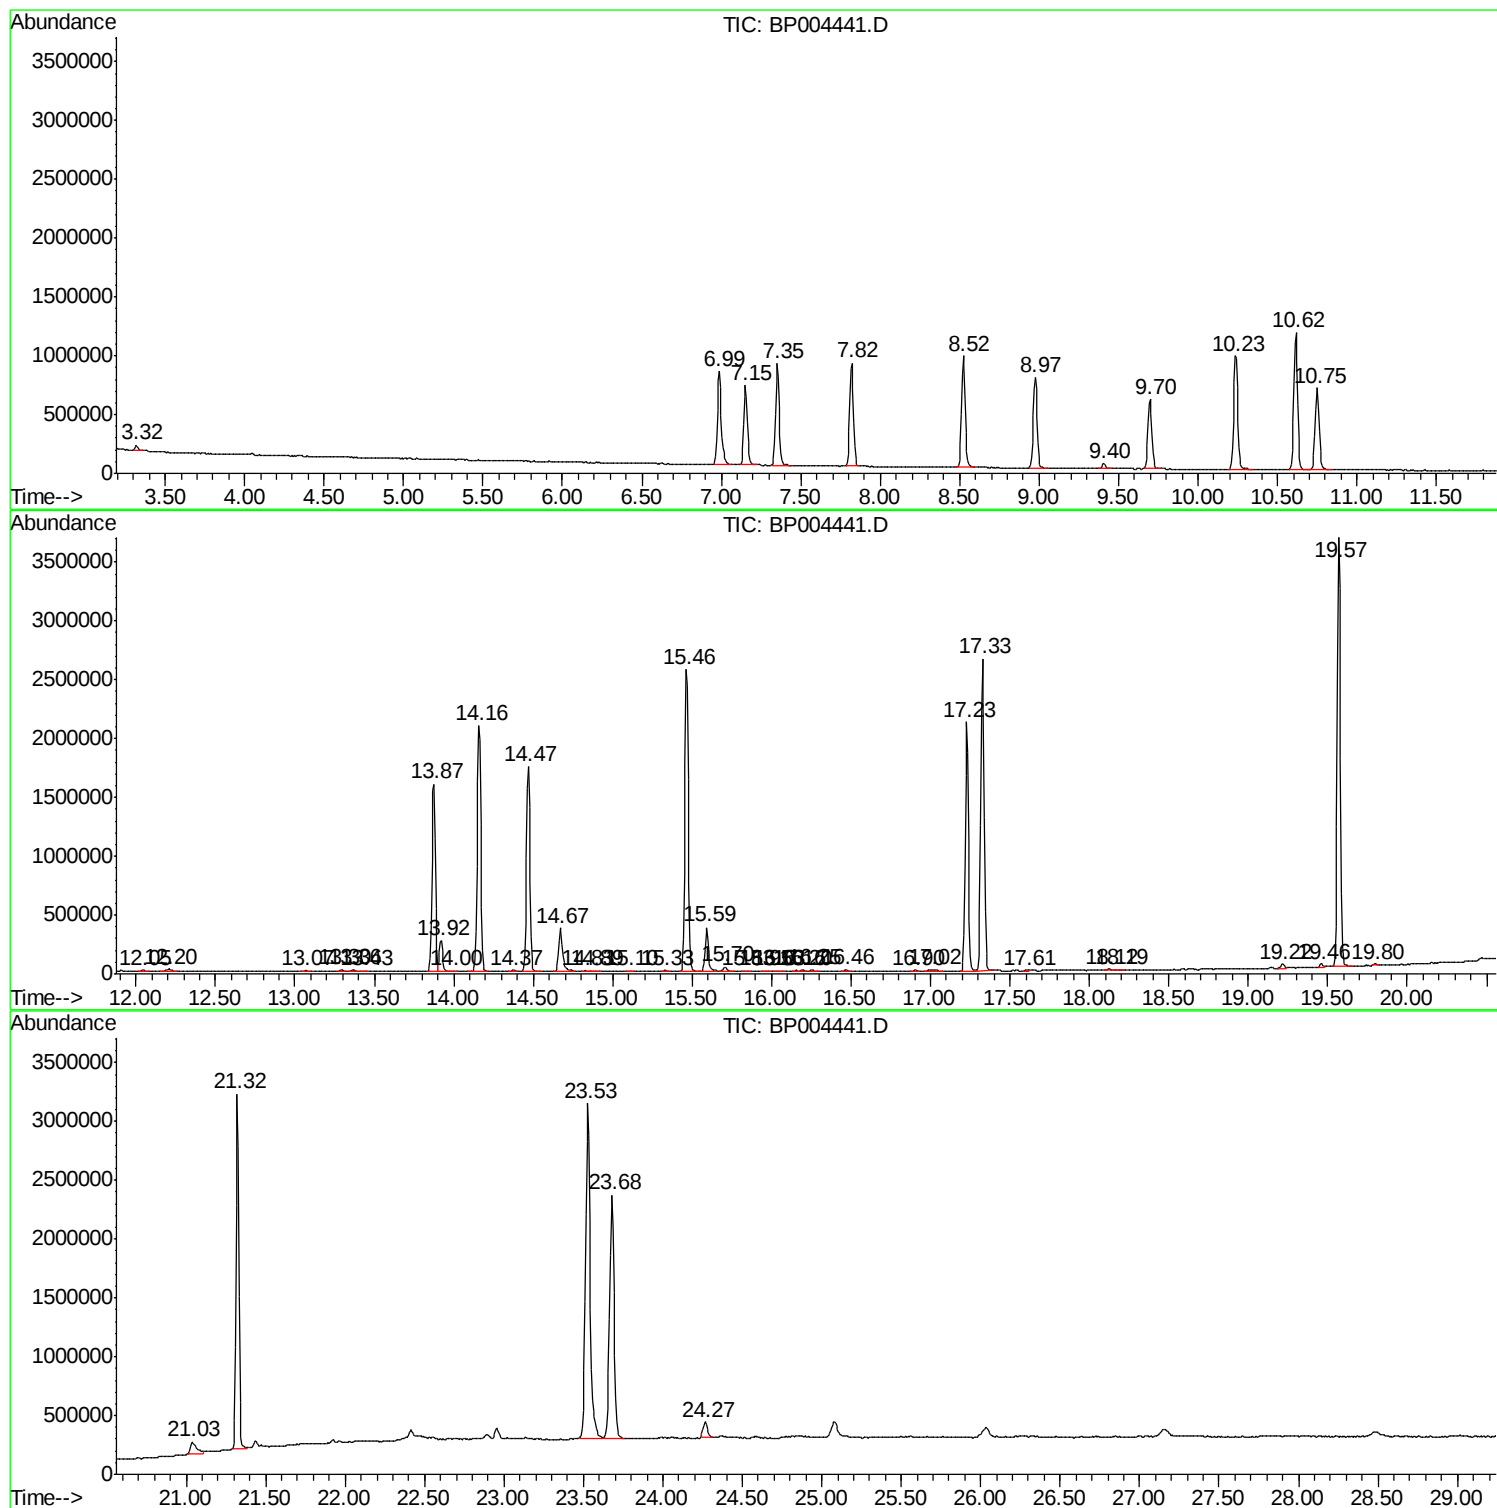

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004441.D
Acq On : 24 Dec 2020 20:00
Operator : CG/JU
Sample : L5132-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004441.D
Acq On : 24 Dec 2020 20:00
Operator : CG/JU
Sample : L5132-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc