

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
 Data File : BP004442.D
 Acq On : 24 Dec 2020 20:34
 Operator : CG/JU
 Sample : L5132-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54S3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	19	22	29	rVB	59031	86647	1.54%	0.148%
2	6.987	639	646	661	rBV2	995011	2196614	38.98%	3.764%
3	7.152	668	674	689	rVB	812431	1301271	23.09%	2.230%
4	7.352	701	708	717	rBV	1066809	1720933	30.54%	2.949%
5	7.822	781	788	796	rBV	883450	1437921	25.52%	2.464%
6	8.522	900	907	918	rBV	1191807	1937111	34.38%	3.319%
7	8.975	977	984	993	rBV	911775	1526506	27.09%	2.616%
8	9.140	1010	1012	1019	rVB4	10690	16339	0.29%	0.028%
9	9.410	1052	1058	1064	rVB	80577	133658	2.37%	0.229%
10	9.699	1100	1107	1120	rVB	720894	1240712	22.02%	2.126%
11	10.234	1191	1198	1211	rBV	1198545	2070789	36.75%	3.548%
12	10.616	1255	1263	1272	rBV	1145817	1925533	34.17%	3.300%
13	10.751	1278	1286	1299	rBV	1078799	1906049	33.83%	3.266%
14	11.628	1431	1435	1442	rBV5	6734	14727	0.26%	0.025%
15	11.787	1458	1462	1466	rBV5	5529	8411	0.15%	0.014%
16	11.822	1466	1468	1475	rVB3	8973	13123	0.23%	0.022%
17	11.904	1478	1482	1488	rVB4	8629	12242	0.22%	0.021%
18	12.046	1502	1506	1514	rVB4	10344	16530	0.29%	0.028%
19	12.204	1527	1533	1541	rVB	22260	42176	0.75%	0.072%
20	12.422	1564	1570	1575	rBV9	2938	6191	0.11%	0.011%
21	12.863	1642	1645	1652	rVB8	4028	7164	0.13%	0.012%
22	13.010	1666	1670	1676	rVB7	5792	10166	0.18%	0.017%
23	13.069	1676	1680	1685	rBV3	9280	14694	0.26%	0.025%
24	13.298	1714	1719	1725	rBV2	29929	57673	1.02%	0.099%
25	13.363	1725	1730	1738	rVV6	13665	30033	0.53%	0.051%
26	13.428	1738	1741	1749	rVB6	5893	9970	0.18%	0.017%
27	13.781	1796	1801	1805	rBV7	3350	6586	0.12%	0.011%
28	13.875	1810	1817	1821	rVV	1882180	2668927	47.37%	4.573%
29	13.916	1821	1824	1834	rVV	227507	340829	6.05%	0.584%
30	14.004	1834	1839	1846	rVB9	8799	16581	0.29%	0.028%
31	14.157	1853	1865	1876	rBV	2396925	3651903	64.81%	6.258%
32	14.375	1897	1902	1908	rVB3	14781	21620	0.38%	0.037%
33	14.469	1908	1918	1931	rBV	1618714	2434681	43.21%	4.172%
34	14.598	1935	1940	1946	rBV10	4013	7059	0.13%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
 Data File : BP004442.D
 Acq On : 24 Dec 2020 20:34
 Operator : CG/JU
 Sample : L5132-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54S3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	14.669	1946	1952	1969	rBV	624282	1022938	18.15%	1.753%
36	14.828	1976	1979	1983	rVB6	5183	7492	0.13%	0.013%
37	14.887	1983	1989	1995	rVB9	7299	17288	0.31%	0.030%
38	15.004	2002	2009	2015	rVB10	4908	11034	0.20%	0.019%
39	15.069	2015	2020	2022	rBV5	4085	6728	0.12%	0.012%
40	15.098	2022	2025	2031	rVB4	7625	12558	0.22%	0.022%
41	15.275	2050	2055	2061	rBV2	22868	40004	0.71%	0.069%
42	15.328	2061	2064	2069	rVB2	14199	18779	0.33%	0.032%
43	15.463	2080	2087	2096	rBV	2869779	4214504	74.79%	7.222%
44	15.592	2101	2109	2122	rBV	606316	884948	15.71%	1.516%
45	15.704	2124	2128	2143	rVV2	37263	75331	1.34%	0.129%
46	15.834	2145	2150	2155	rVB8	5063	8555	0.15%	0.015%
47	16.045	2181	2186	2189	rBV6	5497	10099	0.18%	0.017%
48	16.104	2194	2196	2200	rVV5	9261	12529	0.22%	0.021%
49	16.151	2200	2204	2208	rVV3	24979	40235	0.71%	0.069%
50	16.198	2208	2212	2215	rVV4	14680	25242	0.45%	0.043%
51	16.257	2218	2222	2227	rVB3	24205	37287	0.66%	0.064%
52	16.369	2236	2241	2245	rBV3	11272	17041	0.30%	0.029%
53	16.463	2253	2257	2262	rVB	26220	34138	0.61%	0.058%
54	16.545	2262	2271	2273	rBV9	4206	10149	0.18%	0.017%
55	16.622	2278	2284	2288	rBV5	6314	12069	0.21%	0.021%
56	16.710	2293	2299	2301	rBV7	7196	13666	0.24%	0.023%
57	16.904	2327	2332	2337	rBV5	5860	9333	0.17%	0.016%
58	16.969	2337	2343	2346	rBV4	18801	32789	0.58%	0.056%
59	17.145	2371	2373	2378	rVB6	4504	6910	0.12%	0.012%
60	17.228	2380	2387	2396	rBV	1922204	2668469	47.36%	4.573%
61	17.328	2397	2404	2417	rVV	3035088	4375753	77.66%	7.498%
62	17.422	2417	2420	2426	rVV8	3467	5846	0.10%	0.010%
63	17.533	2434	2439	2441	rBV3	5608	8992	0.16%	0.015%
64	17.598	2448	2450	2455	rVB6	3640	6039	0.11%	0.010%
65	17.881	2494	2498	2499	rBV3	4057	5838	0.10%	0.010%
66	18.116	2534	2538	2544	rBV6	23032	42250	0.75%	0.072%
67	18.410	2584	2588	2591	rBV5	6236	8886	0.16%	0.015%
68	18.604	2618	2621	2625	rVB	11031	14898	0.26%	0.026%
69	18.863	2660	2665	2670	rBV	110987	144754	2.57%	0.248%
70	19.216	2721	2725	2729	rBV	34738	46630	0.83%	0.080%
71	19.251	2729	2731	2738	rVB6	12489	16972	0.30%	0.029%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
Data File : BP004442.D
Acq On : 24 Dec 2020 20:34
Operator : CG/JU
Sample : L5132-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Title : SVOA CALIBRATION

72	19.463	2763	2767	2775	rBV	30765	48124	0.85%	0.082%
73	19.569	2779	2785	2792	rBV	3935221	5200944	92.30%	8.912%
74	21.039	3031	3035	3047	rBV3	81704	227064	4.03%	0.389%
75	21.322	3078	3083	3093	rBV	2475016	3096452	54.95%	5.306%
76	21.433	3099	3102	3107	rBV	46245	74377	1.32%	0.127%
77	23.527	3450	3458	3475	rBV	2839803	5634790	100.00%	9.656%
78	23.680	3476	3484	3494	rVB2	1537261	3257912	57.82%	5.583%


Sum of corrected areas: 58358005

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
Data File : BP004442.D
Acq On : 24 Dec 2020 20:34
Operator : CG/JU
Sample : L5132-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

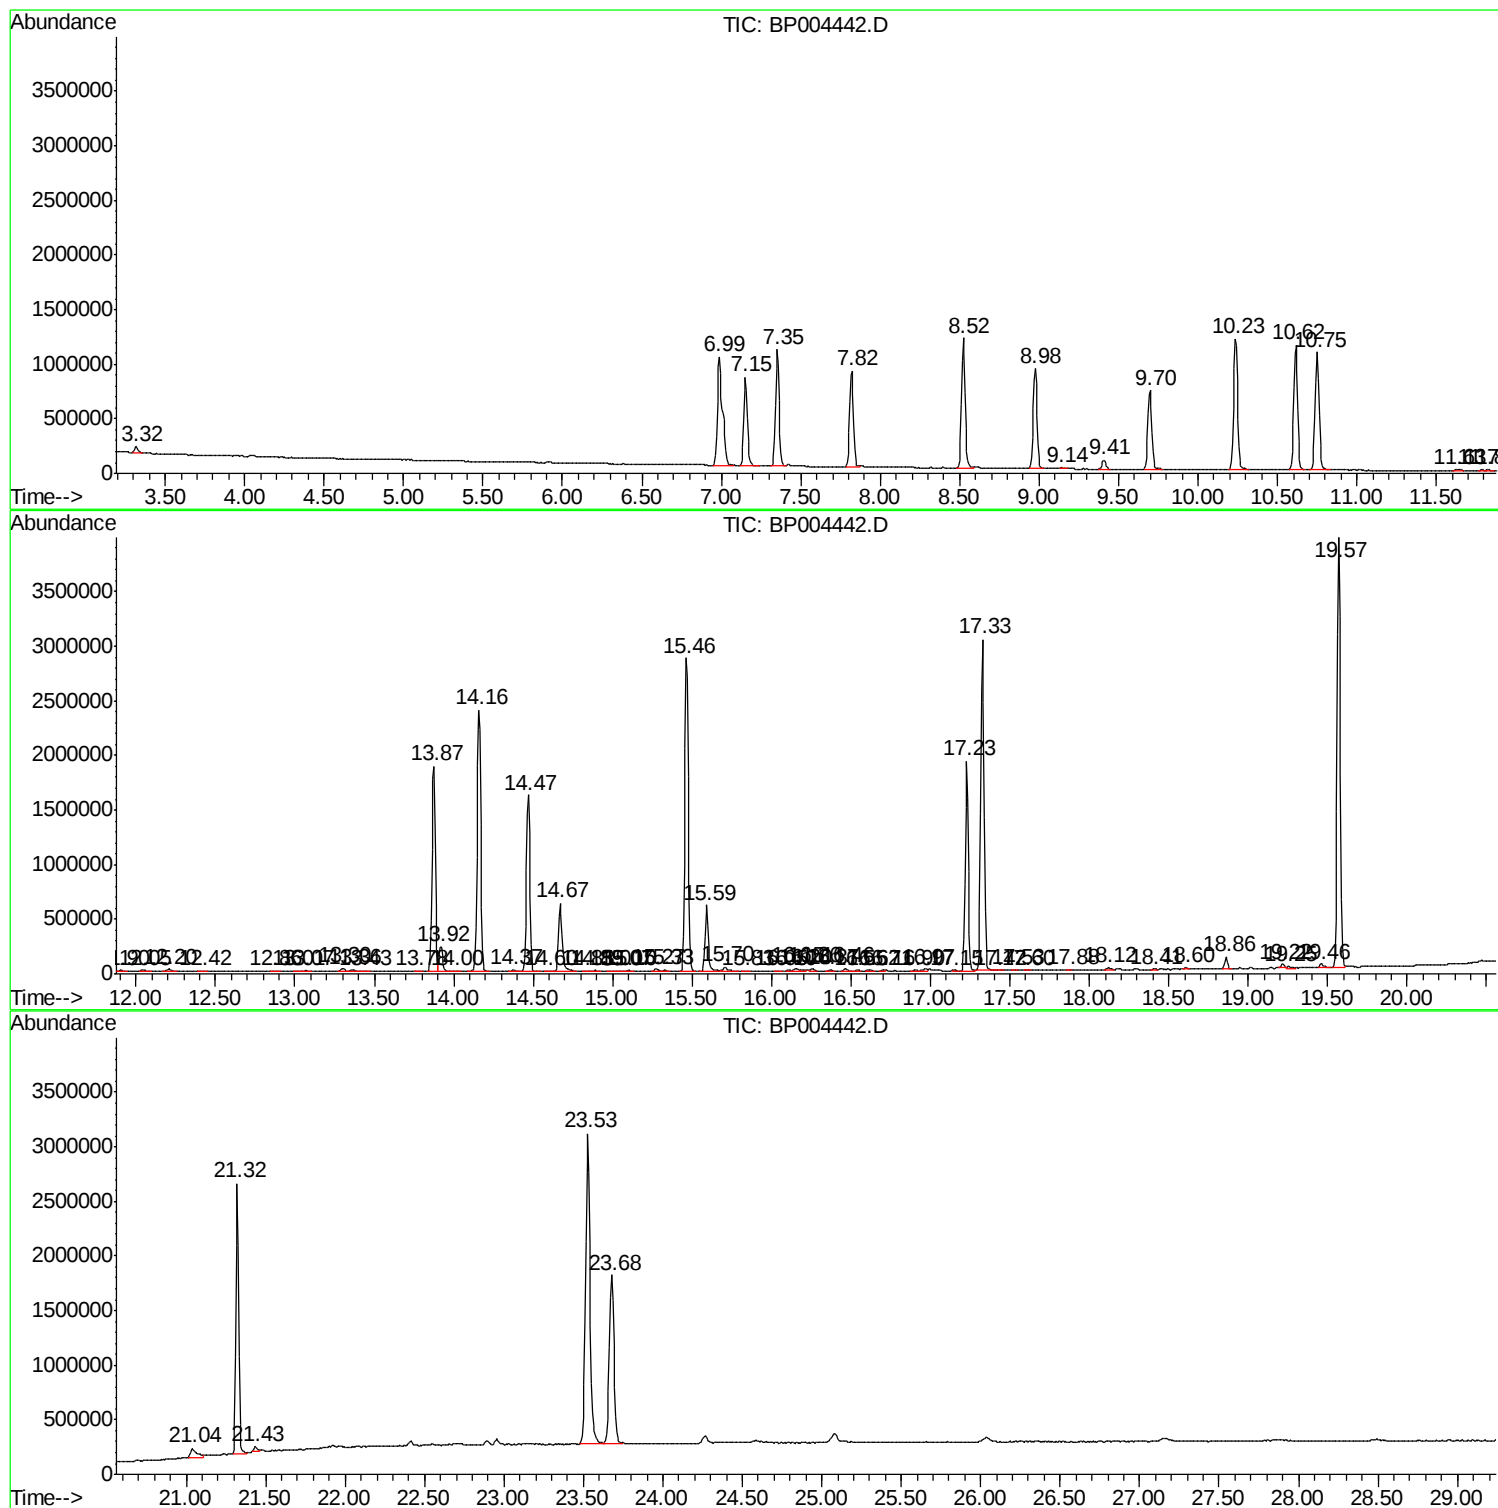

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004442.D
Acq On : 24 Dec 2020 20:34
Operator : CG/JU
Sample : L5132-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004442.D
Acq On : 24 Dec 2020 20:34
Operator : CG/JU
Sample : L5132-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc