

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
 Data File : BP004443.D
 Acq On : 24 Dec 2020 21:08
 Operator : CG/JU
 Sample : L5132-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54S5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.987	640	646	658	rVB	721753	1210370	25.96%	2.661%
2	7.152	668	674	687	rVB	684207	1096782	23.53%	2.411%
3	7.351	702	708	722	rVB	821683	1320199	28.32%	2.902%
4	7.822	781	788	796	rBV	810835	1326287	28.45%	2.916%
5	8.522	900	907	918	rBV	894700	1451144	31.13%	3.190%
6	8.975	977	984	994	rBV	771107	1283878	27.54%	2.823%
7	9.404	1053	1057	1064	rVB2	32918	52499	1.13%	0.115%
8	9.698	1100	1107	1120	rBV	467004	817715	17.54%	1.798%
9	10.234	1191	1198	1217	rBV	873163	1533810	32.90%	3.372%
10	10.616	1254	1263	1275	rBV	1037580	1784206	38.27%	3.922%
11	10.751	1279	1286	1296	rVV	504244	882086	18.92%	1.939%
12	12.204	1528	1533	1540	rBV2	16533	30764	0.66%	0.068%
13	13.069	1675	1680	1687	rVB6	5930	10583	0.23%	0.023%
14	13.298	1714	1719	1723	rBV3	8194	13422	0.29%	0.030%
15	13.363	1723	1730	1735	rVV8	6945	13126	0.28%	0.029%
16	13.434	1737	1742	1748	rVB5	3937	7633	0.16%	0.017%
17	13.875	1810	1817	1821	rBV	1064835	1530174	32.82%	3.364%
18	13.922	1821	1825	1830	rVB	103666	152554	3.27%	0.335%
19	13.998	1835	1838	1842	rVB4	3324	4976	0.11%	0.011%
20	14.157	1855	1865	1881	rBV	2081267	3084900	66.17%	6.782%
21	14.375	1897	1902	1906	rVB3	7431	10034	0.22%	0.022%
22	14.469	1910	1918	1930	rBV	1503106	2235184	47.94%	4.914%
23	14.675	1946	1953	1968	rBV	181076	341466	7.32%	0.751%
24	14.886	1983	1989	1995	rVB10	4513	8696	0.19%	0.019%
25	15.104	2021	2026	2032	rVB9	3250	6432	0.14%	0.014%
26	15.328	2060	2064	2069	rVB4	7389	9594	0.21%	0.021%
27	15.463	2080	2087	2099	rBV	2444907	3560291	76.37%	7.827%
28	15.592	2103	2109	2120	rVV	197963	294128	6.31%	0.647%
29	15.710	2123	2129	2139	rVB2	27477	48326	1.04%	0.106%
30	16.033	2178	2184	2190	rBV10	4415	8890	0.19%	0.020%
31	16.151	2199	2204	2208	rBV6	3497	5456	0.12%	0.012%
32	16.192	2209	2211	2214	rVV3	5242	5572	0.12%	0.012%
33	16.251	2217	2221	2229	rVB4	11065	18441	0.40%	0.041%
34	16.463	2254	2257	2261	rBV2	8483	10748	0.23%	0.024%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
 Data File : BP004443.D
 Acq On : 24 Dec 2020 21:08
 Operator : CG/JU
 Sample : L5132-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54S5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	16.904	2329	2332	2336	rVB5	4500	5586	0.12%	0.012%
36	17.016	2340	2351	2356	rBV5	8442	27455	0.59%	0.060%
37	17.227	2380	2387	2397	rBV	1782217	2453420	52.62%	5.394%
38	17.327	2397	2404	2414	rVV	2568721	3662467	78.56%	8.052%
39	18.122	2536	2539	2545	rBV8	4207	6995	0.15%	0.015%
40	18.186	2545	2550	2554	rBV7	4905	8292	0.18%	0.018%
41	19.216	2721	2725	2735	rBV	27673	40804	0.88%	0.090%
42	19.463	2762	2767	2771	rBV	26221	39040	0.84%	0.086%
43	19.569	2779	2785	2795	rBV	3296089	4357275	93.46%	9.579%
44	21.039	3031	3035	3047	rBV3	94631	247139	5.30%	0.543%
45	21.321	3078	3083	3094	rBV	2166439	2847209	61.07%	6.259%
46	23.527	3451	3458	3472	rVB	2297406	4662160	100.00%	10.250%
47	23.680	3477	3484	3493	rVB2	1488810	2958358	63.45%	6.504%


Sum of corrected areas: 45486566

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122420\
Data File : BP004443.D
Acq On : 24 Dec 2020 21:08
Operator : CG/JU
Sample : L5132-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

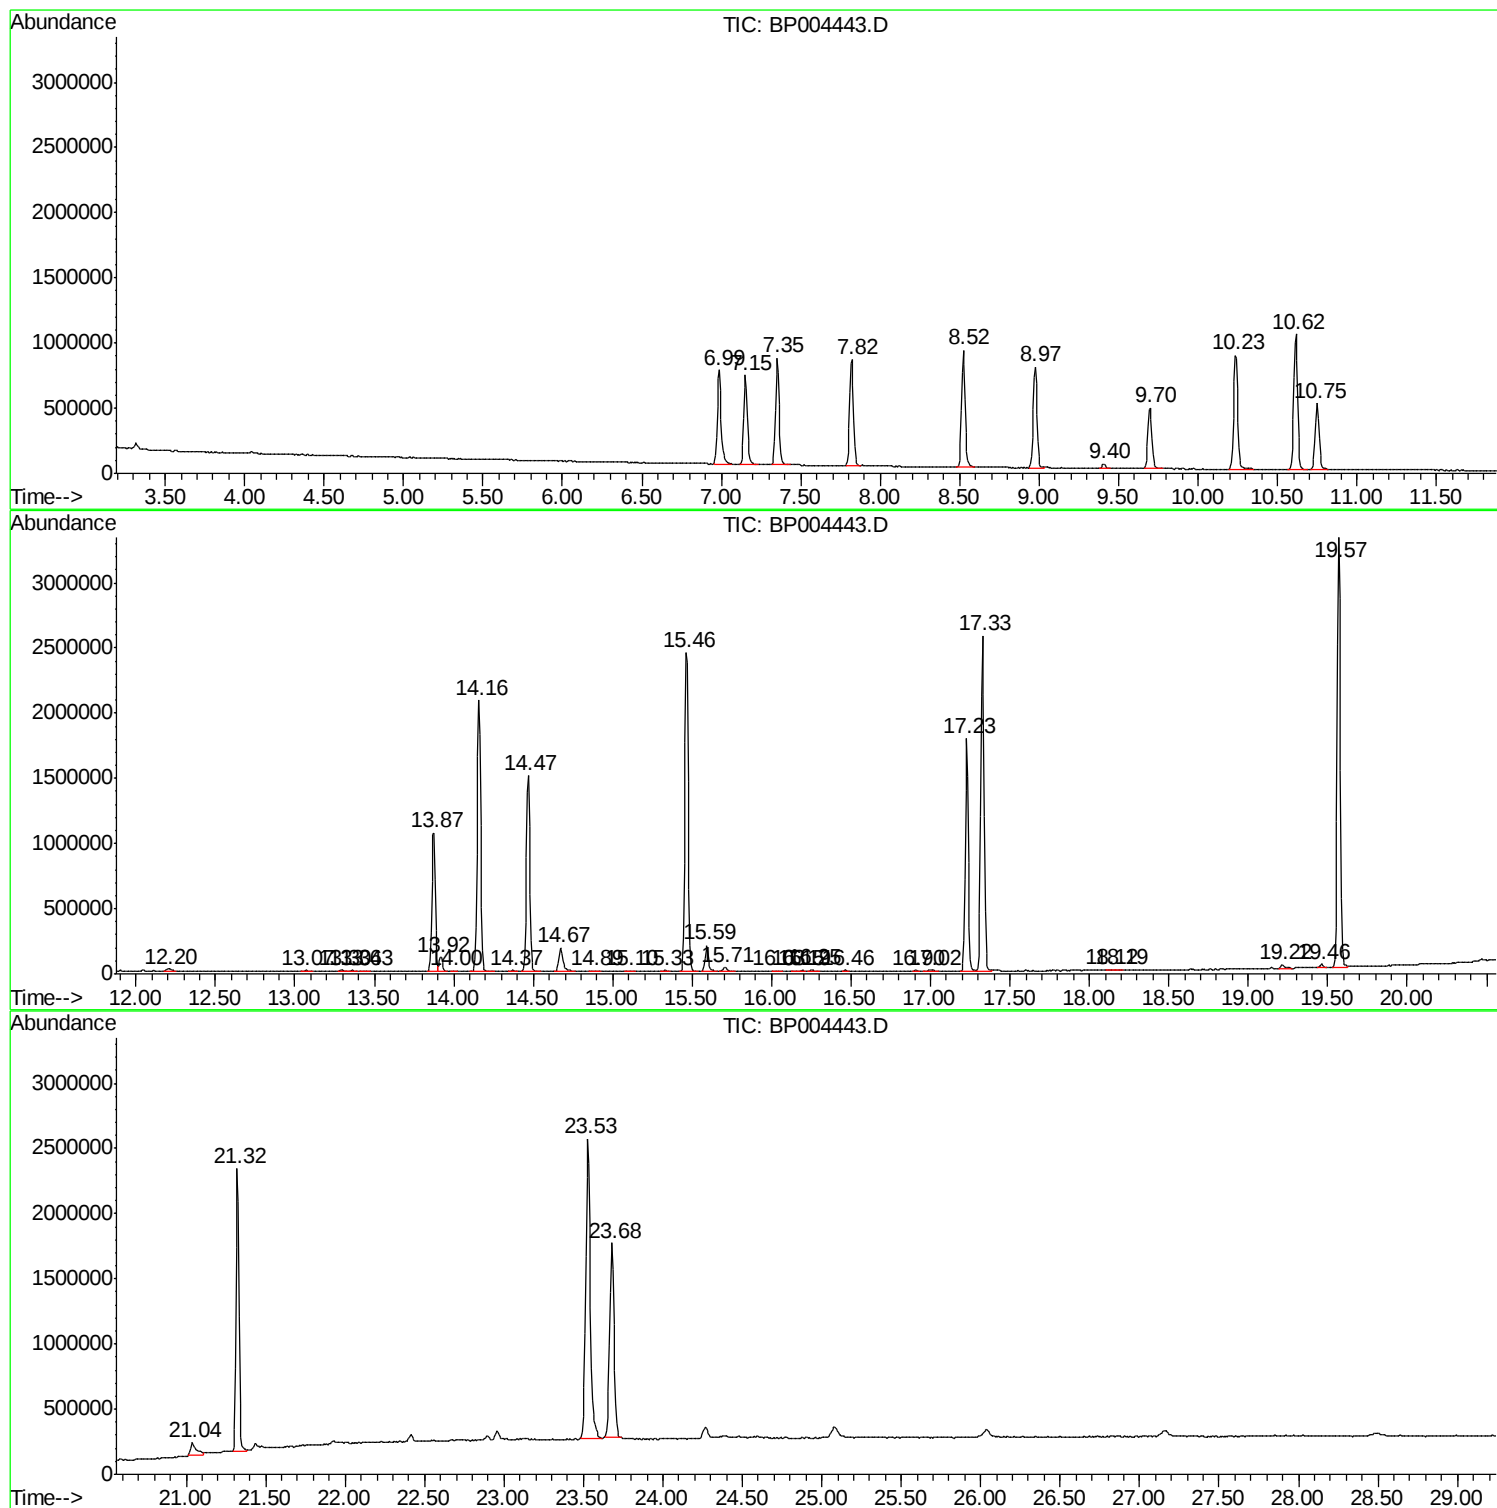

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004443.D
Acq On : 24 Dec 2020 21:08
Operator : CG/JU
Sample : L5132-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122420\
Data File : BP004443.D
Acq On : 24 Dec 2020 21:08
Operator : CG/JU
Sample : L5132-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54S5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc