

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122619\
 Data File : BP001440.D
 Acq On : 27 Dec 2019 02:55
 Operator : JU
 Sample : PB125736TB
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 27 10:33:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 16:04:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	25482	20.00	ng	0.00
21) Naphthalene-d8	10.32	136	88498	20.00	ng	0.00
39) Acenaphthene-d10	13.18	164	55944	20.00	ng	0.00
64) Phenanthrene-d10	15.58	188	113090	20.00	ng	0.00
76) Chrysene-d12	19.22	240	90018	20.00	ng	-0.01
87) Perylene-d12	20.99	264	93565	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.21	112	212023	134.48	ng	0.01
7) Phenol-d6	7.76	99	270753	131.60	ng	0.00
23) Nitrobenzene-d5	9.17	82	196909	85.44	ng	0.00
42) 2,4,6-Tribromophenol	14.48	330	102251	146.19	ng	0.00
45) 2-Fluorobiphenyl	12.10	172	427376	96.60	ng	0.00
79) Terphenyl-d14	17.86	244	566675	107.82	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.53	79	4762	2.467	ng	# 61
19) n-Nitroso-di-n-propylamine	9.17	70	30466	20.860	ng	# 78
32) Benzoic acid	10.01	122	22	5.043	ng	# 51
77) Benzidine	17.52	184	48443	18.483	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122619\
Data File : BP001440.D
Acq On : 27 Dec 2019 02:55
Operator : JU
Sample : PB125736TB
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 27 10:33:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration




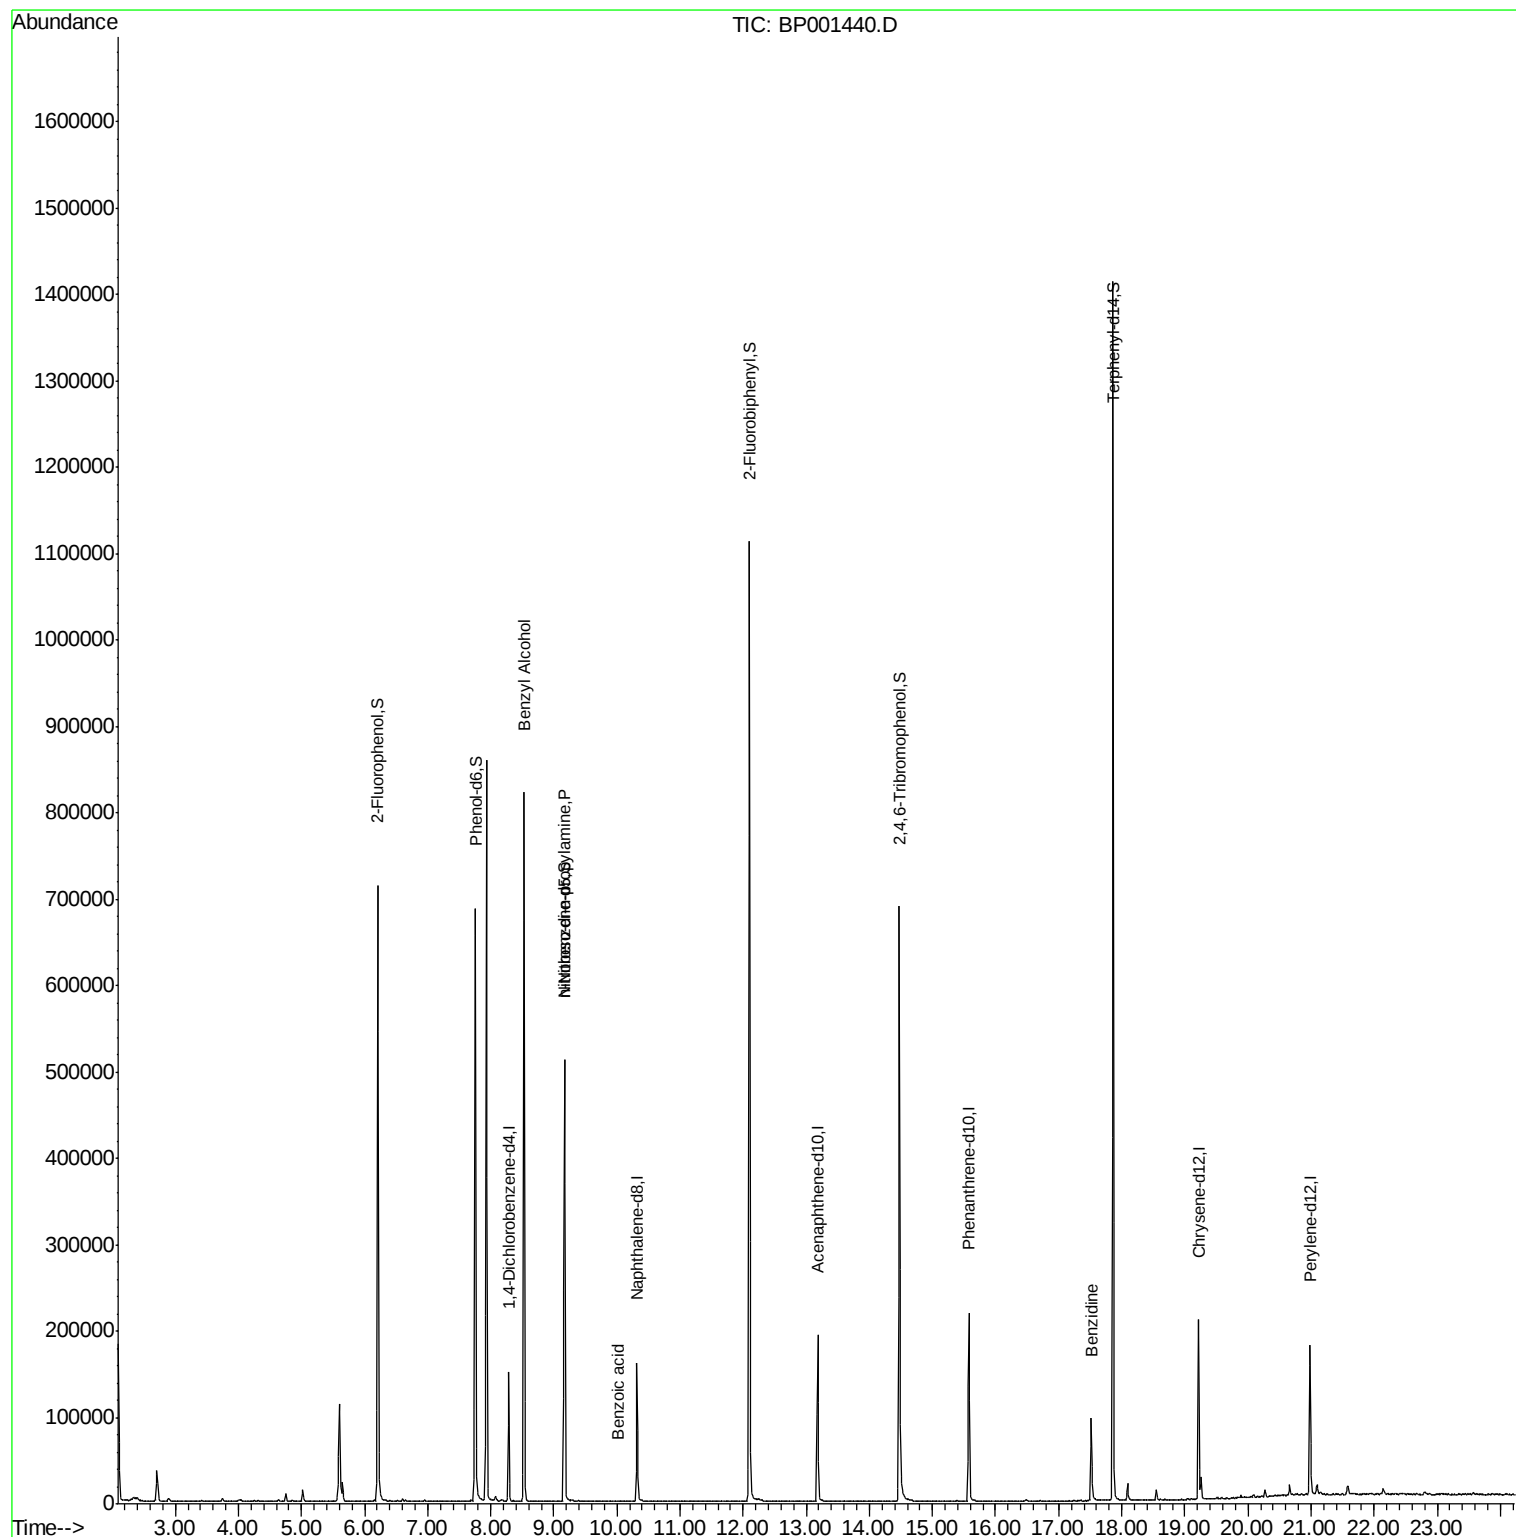




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.28 min Scan# 1053
 Delta R.T. -0.01 min
 Lab File: BP001440.D
 Acq: 27 Dec 2019 02:55




Instrument :
 BNA_P
 ClientSampleId :


Tot Ion:	152	Resp:	25482
Ion	Ratio	Lower	Upper
152	100		
150	151.5	127.0	190.6
115	66.1	56.1	84.1

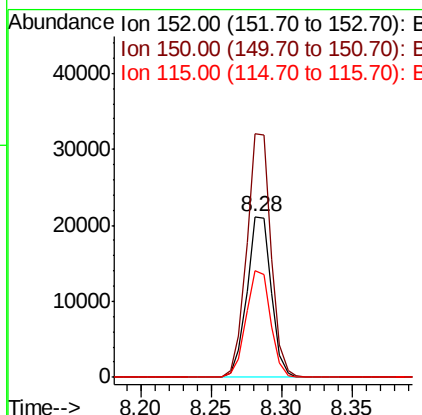

#5
 2-Fluorophenol
 Concen: 134.475 ng
 RT: 6.21 min Scan# 701
 Delta R.T. 0.01 min
 Lab File: BP001440.D
 Acq: 27 Dec 2019 02:55

Tgt Ion:	112	Resp:	212023
Ion	Ratio	Lower	Upper
112	100		
64	63.1	53.9	80.9
63	41.4	33.4	50.0

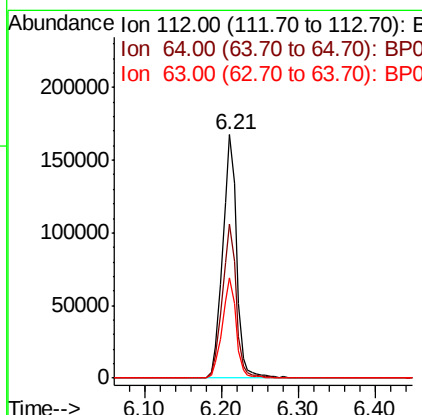

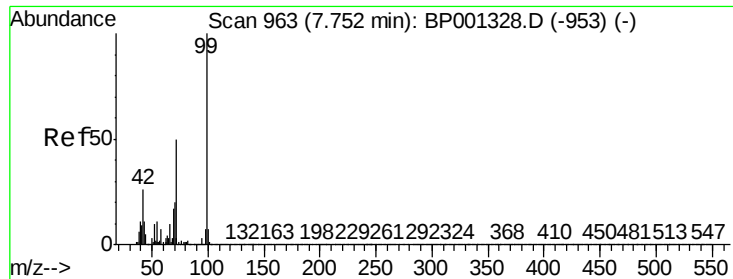

#7

Phenol-d6

Concen: 131.603 ng

RT: 7.76 min Scan# 964

Delta R.T. 0.01 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55

Instrument :

BNA_P

ClientSampleId :





Tot Ion: 99 Resp: 270753

Ion Ratio Lower Upper

99 100

42 24.9 20.8 31.2

71 47.0 38.2 57.4

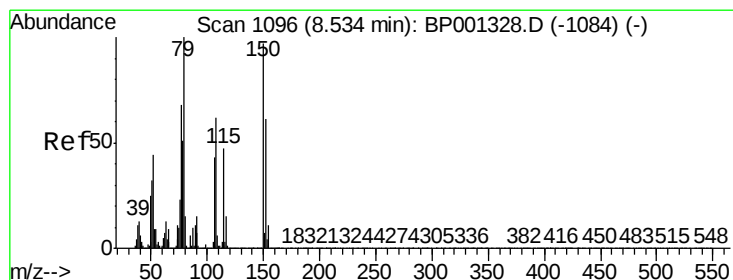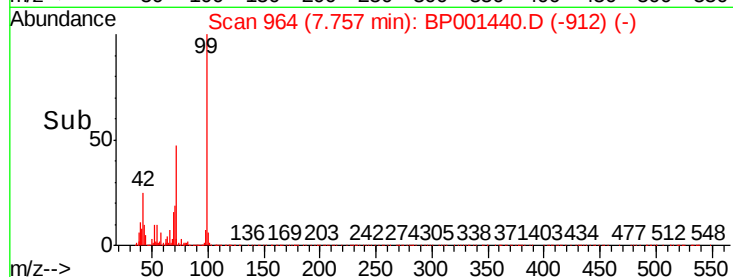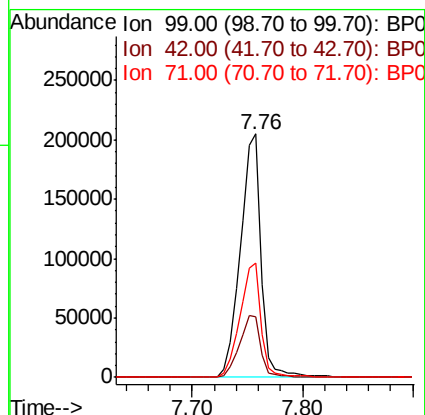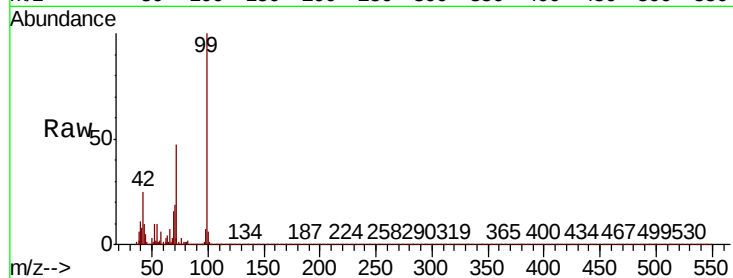

#15

Benzyl Alcohol

Concen: 2.467 ng

RT: 8.53 min Scan# 1095

Delta R.T. 0.01 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55




Tgt Ion: 79 Resp: 4762


Ion Ratio Lower Upper

79 100

108 51.9 49.0 73.4

77 122.6 56.7 85.1#


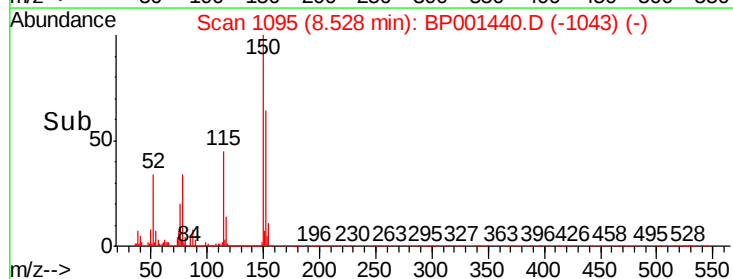
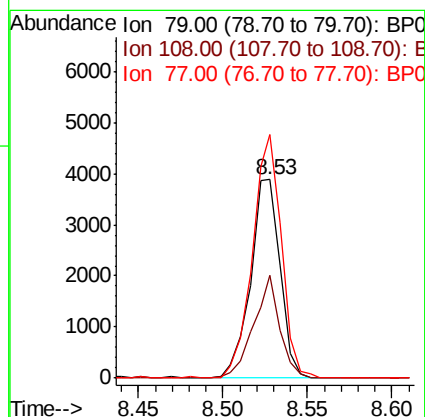
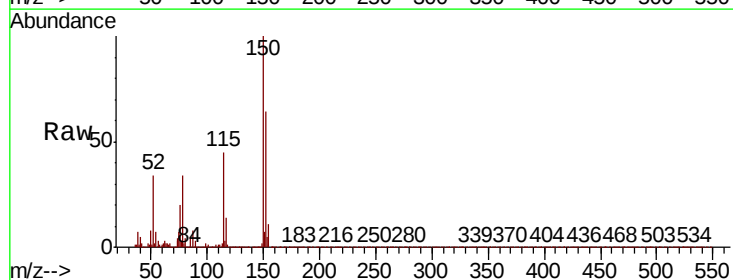


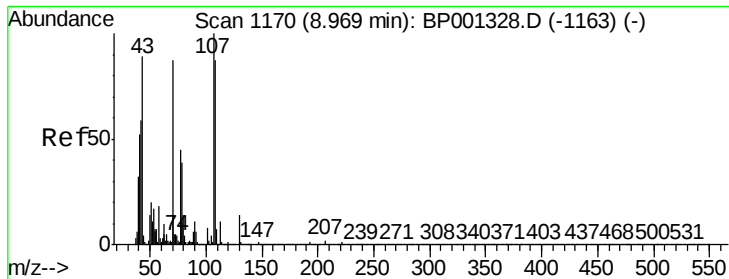

#19
n-Nitroso-di-n-propylamine
Concen: 20.860 ng
RT: 9.17 min Scan# 1204
Delta R.T. 0.21 min
Lab File: BP001440.D
Acq: 27 Dec 2019 02:55




Instrument :
BNA_P
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
70	100		
42	56.4	55.8	83.8
101	0.0	8.2	12.2#
130	1.0	14.5	21.7#

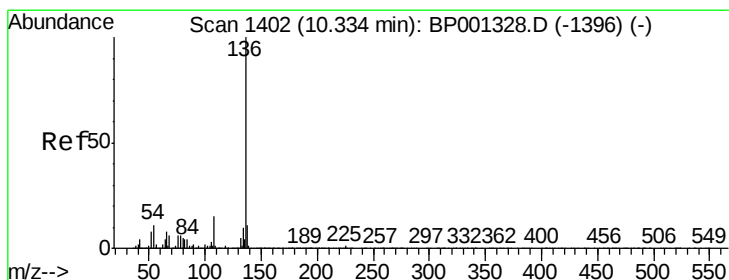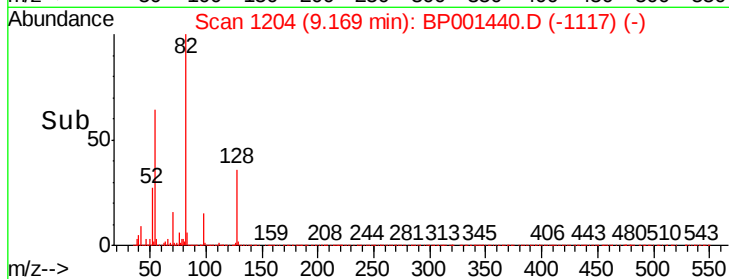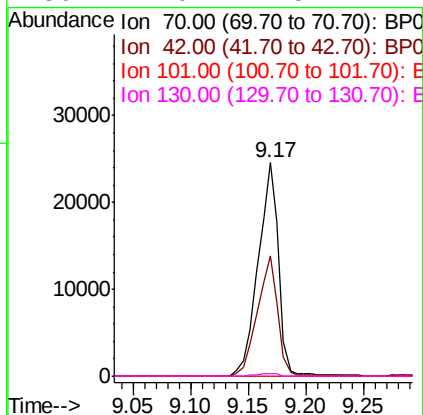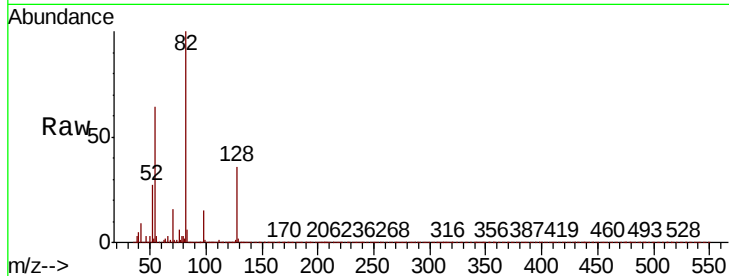

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.32 min Scan# 1399
Delta R.T. -0.01 min
Lab File: BP001440.D
Acq: 27 Dec 2019 02:55

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.8	9.0	13.4
54	10.0	7.3	10.9
68	4.9	3.8	5.6

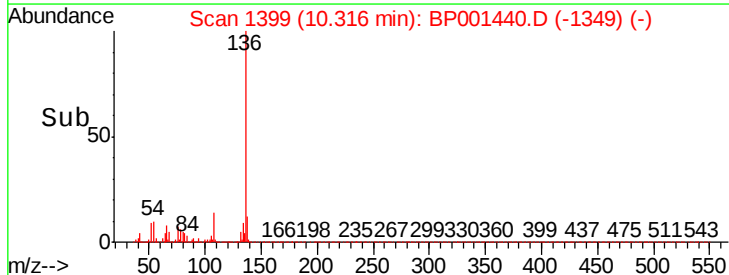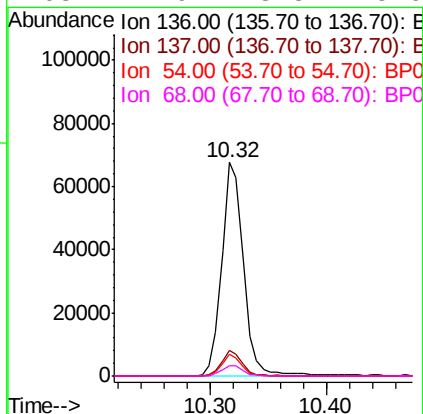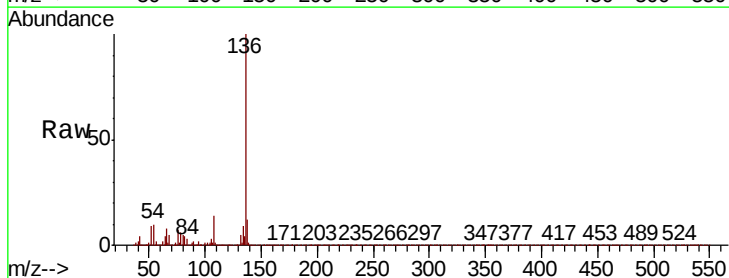

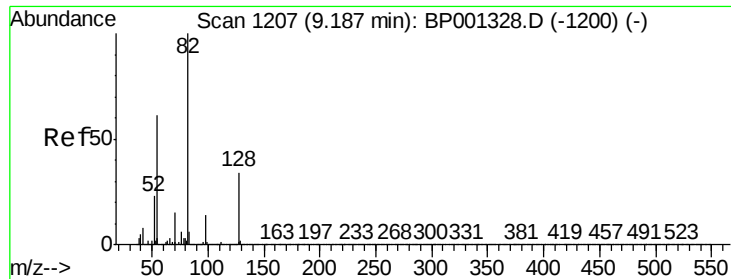

#23

Nitrobenzene-d5

Concen: 85.443 ng

RT: 9.17 min Scan# 1204

Delta R.T. -0.01 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55

Instrument :

BNA_P

ClientSampleId :


Tot Ion: 82 Resp: 196909

Ion Ratio Lower Upper

82 100

128 36.3 27.4 41.0




54 64.1 47.5 71.3



Abundance Ion 82.00 (81.70 to 82.70): BP0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BP0

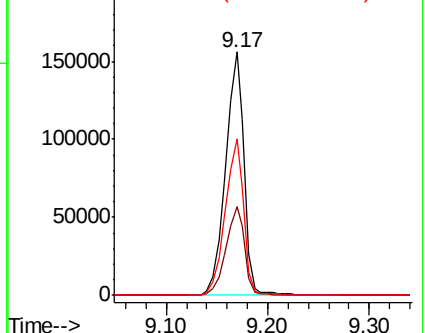

#32

Benzoic acid

Concen: 5.043 ng

RT: 10.01 min Scan# 1347

Delta R.T. 0.01 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55


Tgt Ion:122 Resp: 22

Ion Ratio Lower Upper

122 100

105 34.8 117.8 157.8#



77 104.3 85.6 125.6




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BP0

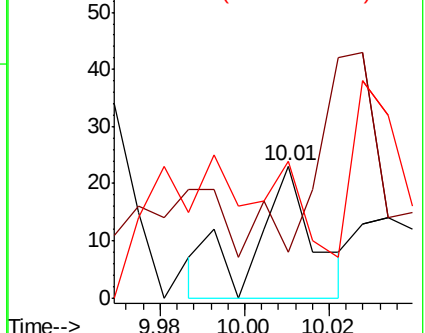

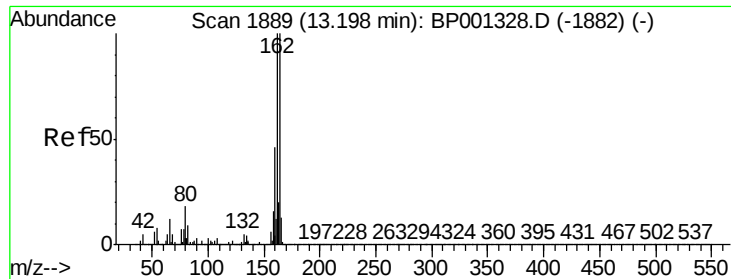

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 13.18 min Scan# 1886

Delta R.T. -0.00 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55

Instrument :

BNA_P

ClientSampleId :


Tot Ion:164 Resp: 55944

Ion Ratio Lower Upper

164 100

162 101.7 78.2 117.4




160 44.4 35.1 52.7



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

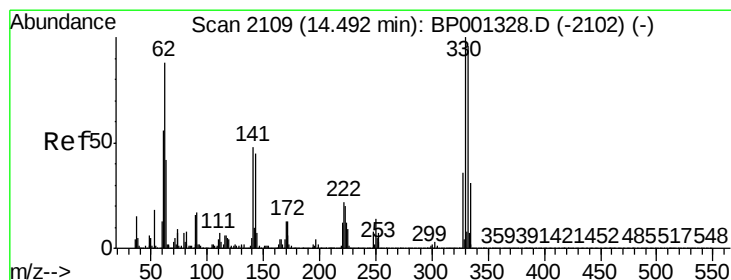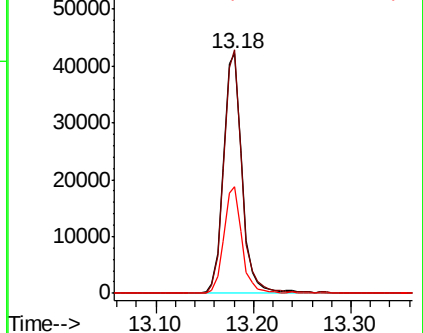

#42

2,4,6-Tribromophenol

Concen: 146.192 ng

RT: 14.48 min Scan# 2107

Delta R.T. -0.00 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55


Tgt Ion:330 Resp: 102251

Ion Ratio Lower Upper

330 100

332 96.2 78.3 117.5



141 40.0 26.8 40.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

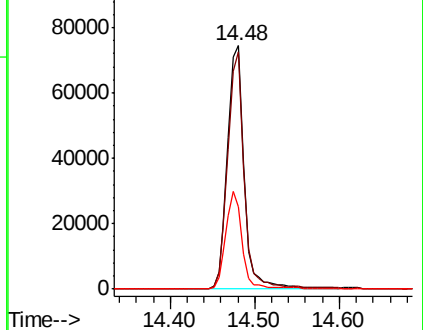



#45

2-Fluorobiphenyl

Concen: 96.599 ng

RT: 12.10 min Scan# 1702

Delta R.T. -0.00 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55


Instrument :

BNA_P

ClientSampleId :

Tot Ion:172 Resp: 427376

Ion	Ratio	Lower	Upper
172	100		
171	35.3	27.4	41.0
170	23.7	18.2	27.4






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

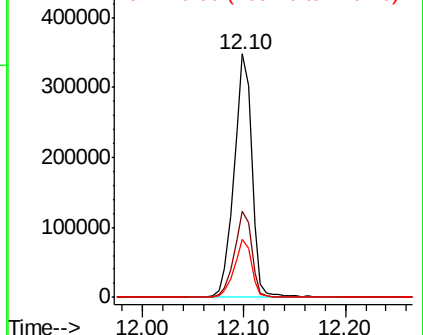

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.58 min Scan# 2294


Delta R.T. -0.00 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55

Tgt Ion:188 Resp: 113090

Ion	Ratio	Lower	Upper
188	100		
94	6.6	5.8	8.8
80	6.8	5.7	8.5






Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0



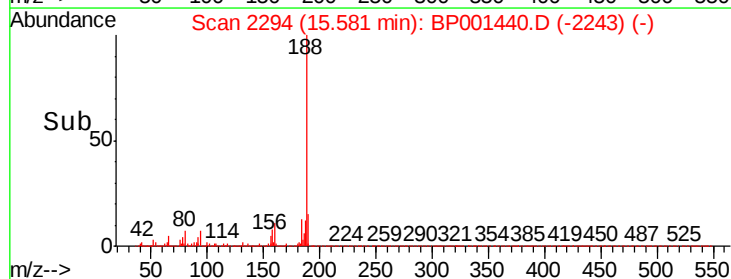
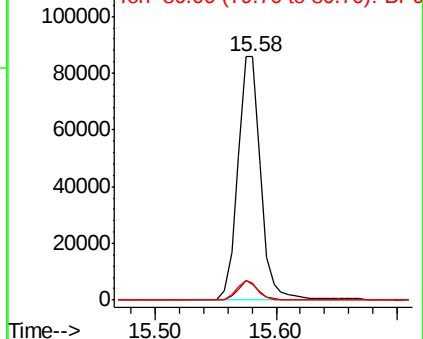


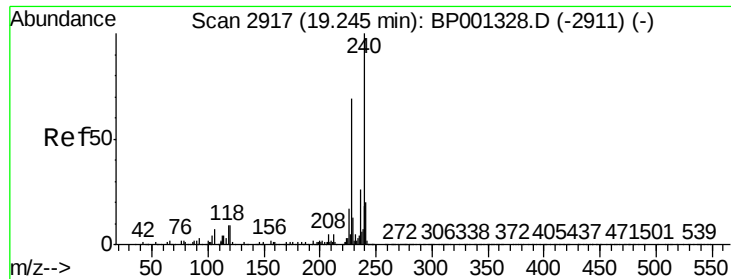

#76
Chrysene-d12
Concen: 20.000 ng
RT: 19.22 min Scan# 2912
Delta R.T. -0.01 min
Lab File: BP001440.D
Acq: 27 Dec 2019 02:55




Instrument :
BNA_P
ClientSampleId :


Tot Ion:240 Resp: 90018
Ion Ratio Lower Upper
240 100
120 7.9 6.2 9.2
236 25.6 20.2 30.2

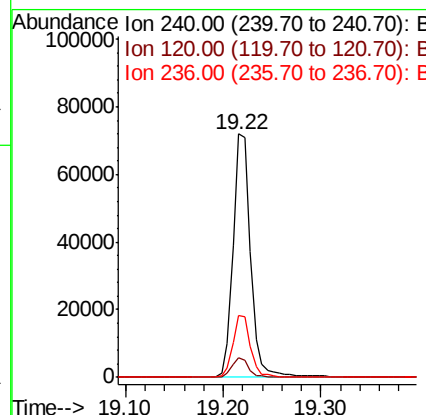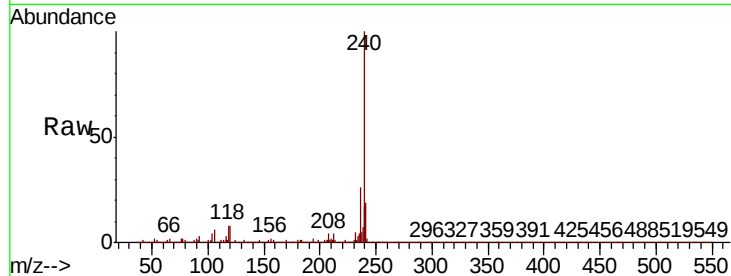

#77
Benzidine
Concen: 18.483 ng
RT: 17.52 min Scan# 2623
Delta R.T. -0.00 min
Lab File: BP001440.D
Acq: 27 Dec 2019 02:55

Tgt Ion:184 Resp: 48443
Ion Ratio Lower Upper
184 100
185 14.4 11.8 17.8
183 11.2 9.6 14.4

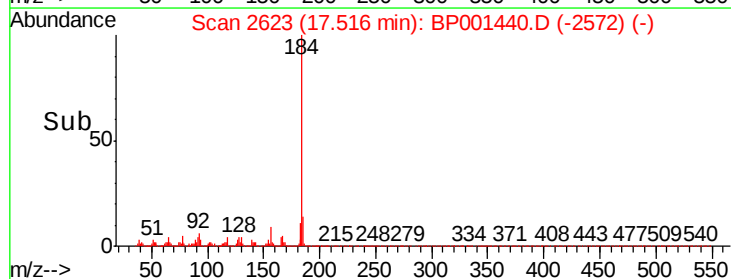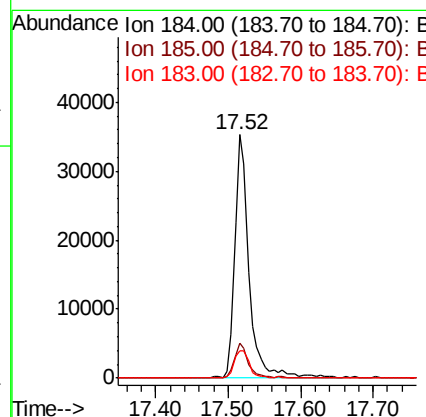



#79

Terphenyl-d14

Concen: 107.821 ng

RT: 17.86 min Scan# 2682

Delta R.T. -0.01 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55

Instrument :

BNA_P

ClientSampleId :


Tot Ion:244 Resp: 566675

Ion Ratio Lower Upper




244 100

212 7.3 5.8 8.8

122 10.0 6.4 9.6#



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

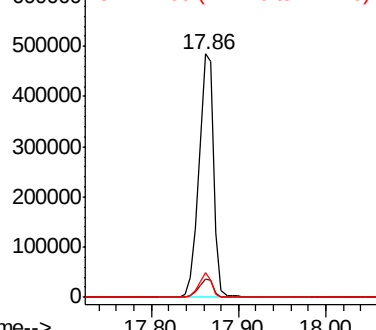

#87

Perylene-d12

Concen: 20.000 ng

RT: 20.99 min Scan# 3213

Delta R.T. -0.01 min

Lab File: BP001440.D

Acq: 27 Dec 2019 02:55


Tgt Ion:264 Resp: 93565

Ion Ratio Lower Upper

264 100

260 23.3 19.0 28.4

265 22.2 17.0 25.4



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

