
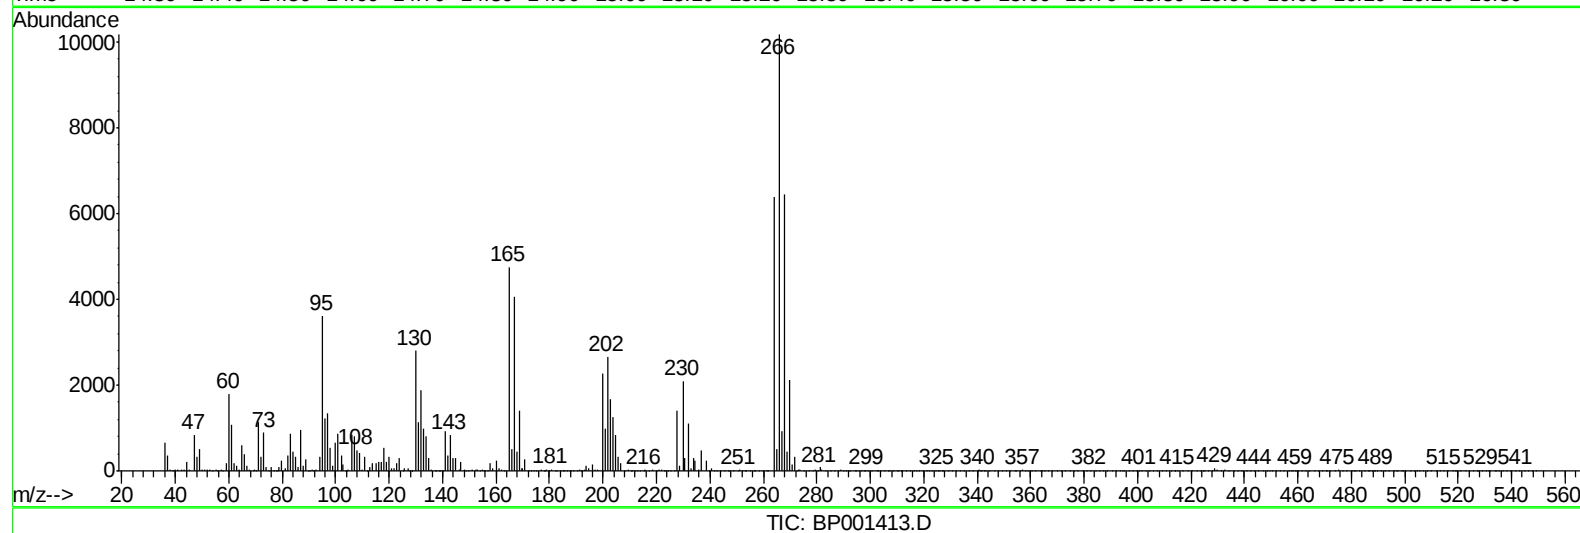


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122619\
Data File : BP001413.D
Acq On : 26 Dec 2019 10:09
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 07:17:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

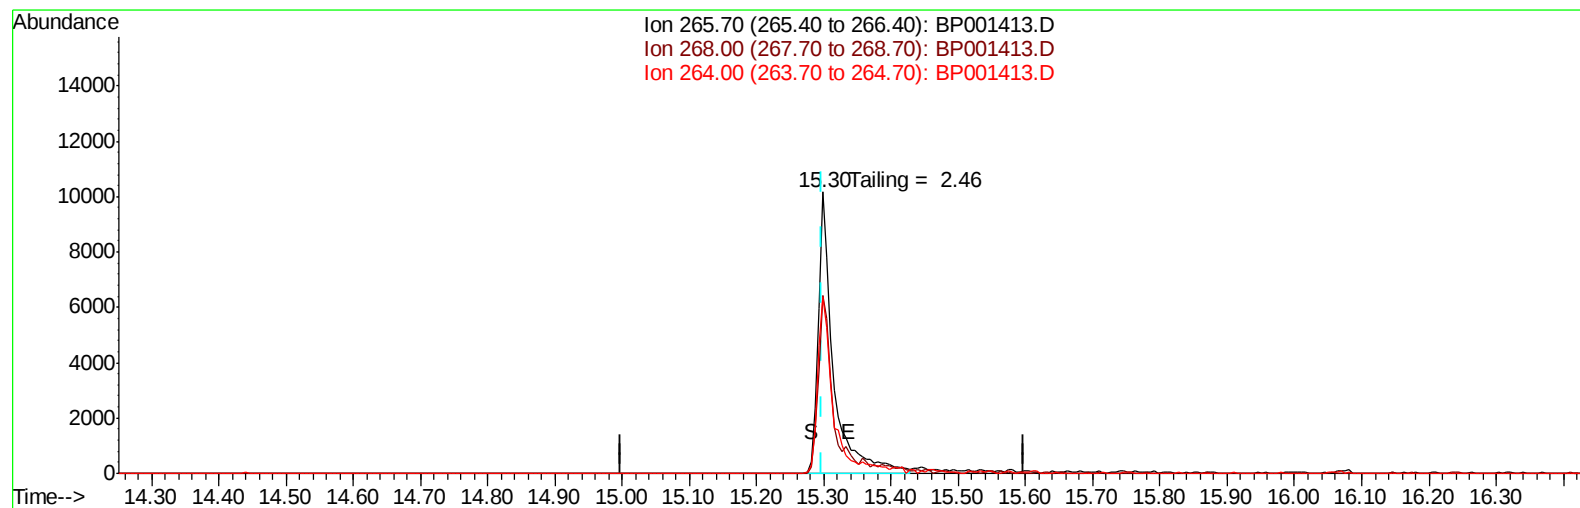

(70) Pentachlorophenol (C)



15.298min (-0.000) 50417.06ng

response 16356

Ion	Exp%	Act%
265.70	100	100
268.00	71.20	67.79
264.00	63.50	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122619\
Data File : BP001413.D
Acq On : 26 Dec 2019 10:09
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 07:17:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

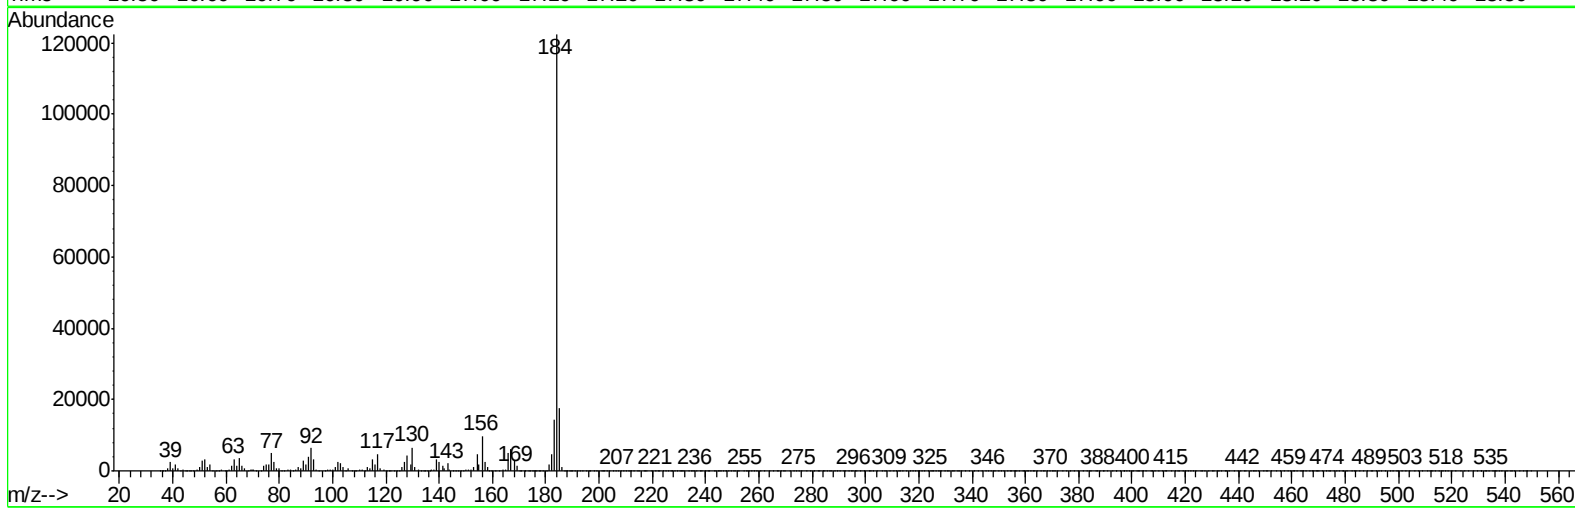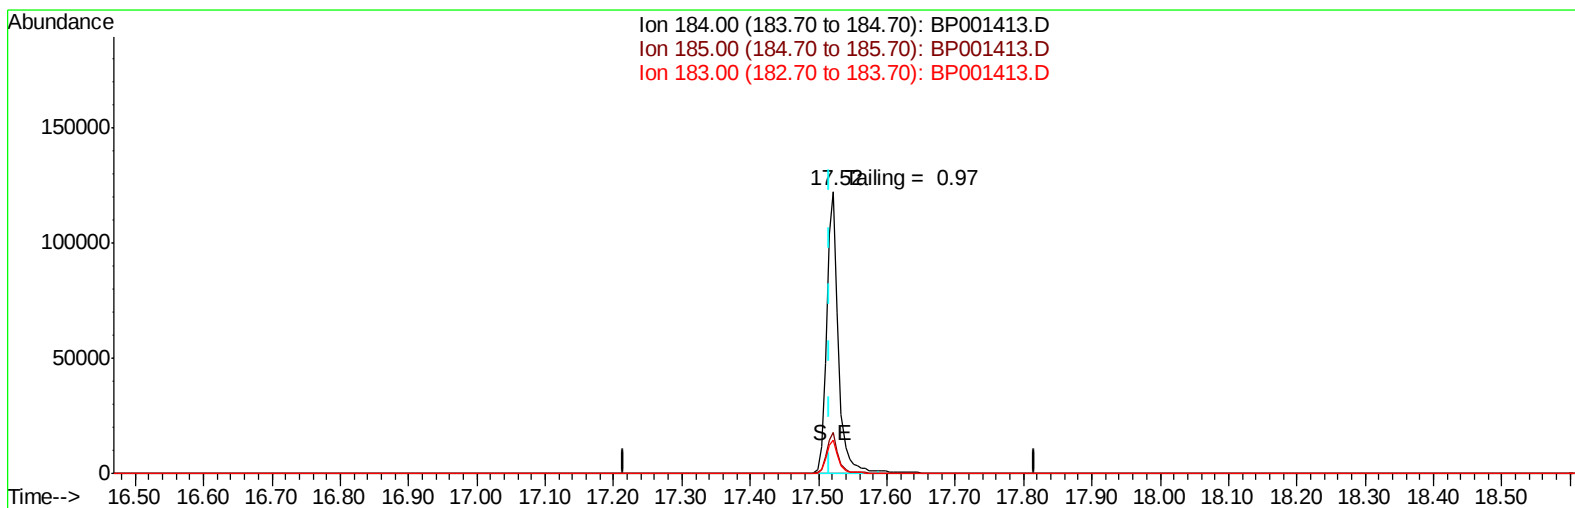

TIC: BP001413.D

(77) Benzidine

17.522min (+0.006) 133642.62ng

response 147859

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.50
183.00	12.00	11.82
0.00	0.00	0.00