

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122619\
 Data File : BP001441.D
 Acq On : 27 Dec 2019 03:24
 Operator : JU
 Sample : PB125736BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB125736BL

Quant Time: Dec 27 11:36:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 16:04:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	26767	20.00	ng	0.00
21) Naphthalene-d8	10.32	136	94362	20.00	ng	0.00
39) Acenaphthene-d10	13.18	164	59184	20.00	ng	0.00
64) Phenanthrene-d10	15.57	188	116455	20.00	ng	0.00
76) Chrysene-d12	19.22	240	90325	20.00	ng	0.00
87) Perylene-d12	20.99	264	94484	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.20	112	159616	96.38	ng	0.00
7) Phenol-d6	7.75	99	136140	63.00	ng	0.00
23) Nitrobenzene-d5	9.17	82	221574	90.17	ng	0.00
42) 2,4,6-Tribromophenol	14.47	330	105115	142.06	ng	0.00
45) 2-Fluorobiphenyl	12.10	172	442531	94.55	ng	0.00
79) Terphenyl-d14	17.86	244	605633	114.84	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122619\
Data File : BP001441.D
Acq On : 27 Dec 2019 03:24
Operator : JU
Sample : PB125736BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB125736BL

Quant Time: Dec 27 11:36:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

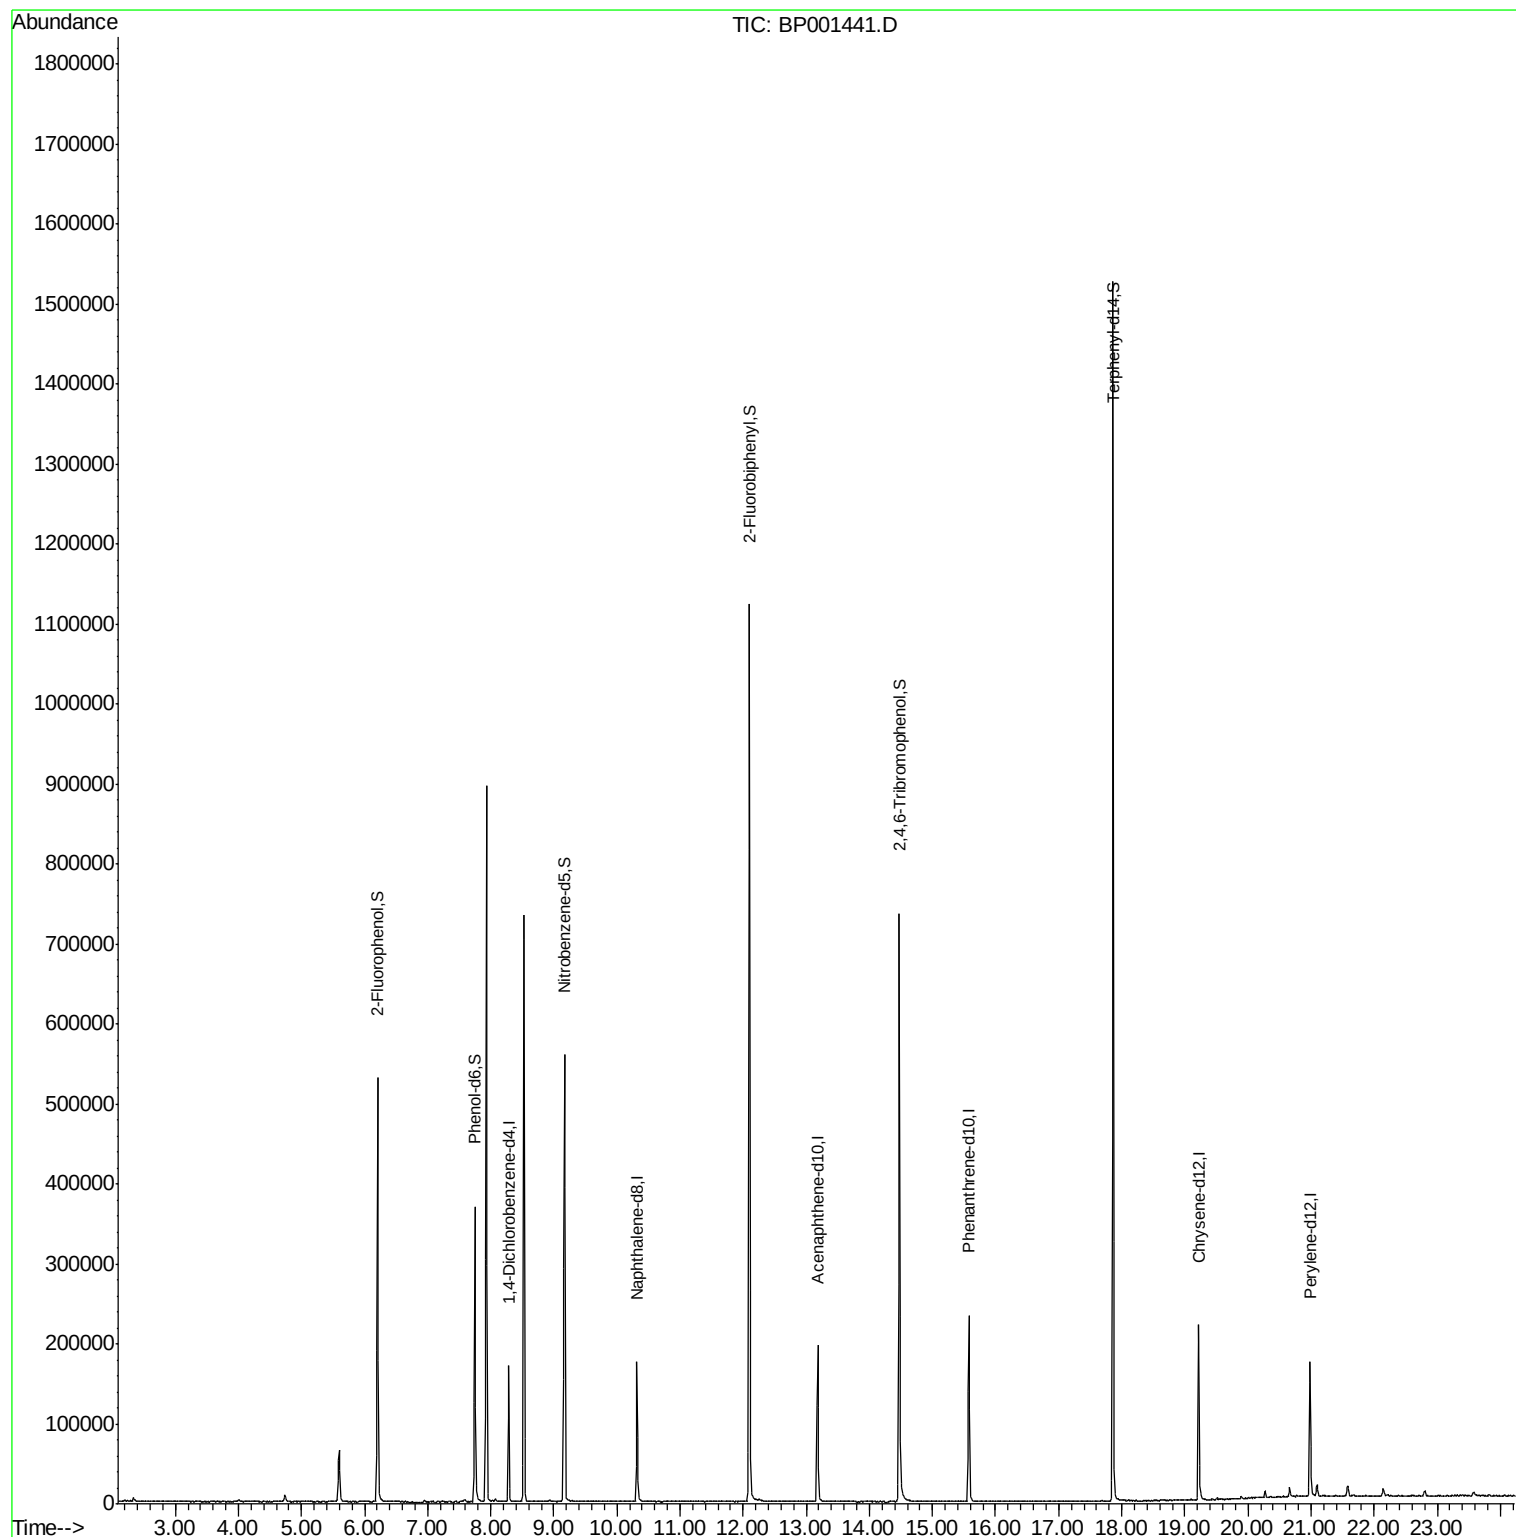

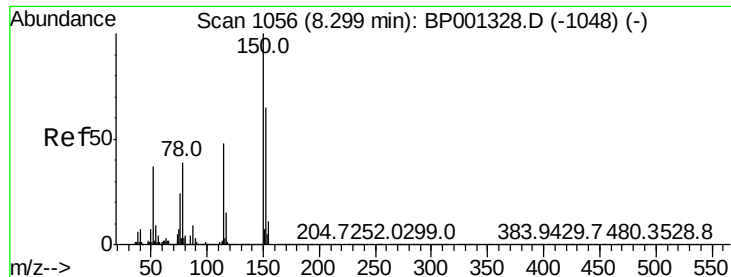

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.28 min Scan# 1053

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24

Instrument :

BNA_P

ClientSampleId :

PB125736BL


Tot Ion:152 Resp: 26767

Ion Ratio Lower Upper

152 100

150 160.9 127.0 190.6




115 69.2 56.1 84.1

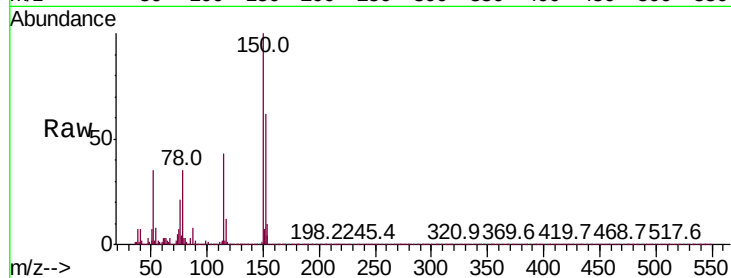

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

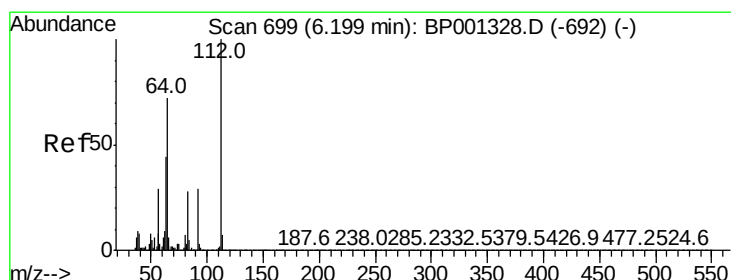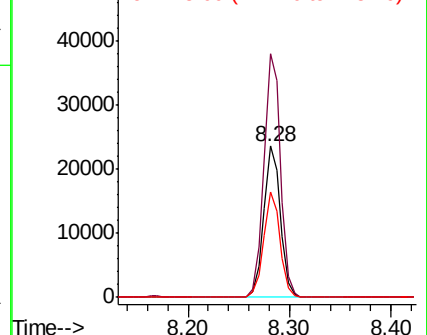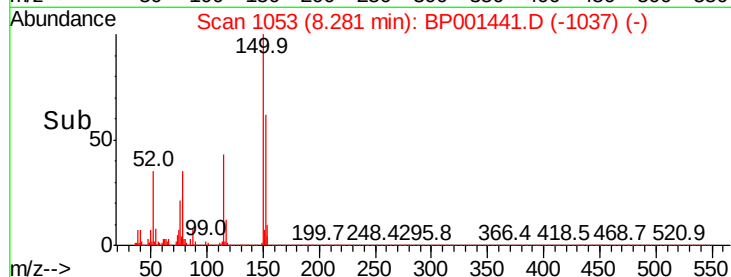

#5

2-Fluorophenol

Concen: 96.376 ng

RT: 6.20 min Scan# 700

Delta R.T. 0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24


Tgt Ion:112 Resp: 159616

Ion Ratio Lower Upper

112 100

64 62.7 53.9 80.9



63 41.3 33.4 50.0

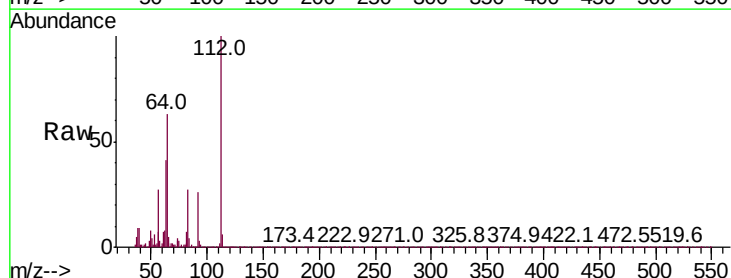


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

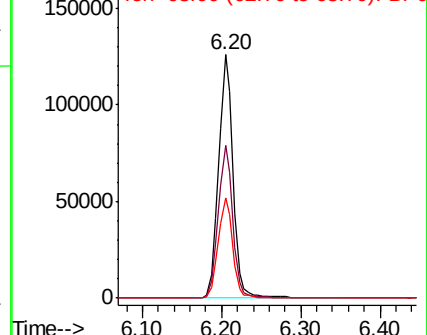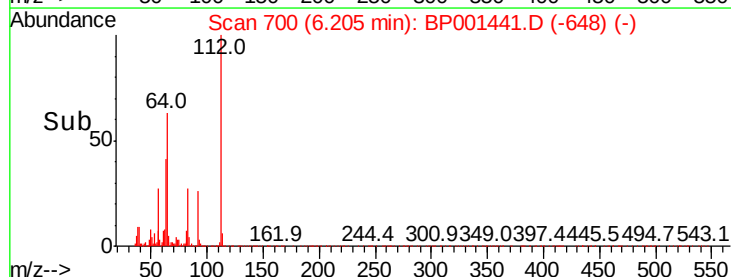

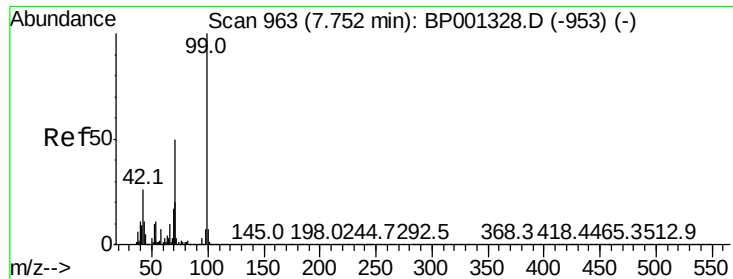

#7

Phenol-d6

Concen: 62.996 ng

RT: 7.75 min Scan# 962

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24

Instrument :

BNA_P

ClientSampled :

PB125736BL





Tot Ion: 99 Resp: 136140

Ion Ratio Lower Upper

99 100

42 27.9 20.8 31.2

71 47.3 38.2 57.4

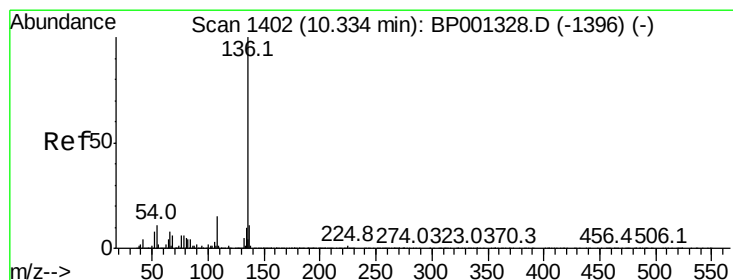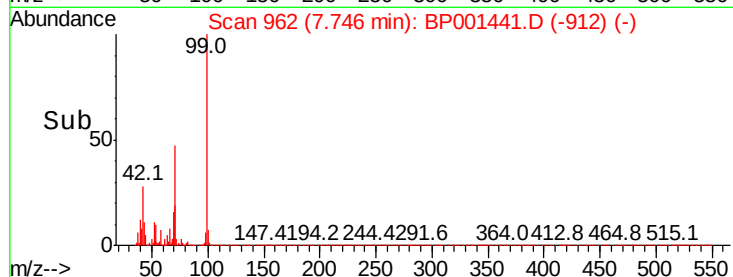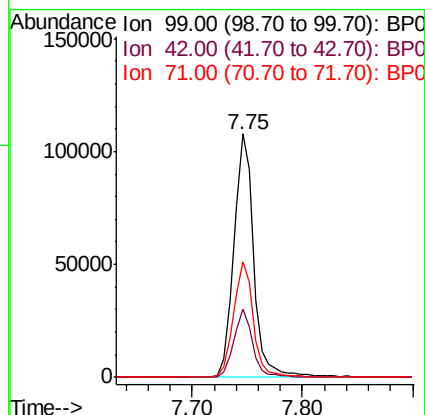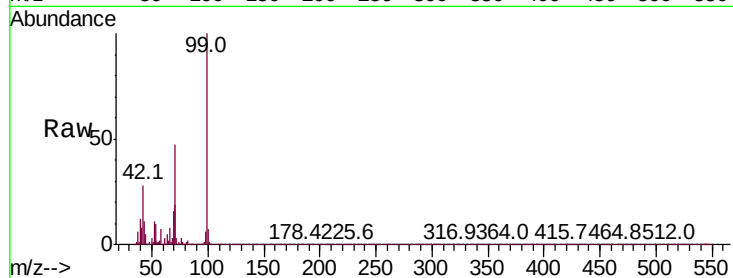

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.32 min Scan# 1399

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24

Tgt Ion: 136 Resp: 94362




Ion Ratio Lower Upper


136 100

137 11.8 9.0 13.4

54 10.3 7.3 10.9

68 5.6 3.8 5.6#


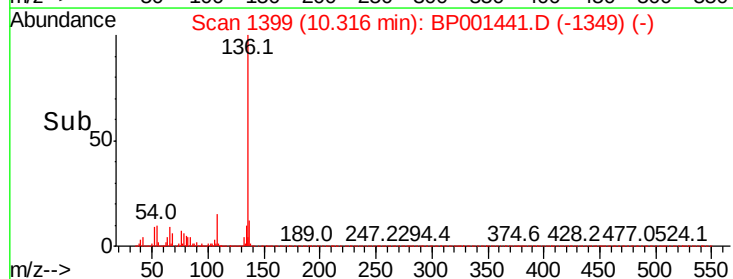
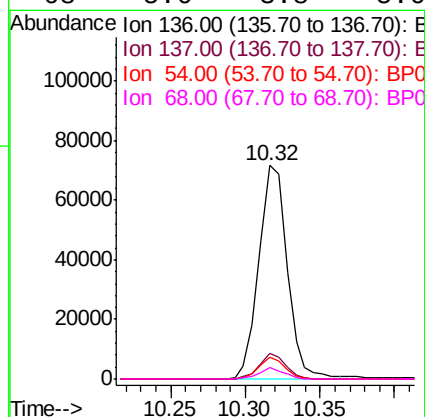
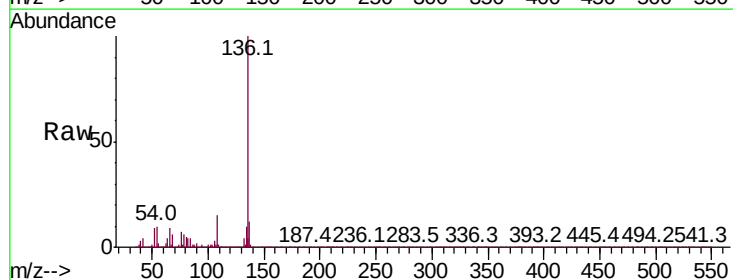


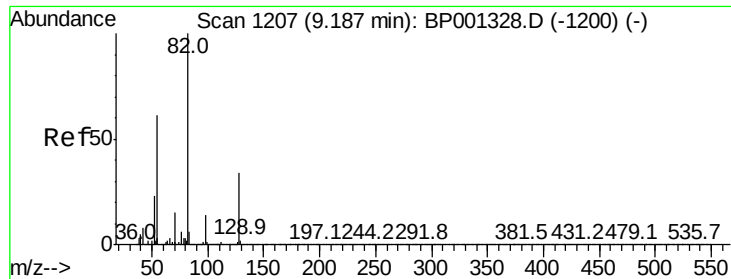

#23
 Nitrobenzene-d5
 Concen: 90.171 ng
 RT: 9.17 min Scan# 1204
 Delta R.T. -0.01 min
 Lab File: BP001441.D
 Acq: 27 Dec 2019 03:24




Instrument :
 BNA_P
 ClientSampleId :
 PB125736BL


Tot Ion	82	Resp	221574
Ion Ratio	100	Lower	Upper
128	36.5	27.4	41.0
54	63.8	47.5	71.3

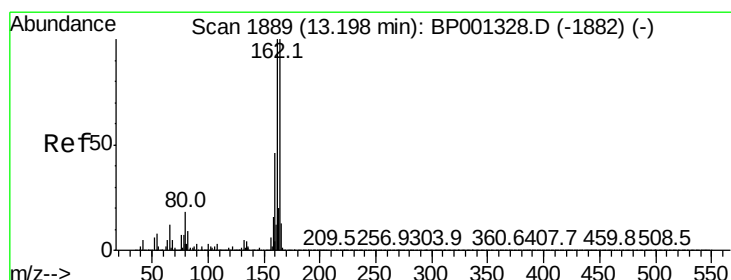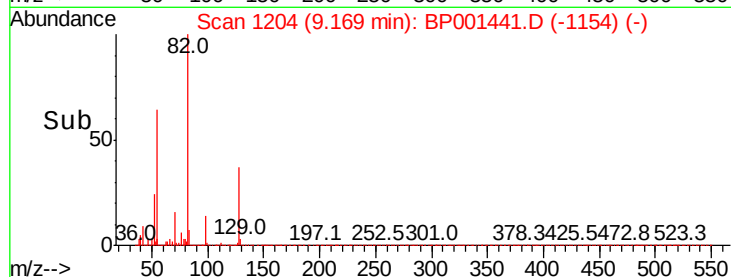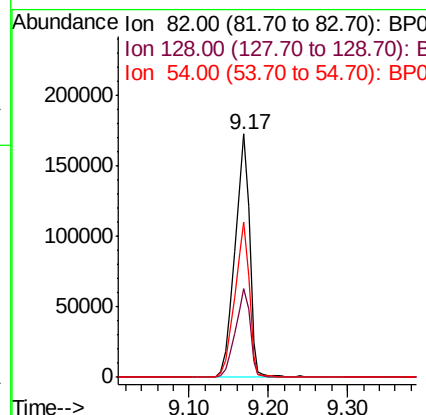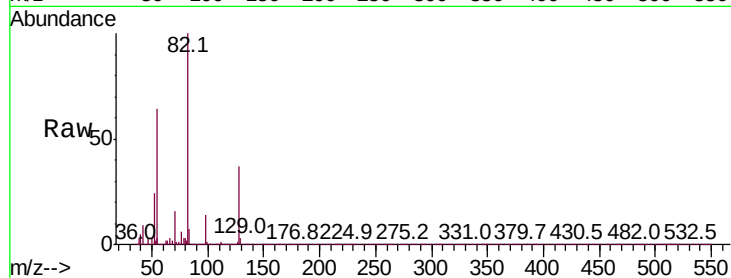

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 13.18 min Scan# 1886
 Delta R.T. 0.00 min
 Lab File: BP001441.D
 Acq: 27 Dec 2019 03:24

Tgt Ion	164	Resp	59184
Ion Ratio	100	Lower	Upper
162	96.9	78.2	117.4
160	42.3	35.1	52.7

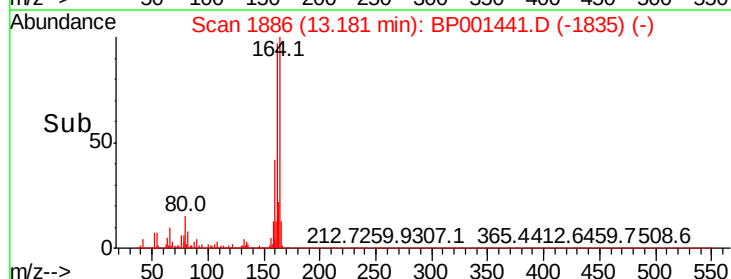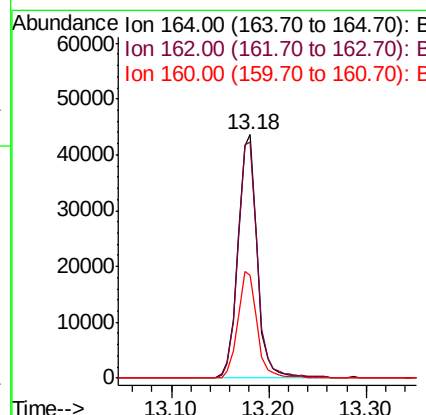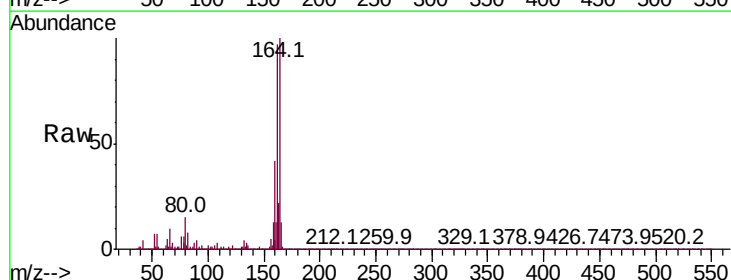


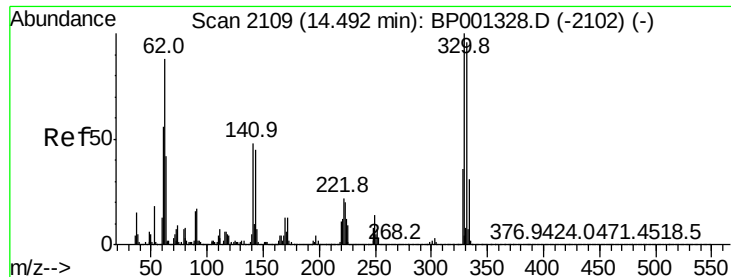

#42
 2,4,6-Tribromophenol
 Concen: 142.060 ng
 RT: 14.47 min Scan# 2106
 Delta R.T. -0.01 min
 Lab File: BP001441.D
 Acq: 27 Dec 2019 03:24

Instrument :
 BNA_P
 ClientSampleId :
 PB125736BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	78.3	117.5
141	39.6	26.8	40.2



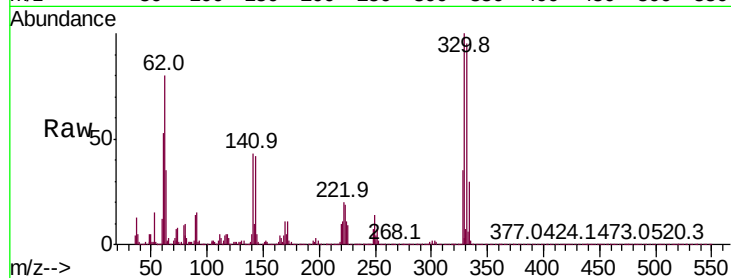


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

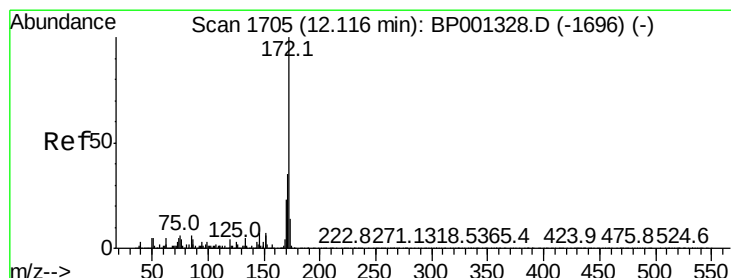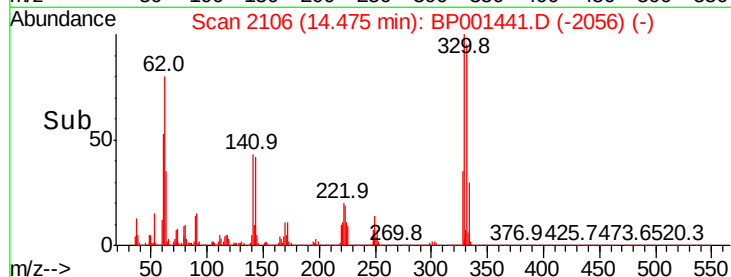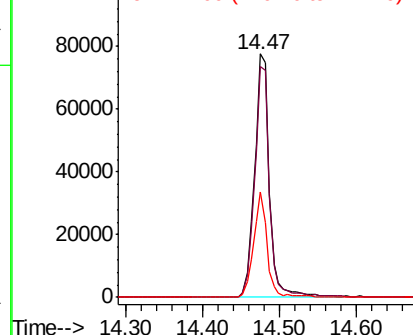

#45
 2-Fluorobiphenyl
 Concen: 94.548 ng
 RT: 12.10 min Scan# 1702
 Delta R.T. 0.00 min
 Lab File: BP001441.D
 Acq: 27 Dec 2019 03:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.9	27.4	41.0
170	22.9	18.2	27.4


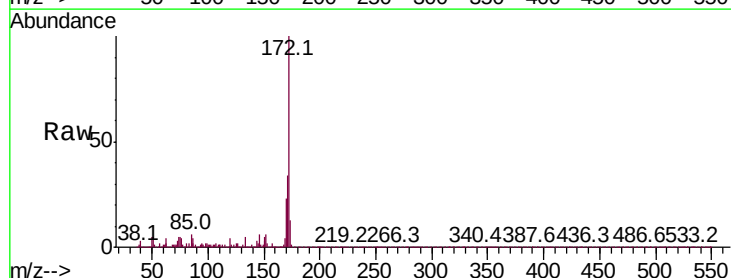



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

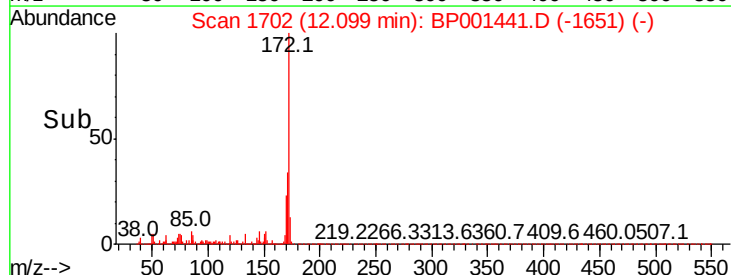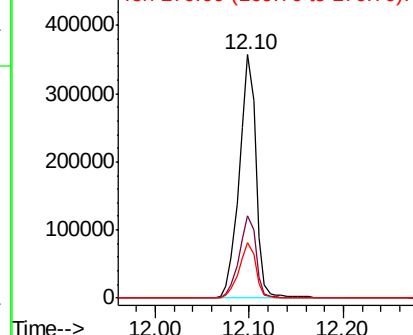

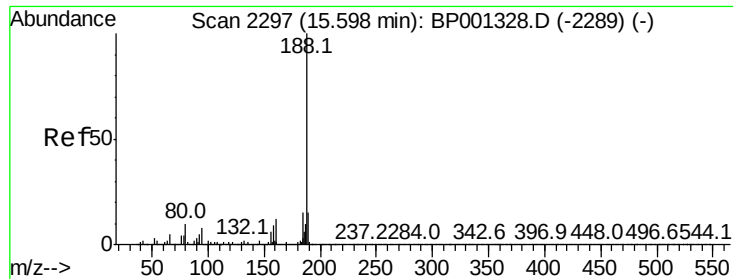

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.57 min Scan# 2293

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24

Instrument :

BNA_P

ClientSampleId :

PB125736BL


Tot Ion:188 Resp: 116455

Ion Ratio Lower Upper

188 100

94 7.7 5.8 8.8




80 7.6 5.7 8.5

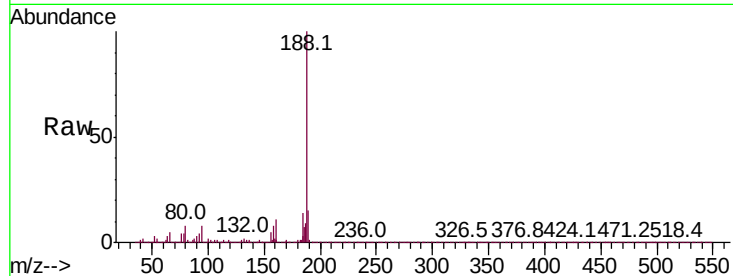

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

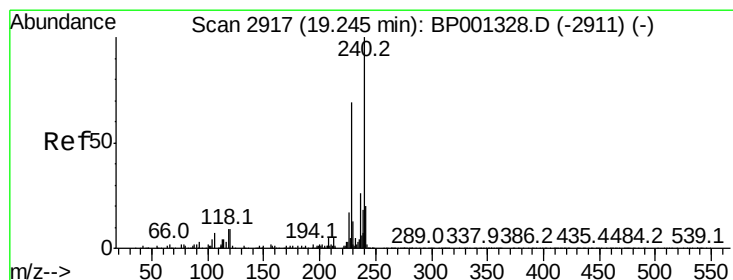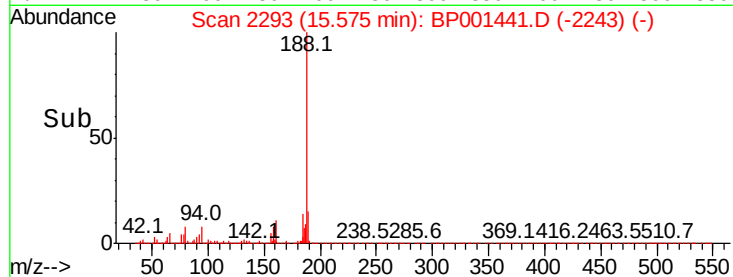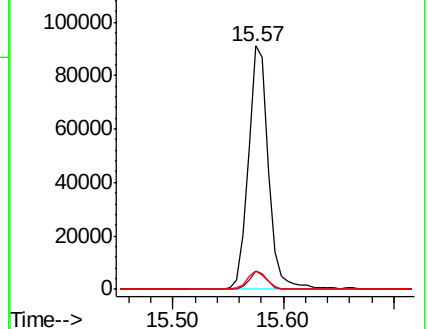

#76

Chrysene-d12

Concen: 20.000 ng

RT: 19.22 min Scan# 2913

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24


Tgt Ion:240 Resp: 90325

Ion Ratio Lower Upper

240 100

120 7.3 6.2 9.2



236 26.6 20.2 30.2

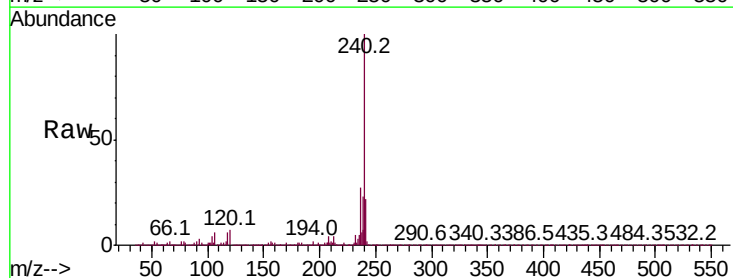


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

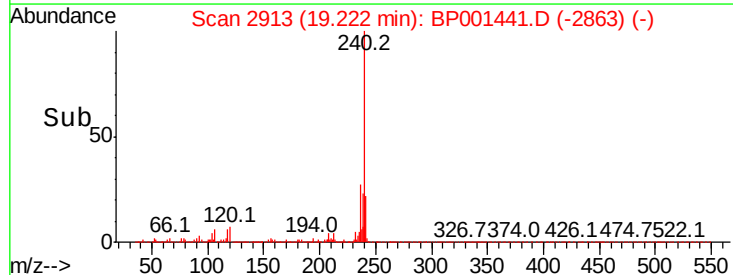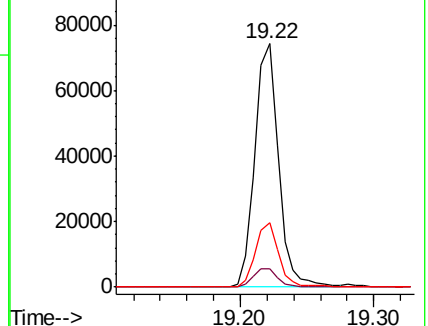

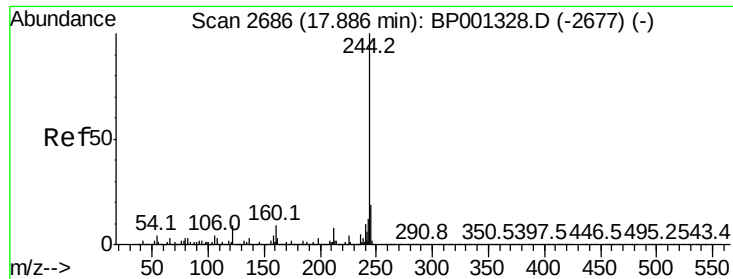

#79

Terphenyl-d14

Concen: 114.842 ng

RT: 17.86 min Scan# 2682

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24

Instrument :

BNA_P

ClientSampleId :

PB125736BL


Tot Ion:244 Resp: 605633

Ion Ratio Lower Upper

244 100

212 7.8 5.8 8.8




122 9.2 6.4 9.6

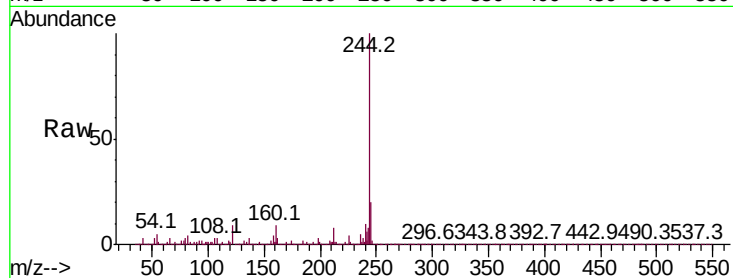

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

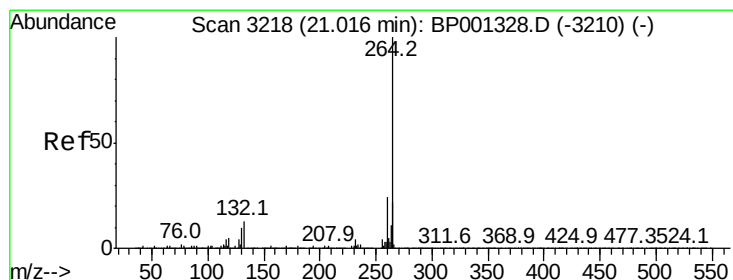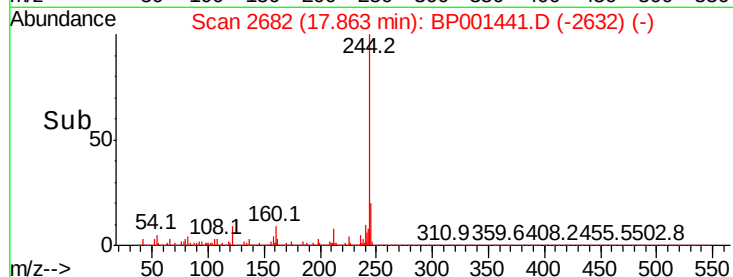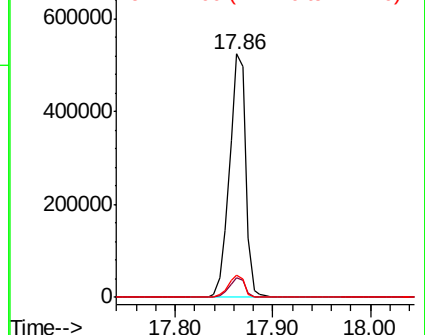

#87

Perylene-d12

Concen: 20.000 ng

RT: 20.99 min Scan# 3213

Delta R.T. -0.01 min

Lab File: BP001441.D

Acq: 27 Dec 2019 03:24


Tgt Ion:264 Resp: 94484

Ion Ratio Lower Upper

264 100

260 22.4 19.0 28.4

265 19.6 17.0 25.4

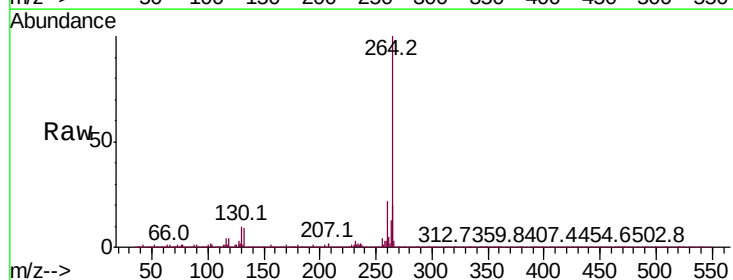

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

