


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122619\
 Data File : BP001413.D
 Acq On : 26 Dec 2019 10:09
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 16:04:49 2019

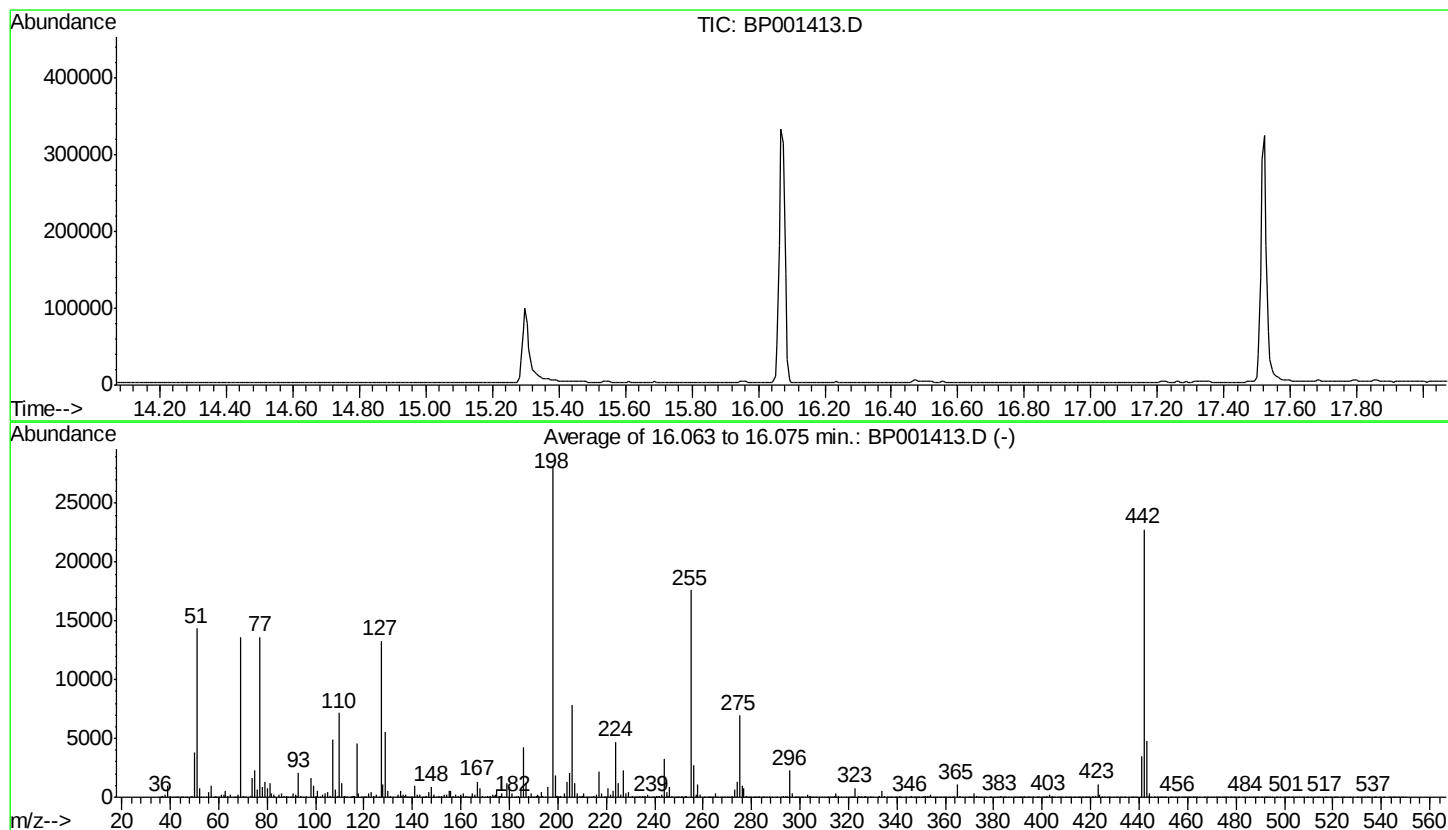

AutoFind: Scans 2376, 2377, 2378; Background Corrected with Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	14349	PASS
68	69	0.00	2	1.5	203	PASS
69	198	0.00	100	48.2	13589	PASS
70	69	0.00	2	0.8	114	PASS
127	198	10	80	47.3	13338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28205	PASS
199	198	5	9	6.6	1873	PASS
275	198	10	60	24.6	6947	PASS
365	198	1	100	3.8	1072	PASS
441	198	0.01	100	12.3	3458	PASS
442	198	50	100	80.9	22812	PASS
443	442	15	24	20.8	4742	PASS