


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122619\
 Data File : BP001437.D
 Acq On : 27 Dec 2019 00:55
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 16:04:49 2019

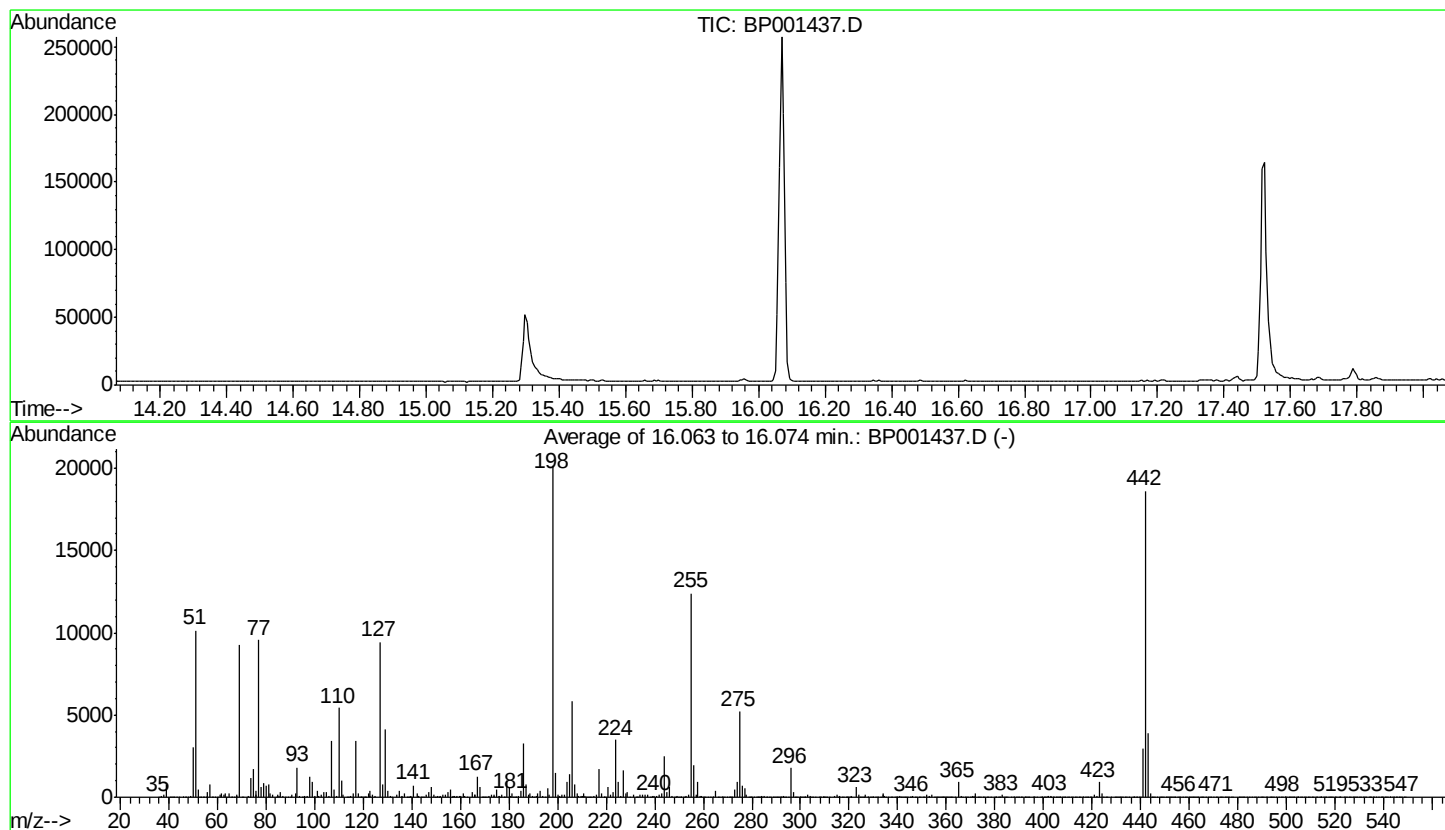

AutoFind: Scans 2376, 2377, 2378; Background Corrected with Scan 2366

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	10129	PASS
68	69	0.00	2	1.7	156	PASS
69	198	0.00	100	45.9	9259	PASS
70	69	0.00	2	0.2	20	PASS
127	198	10	80	46.8	9443	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20160	PASS
199	198	5	9	7.3	1462	PASS
275	198	10	60	25.7	5187	PASS
365	198	1	100	4.5	901	PASS
441	198	0.01	100	14.8	2982	PASS
442	198	50	100	92.3	18617	PASS
443	442	15	24	20.9	3896	PASS