




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019097.D
Acq On : 26 Dec 2023 23:26
Operator : MA/JU
Sample : 05976-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X2

Manual IntegrationsAPPROVED

Quant Time: Dec 26 23:55:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 26 22:20:53 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/28/2023

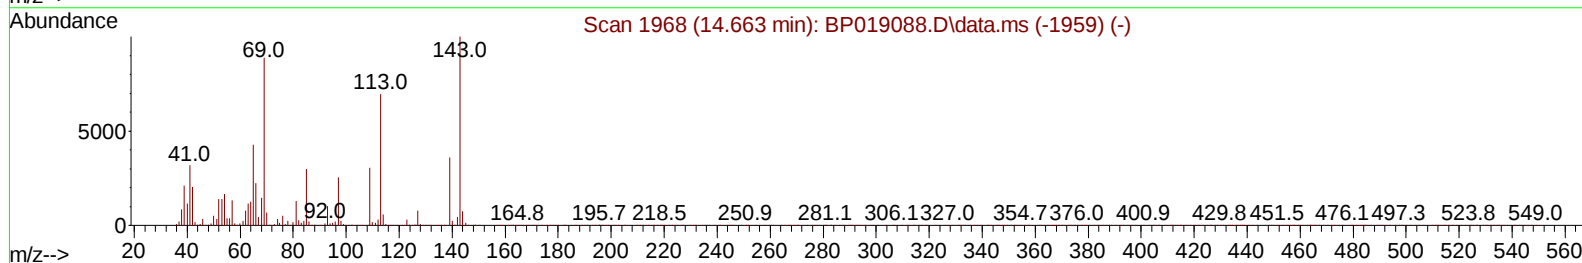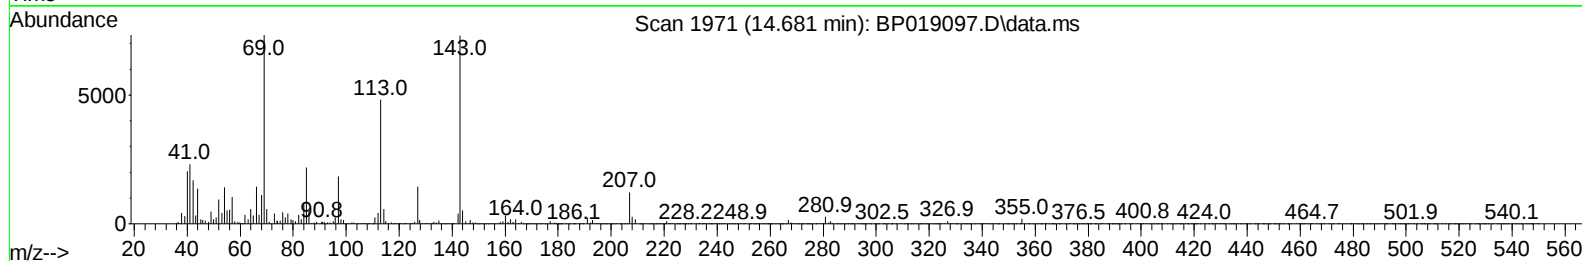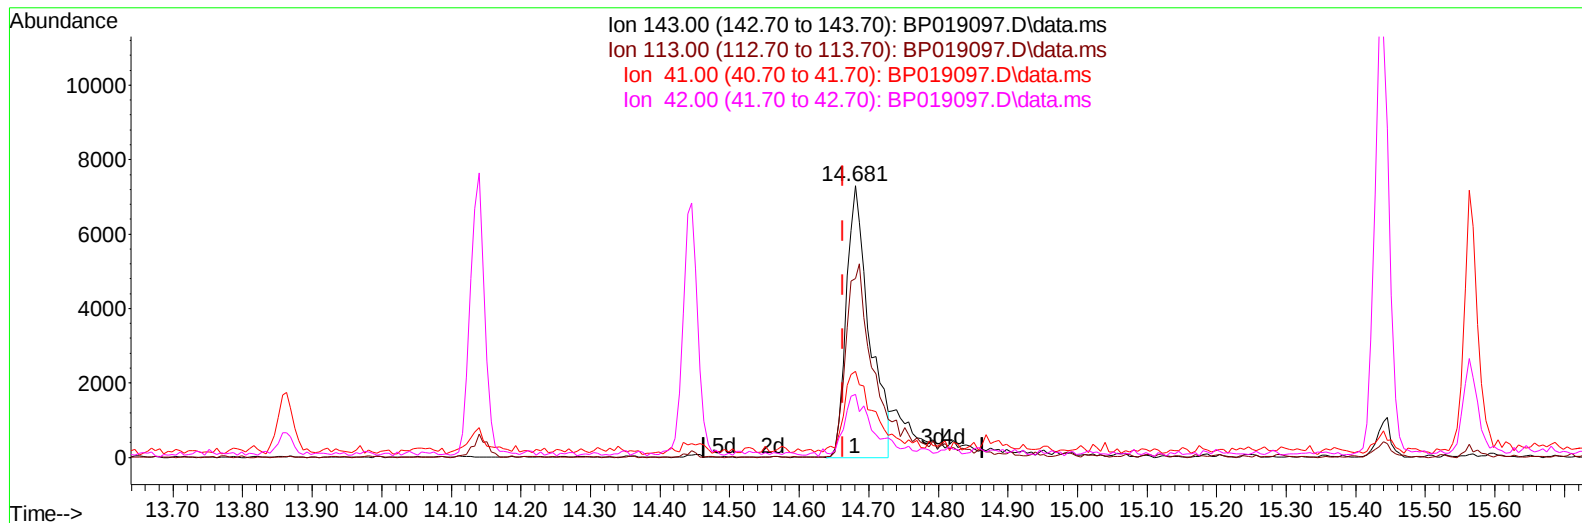

TIC: BP019097.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.018) 2.95 ng/u1

response 16642

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	65.97
41.00	34.60	31.76
42.00	23.00	23.30




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019097.D
 Acq On : 26 Dec 2023 23:26
 Operator : MA/JU
 Sample : 05976-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X2

Manual IntegrationsAPPROVED

Quant Time: Dec 26 23:55:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 26 22:20:53 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/28/2023

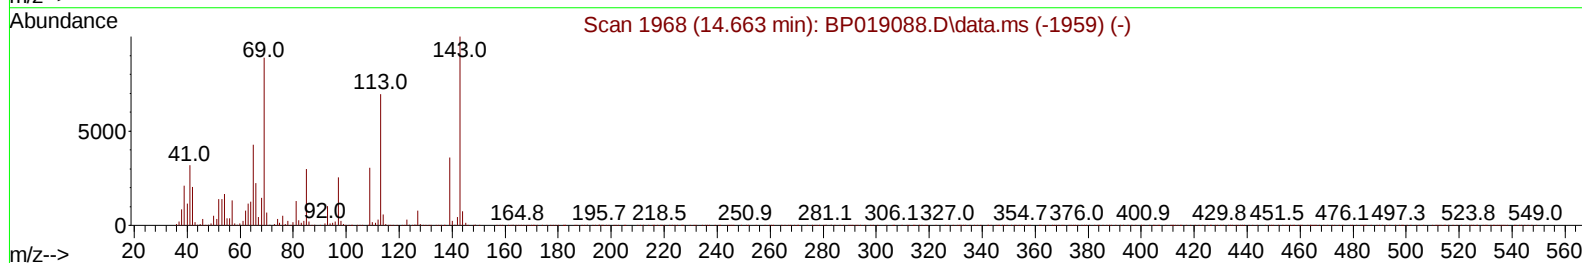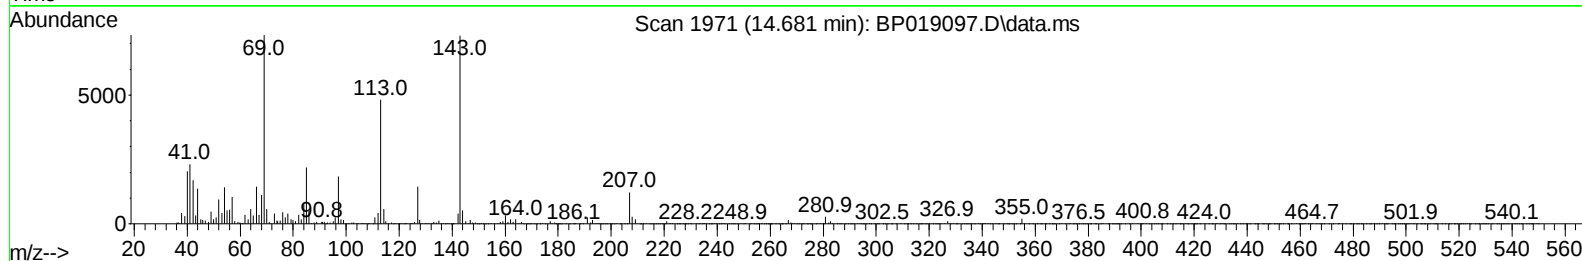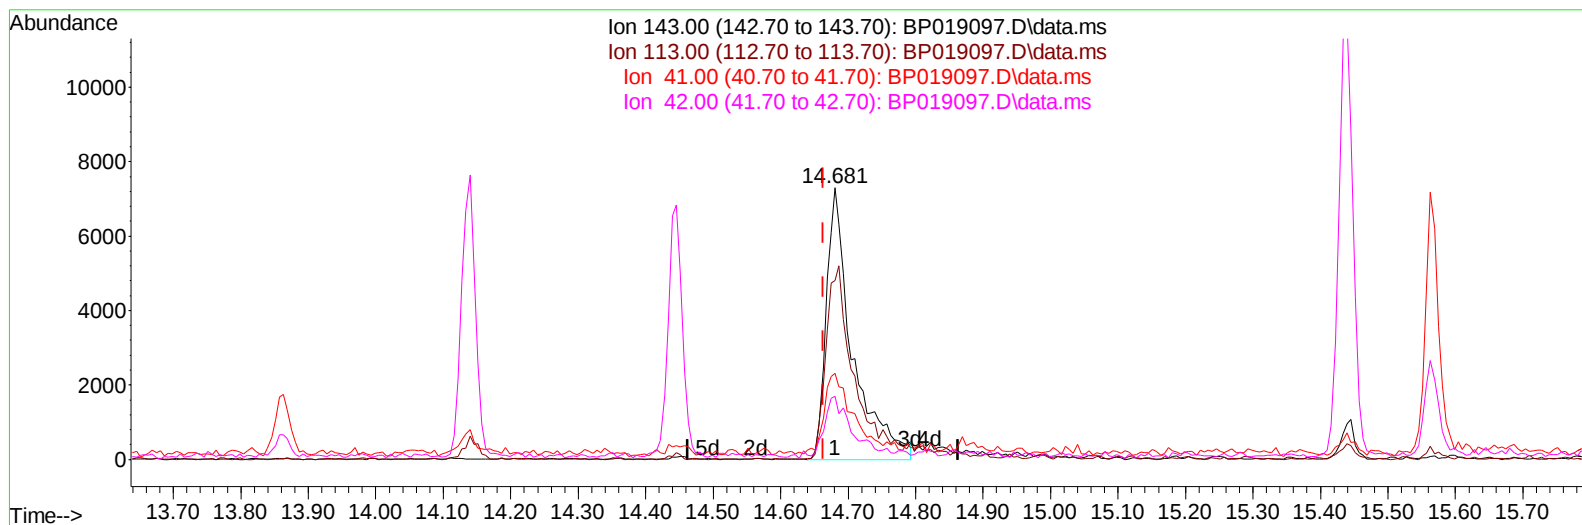

TIC: BP019097.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.018) 3.48 ng/ul m

response 19637

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	65.97
41.00	34.60	31.76
42.00	23.00	23.30

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019097.D
 Acq On : 26 Dec 2023 23:26
 Operator : MA/JU
 Sample : 05976-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/28/2023

Quant Time: Dec 26 23:56:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 26 22:20:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	153137	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	593314	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	384692	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	910154	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	998237	20.000	ng/ul	0.00
88) Perylene-d12	23.639	264	1181306	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	13731	3.056	ng/uL	0.00
4) Pyridine-d5	3.670	84	63373	5.265	ng/ul	0.00
7) Phenol-d5	6.987	99	59766	3.889	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	228683	25.107	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	212737	17.741	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	120225	9.667	ng/ul	0.00
21) Nitrobenzene-d5	8.975	128	142016	26.893	ng/ul	0.00
24) 2-Nitrophenol-d4	9.693	143	144270	26.351	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	251845	22.496	ng/ul	0.00
31) 4-Chloroaniline-d4	10.752	131	312238	21.342	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	980269	28.551	ng/ul	0.00
49) Acenaphthylene-d8	14.140	160	1061261	28.071	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	19637m	3.484	ng/ul	0.02
60) Fluorene-d10	15.440	176	894715	31.045	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	148108	27.139	ng/ul	0.00
73) Anthracene-d10	17.292	188	1588230	33.193	ng/ul	0.00
81) Pyrene-d10	19.533	212	2064520	26.569	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.492	264	2305325	33.469	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019097.D
Acq On : 26 Dec 2023 23:26
Operator : MA/JU
Sample : 05976-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/28/2023

Quant Time: Dec 26 23:56:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 26 22:20:53 2023
Response via : Initial Calibration

