

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019084.D
 Acq On : 26 Dec 2023 15:30
 Operator : MA/JU
 Sample : 05976-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	18	21	24	rBV3	10343	11935	0.27%	0.035%
2	3.246	24	27	35	rVB	35162	41887	0.96%	0.124%
3	3.534	74	76	83	rBV	11317	16797	0.38%	0.050%
4	3.669	95	99	115	rBV	172110	266324	6.09%	0.788%
5	3.893	135	137	141	rVB3	6057	6459	0.15%	0.019%
6	3.987	150	153	159	rBV2	9311	14972	0.34%	0.044%
7	6.987	657	663	673	rBV	130880	212394	4.85%	0.628%
8	7.152	684	691	701	rBV	515771	777705	17.77%	2.300%
9	7.346	716	724	737	rBV	487419	771743	17.64%	2.283%
10	7.452	737	742	746	rVB8	2947	4506	0.10%	0.013%
11	7.810	797	803	812	rBV	544447	854565	19.53%	2.528%
12	8.528	915	925	936	rBV	371367	600394	13.72%	1.776%
13	8.975	993	1001	1013	rBV	561513	902159	20.62%	2.668%
14	9.381	1066	1070	1076	rVB8	4318	8022	0.18%	0.024%
15	9.551	1093	1099	1104	rBV5	7602	13654	0.31%	0.040%
16	9.693	1116	1123	1133	rBV	417263	686512	15.69%	2.031%
17	10.234	1207	1215	1228	rBV	614427	1047685	23.94%	3.099%
18	10.604	1271	1278	1289	rVB	691967	1141156	26.08%	3.375%
19	10.751	1296	1303	1317	rBV	545828	951181	21.74%	2.813%
20	11.181	1371	1376	1382	rVB10	2280	5469	0.12%	0.016%
21	11.369	1402	1408	1417	rBV3	13594	31871	0.73%	0.094%
22	12.198	1543	1549	1554	rBV2	12575	20815	0.48%	0.062%
23	13.081	1695	1699	1711	rVB9	5852	13047	0.30%	0.039%
24	13.275	1728	1732	1735	rBV6	4081	5073	0.12%	0.015%
25	13.351	1739	1745	1749	rBV4	10034	16635	0.38%	0.049%
26	13.863	1824	1832	1841	rBV	1172366	1615091	36.91%	4.777%
27	14.139	1867	1879	1889	rBV	1350660	1976951	45.18%	5.847%
28	14.445	1924	1931	1941	rBV	977662	1423947	32.54%	4.212%
29	14.681	1963	1971	1986	rBV	55505	151260	3.46%	0.447%
30	14.875	1999	2004	2005	rBV4	3454	4930	0.11%	0.015%
31	15.198	2055	2059	2064	rVB4	4199	5685	0.13%	0.017%
32	15.439	2093	2100	2112	rBV	1805061	2589449	59.18%	7.659%
33	15.569	2116	2122	2132	rVV	470810	683289	15.61%	2.021%
34	15.675	2136	2140	2147	rVB5	9392	18354	0.42%	0.054%
35	16.010	2193	2197	2201	rBV7	4289	6149	0.14%	0.018%
36	16.228	2229	2234	2239	rVB6	7618	10808	0.25%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019084.D
 Acq On : 26 Dec 2023 15:30
 Operator : MA/JU
 Sample : 05976-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.010	2365	2367	2375	rVB8	6445	9909	0.23%	0.029%
38	17.198	2392	2399	2408	rBV	1170722	1617035	36.95%	4.783%
39	17.298	2409	2416	2432	rVV	1985108	2946116	67.33%	8.714%
40	17.875	2511	2514	2518	rVB3	8611	9670	0.22%	0.029%
41	18.086	2546	2550	2559	rBV2	57450	93722	2.14%	0.277%
42	19.116	2721	2725	2730	rBV2	27860	37487	0.86%	0.111%
43	19.186	2733	2737	2745	rBV	29791	48634	1.11%	0.144%
44	19.327	2758	2761	2765	rBV3	23010	24998	0.57%	0.074%
45	19.539	2791	2797	2804	rBV	2759795	3620247	82.73%	10.708%
46	21.292	3090	3095	3103	rBV	1508340	1927243	44.04%	5.700%
47	23.492	3463	3469	3484	rVB	2194351	4375911	100.00%	12.943%
48	23.645	3489	3495	3504	rVB	1087155	2188855	50.02%	6.474%




Sum of corrected areas: 33808700

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019084.D
Acq On : 26 Dec 2023 15:30
Operator : MA/JU
Sample : 05976-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7T8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

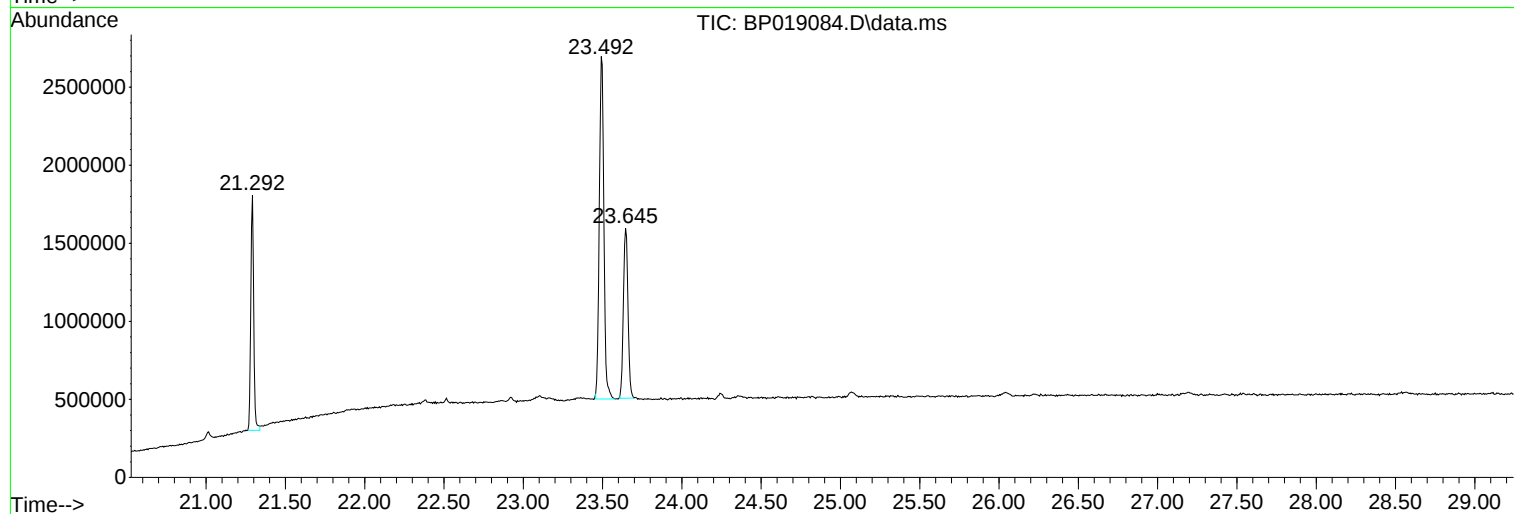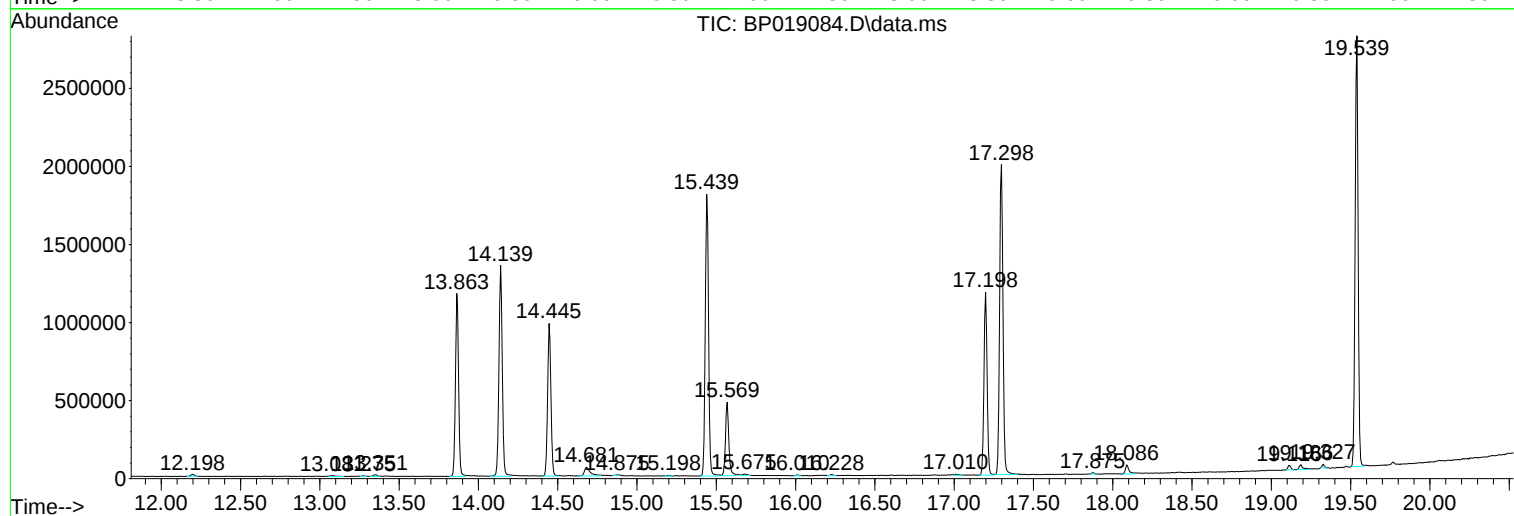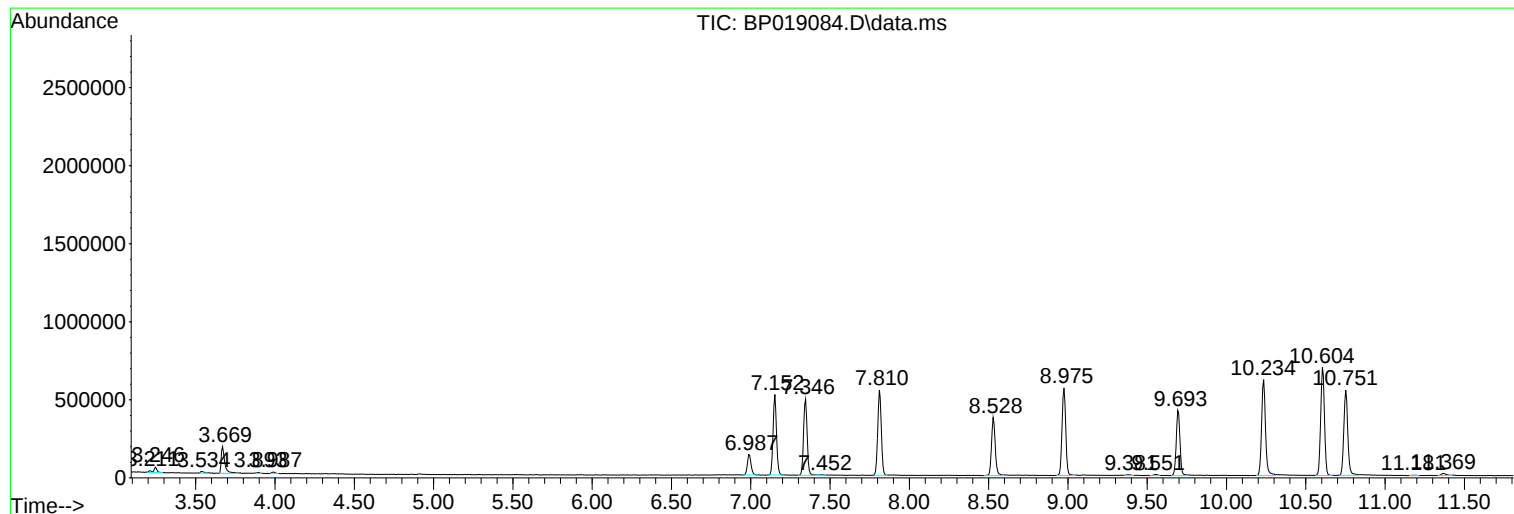

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019084.D
Acq On : 26 Dec 2023 15:30
Operator : MA/JU
Sample : 05976-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7T8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019084.D
Acq On : 26 Dec 2023 15:30
Operator : MA/JU
Sample : 05976-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7T8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------