

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019086.D
 Acq On : 26 Dec 2023 16:38
 Operator : MA/JU
 Sample : 05808-08MEDL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COB02MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	34	rVB	11292	15578	0.56%	0.071%
2	3.675	96	100	111	rBV	67322	112731	4.07%	0.512%
3	3.987	149	153	160	rVB	43637	58088	2.09%	0.264%
4	4.916	308	311	314	rBV5	2205	3390	0.12%	0.015%
5	6.993	656	664	680	rVB	123170	215566	7.77%	0.978%
6	7.151	685	691	699	rVB	115331	176928	6.38%	0.803%
7	7.345	717	724	735	rBV	132328	210691	7.60%	0.956%
8	7.698	778	784	791	rVB	14866	24387	0.88%	0.111%
9	7.810	795	803	814	rBV	507155	800256	28.86%	3.631%
10	8.163	857	863	871	rVB	29612	47373	1.71%	0.215%
11	8.534	918	926	936	rBV	141394	250817	9.04%	1.138%
12	8.975	995	1001	1008	rBV	116277	196126	7.07%	0.890%
13	9.539	1089	1097	1099	rBV7	4553	8289	0.30%	0.038%
14	9.698	1117	1124	1129	rBV	79066	136420	4.92%	0.619%
15	9.745	1129	1132	1139	rVB9	6128	11905	0.43%	0.054%
16	9.869	1147	1153	1155	rBV7	1618	3427	0.12%	0.016%
17	9.987	1170	1173	1177	rVB6	2828	3631	0.13%	0.016%
18	10.234	1208	1215	1227	rBV	119302	239107	8.62%	1.085%
19	10.322	1229	1230	1237	rVB7	2060	3447	0.12%	0.016%
20	10.469	1247	1255	1267	rBV	1673017	2773031	100.00%	12.583%
21	10.604	1270	1278	1289	rVB	628404	1058735	38.18%	4.804%
22	10.757	1296	1304	1316	rBV	125507	242696	8.75%	1.101%
23	10.986	1335	1343	1352	rVB	709778	1190233	42.92%	5.401%
24	11.369	1404	1408	1416	rBV8	3213	6776	0.24%	0.031%
25	11.875	1490	1494	1496	rBV5	2816	4066	0.15%	0.018%
26	11.898	1496	1498	1503	rVB6	3120	4377	0.16%	0.020%
27	12.028	1516	1520	1526	rVB9	3602	6047	0.22%	0.027%
28	12.175	1541	1545	1555	rVB9	6749	15313	0.55%	0.069%
29	12.351	1570	1575	1581	rVB5	9138	15875	0.57%	0.072%
30	12.604	1610	1618	1620	rBV	113059	177599	6.40%	0.806%
31	12.633	1620	1623	1633	rVV	211655	336172	12.12%	1.525%
32	12.704	1633	1635	1639	rVB5	5468	6999	0.25%	0.032%
33	13.175	1709	1715	1719	rBV9	2047	3578	0.13%	0.016%
34	13.245	1719	1727	1738	rBV	1543038	2354173	84.90%	10.683%
35	13.351	1741	1745	1750	rVB6	12152	20863	0.75%	0.095%
36	13.439	1757	1760	1765	rVB6	3390	4952	0.18%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019086.D
 Acq On : 26 Dec 2023 16:38
 Operator : MA/JU
 Sample : 05808-08MEDL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B02MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.480	1765	1767	1771	rVB5	1988	2820	0.10%	0.013%
38	13.704	1802	1805	1810	rBV7	1553	2805	0.10%	0.013%
39	13.863	1826	1832	1845	rBV	240946	368634	13.29%	1.673%
40	14.139	1872	1879	1889	rBV	288972	437796	15.79%	1.987%
41	14.251	1894	1898	1907	rVB	4924	11954	0.43%	0.054%
42	14.445	1924	1931	1946	rBV	894922	1356551	48.92%	6.156%
43	14.539	1946	1947	1951	rVV4	2986	3594	0.13%	0.016%
44	14.686	1965	1972	1979	rBV3	34785	87581	3.16%	0.397%
45	14.763	1980	1985	1998	rVB	263228	393552	14.19%	1.786%
46	15.439	2093	2100	2111	rBV	393683	596007	21.49%	2.705%
47	15.574	2117	2123	2132	rBV	51308	88800	3.20%	0.403%
48	16.216	2228	2232	2238	rBV8	6115	10367	0.37%	0.047%
49	16.498	2276	2280	2286	rVB7	8166	12548	0.45%	0.057%
50	16.980	2359	2362	2363	rBV3	4040	4181	0.15%	0.019%
51	17.198	2393	2399	2409	rBV	1080129	1566308	56.48%	7.107%
52	17.298	2410	2416	2427	rVB	391930	593483	21.40%	2.693%
53	17.598	2461	2467	2474	rBV6	16206	35626	1.28%	0.162%
54	18.086	2545	2550	2558	rBV3	38468	62045	2.24%	0.282%
55	18.504	2617	2621	2625	rBV3	27366	31032	1.12%	0.141%
56	19.186	2734	2737	2740	rBV3	11333	15305	0.55%	0.069%
57	19.327	2758	2761	2764	rBV5	20986	26832	0.97%	0.122%
58	19.468	2783	2785	2790	rVB5	13648	15596	0.56%	0.071%
59	19.539	2791	2797	2804	rBV	537737	751743	27.11%	3.411%
60	21.292	3090	3095	3102	rBV	1365882	1824426	65.79%	8.279%
61	23.492	3464	3469	3483	rVB	424790	900991	32.49%	4.088%
62	23.645	3489	3495	3506	rVB	1022958	2097338	75.63%	9.517%




Sum of corrected areas: 22037557

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019086.D
Acq On : 26 Dec 2023 16:38
Operator : MA/JU
Sample : 05808-08MEDL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B02MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

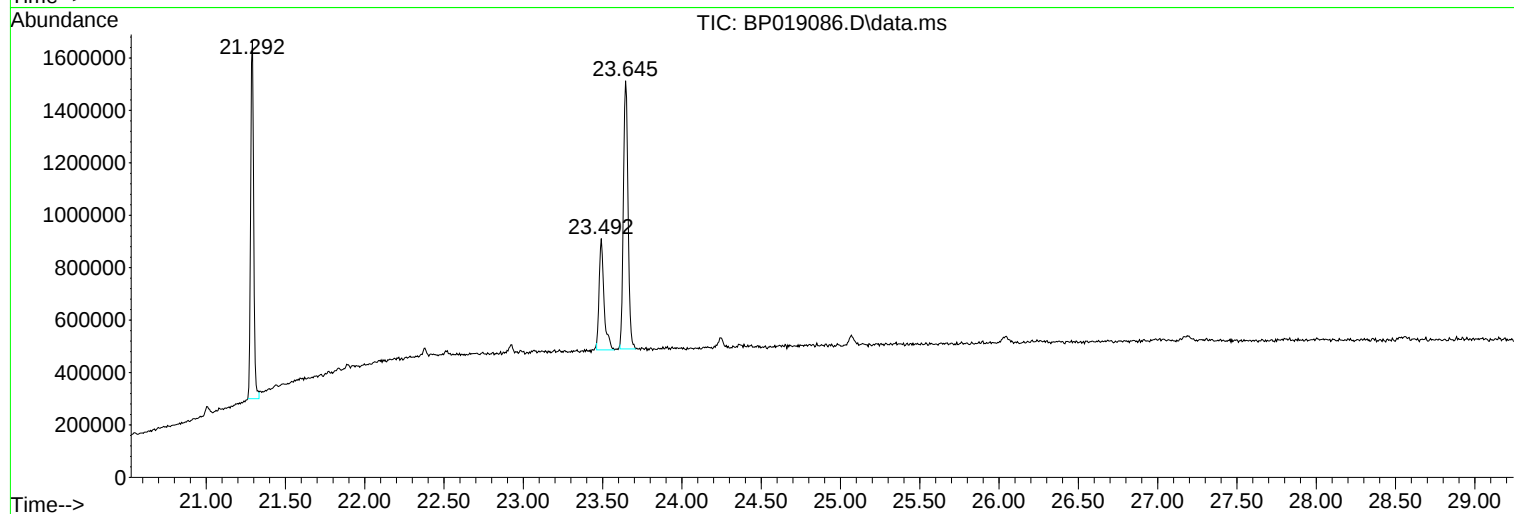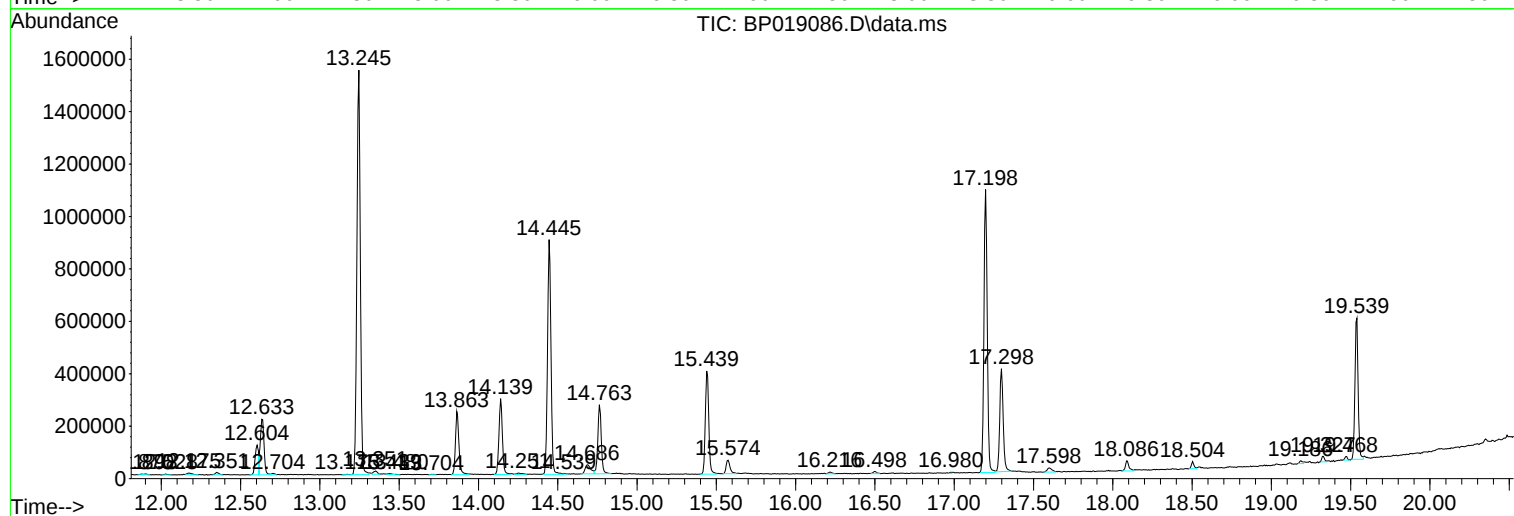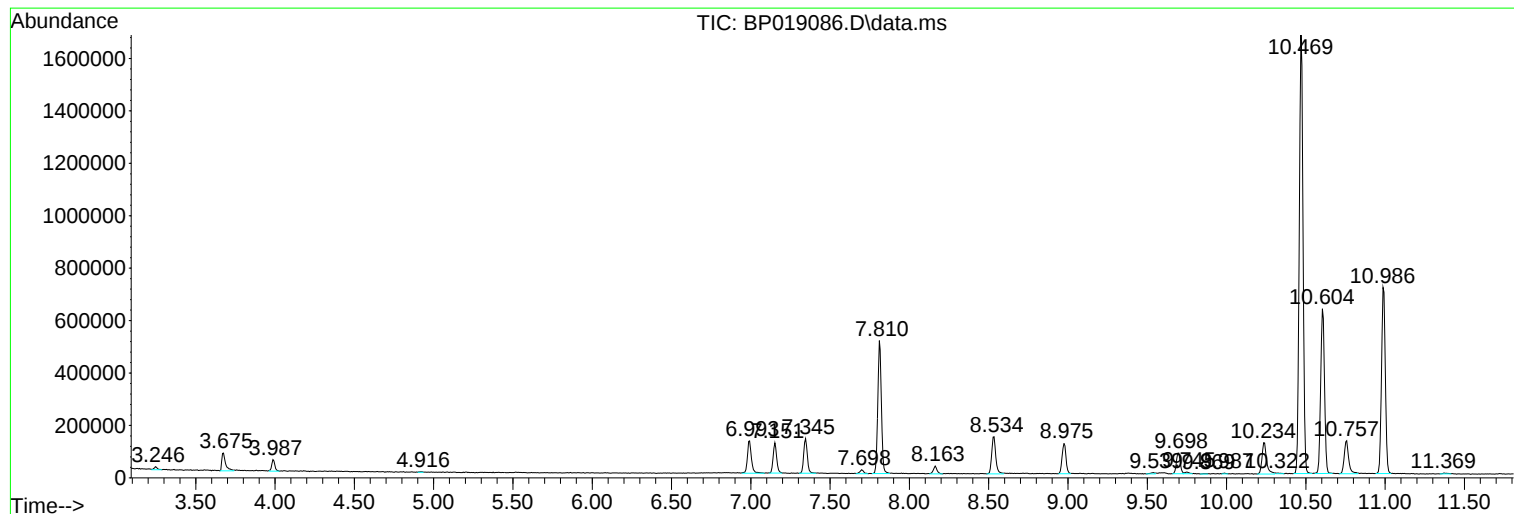

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019086.D
Acq On : 26 Dec 2023 16:38
Operator : MA/JU
Sample : 05808-08MEDL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B02MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019086.D
Acq On : 26 Dec 2023 16:38
Operator : MA/JU
Sample : 05808-08MEDL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B02MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc