

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019089.D
 Acq On : 26 Dec 2023 18:54
 Operator : MA/JU
 Sample : PB158028BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	32	rVB	53471	63768	1.88%	0.169%
2	3.664	94	98	115	rBV	628586	901520	26.57%	2.392%
3	3.987	150	153	157	rVB	12536	15457	0.46%	0.041%
4	6.987	657	663	677	rBV	672348	1027939	30.29%	2.727%
5	7.152	682	691	700	rVB	558300	849205	25.03%	2.253%
6	7.346	716	724	734	rBV	645068	1042210	30.71%	2.765%
7	7.810	795	803	812	rBV	612749	956141	28.18%	2.537%
8	8.528	918	925	943	rBV	770338	1260901	37.16%	3.345%
9	8.975	993	1001	1012	rBV	611643	988295	29.13%	2.622%
10	9.693	1115	1123	1136	rBV	474020	781309	23.03%	2.073%
11	10.234	1207	1215	1230	rBV	714141	1262936	37.22%	3.351%
12	10.604	1271	1278	1286	rVB	792210	1301741	38.36%	3.454%
13	10.751	1295	1303	1319	rBV	762099	1291217	38.05%	3.426%
14	12.204	1545	1550	1557	rVB2	12100	23891	0.70%	0.063%
15	13.351	1737	1745	1748	rBV6	4114	6351	0.19%	0.017%
16	13.422	1750	1757	1762	rBV10	2580	5861	0.17%	0.016%
17	13.863	1825	1832	1844	rBV	1285749	1800589	53.07%	4.777%
18	14.139	1871	1879	1891	rBV	1520984	2230215	65.73%	5.917%
19	14.445	1924	1931	1943	rBV	1265161	1762354	51.94%	4.676%
20	14.669	1962	1969	1993	rBV	338411	764442	22.53%	2.028%
21	15.439	2093	2100	2114	rBV	1939718	2800852	82.54%	7.431%
22	15.569	2115	2122	2137	rVV	418087	632053	18.63%	1.677%
23	15.675	2137	2140	2145	rVB3	8214	14430	0.43%	0.038%
24	16.004	2193	2196	2202	rVB8	2807	4957	0.15%	0.013%
25	16.228	2231	2234	2239	rVB6	6071	8408	0.25%	0.022%
26	16.869	2341	2343	2348	rVB6	3419	3925	0.12%	0.010%
27	16.986	2359	2363	2367	rBV4	3161	5523	0.16%	0.015%
28	17.198	2392	2399	2406	rBV	1441231	2010345	59.25%	5.333%
29	17.298	2409	2416	2430	rVV	1962245	2884501	85.01%	7.653%
30	17.598	2466	2467	2471	rBV4	3237	3627	0.11%	0.010%
31	19.116	2721	2725	2729	rBV3	25938	34215	1.01%	0.091%
32	19.180	2733	2736	2741	rVV	21539	31096	0.92%	0.082%
33	19.533	2791	2796	2806	rBV	2428566	3249700	95.77%	8.621%
34	21.292	3090	3095	3104	rBV	1527003	2053525	60.52%	5.448%
35	23.492	3462	3469	3483	rVB	1715517	3393174	100.00%	9.002%
36	23.645	3489	3495	3506	rVB	1080102	2226315	65.61%	5.906%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019089.D
Acq On : 26 Dec 2023 18:54
Operator : MA/JU
Sample : PB158028BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK028

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 37692988

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019089.D
Acq On : 26 Dec 2023 18:54
Operator : MA/JU
Sample : PB158028BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK028

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

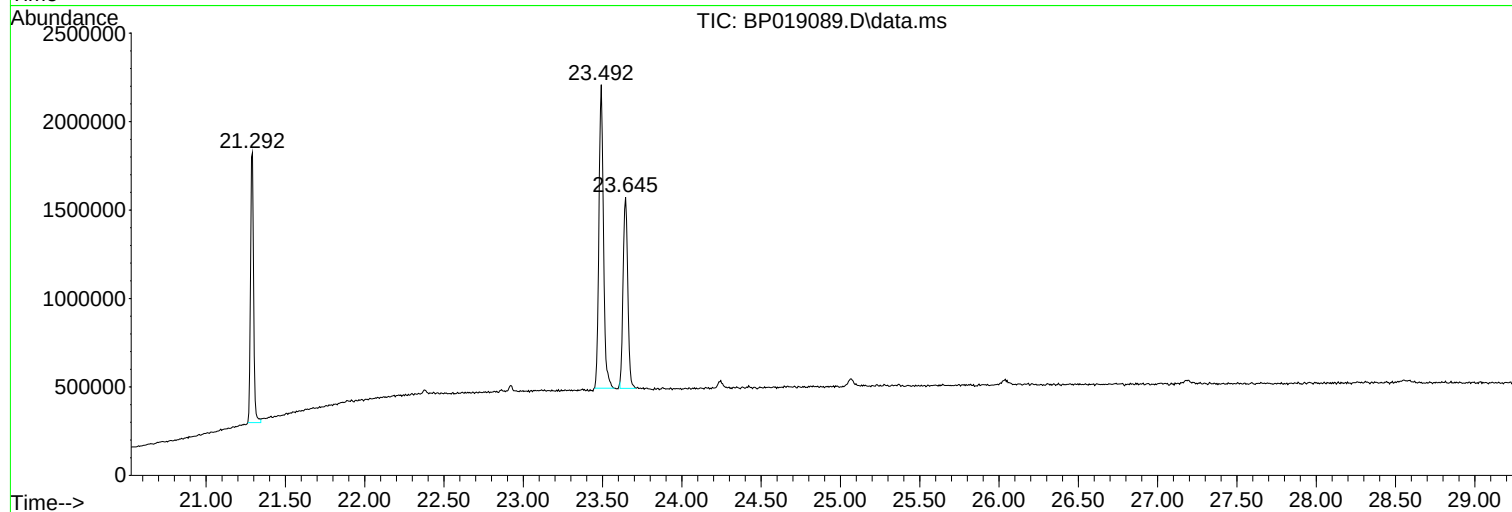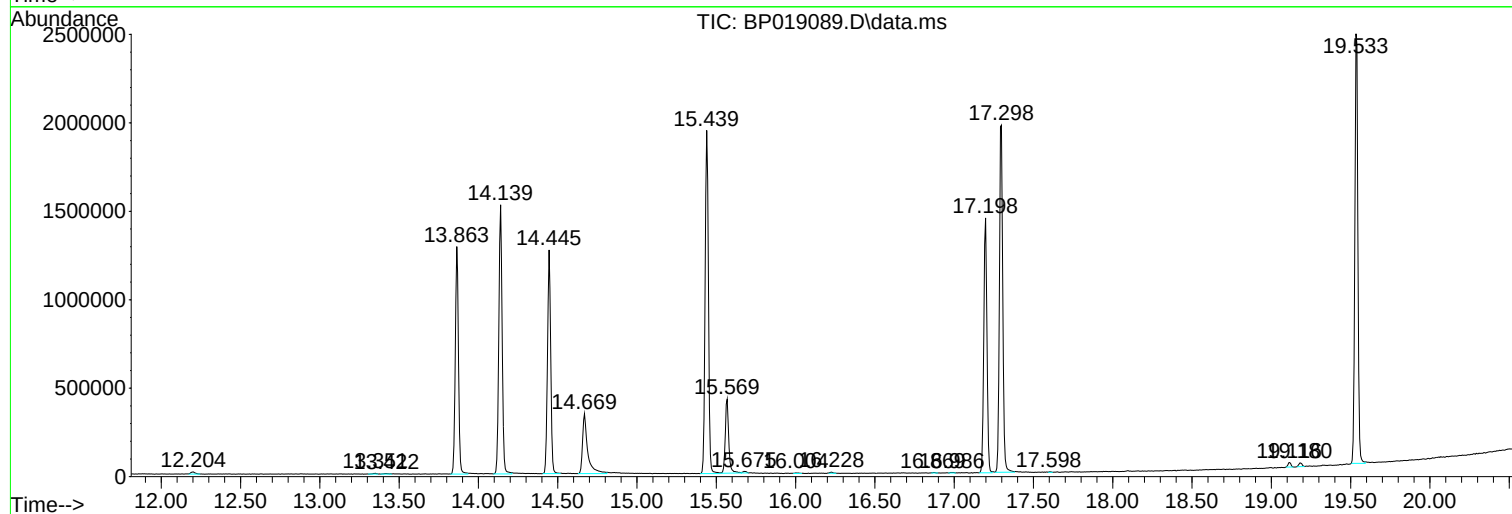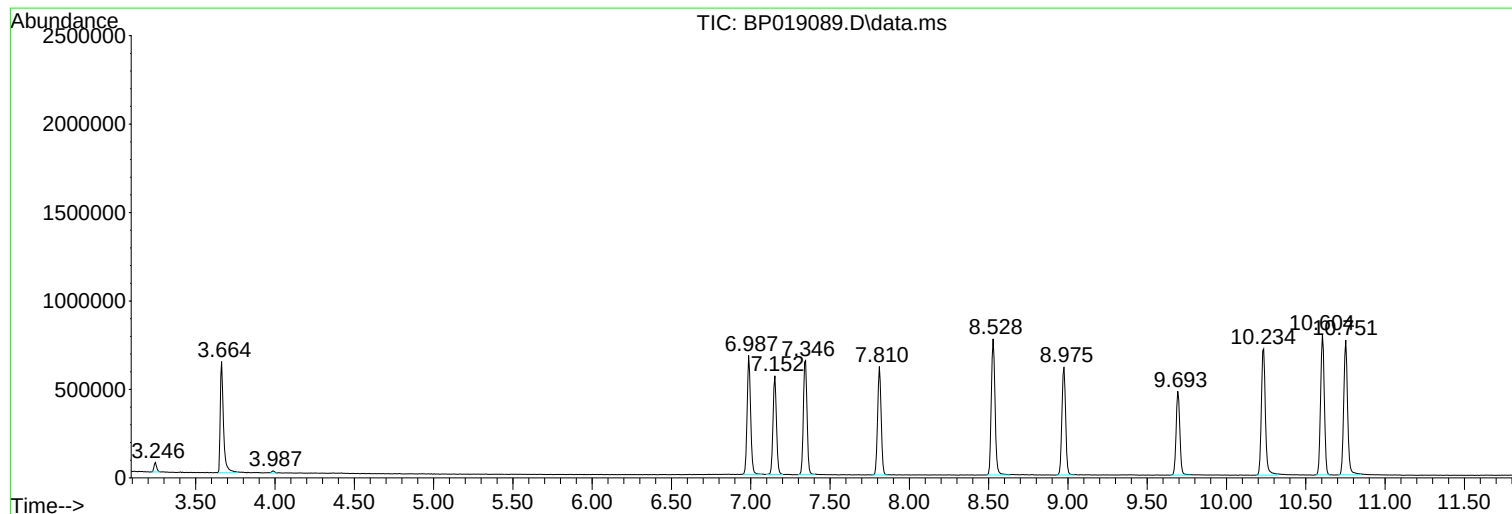

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019089.D
Acq On : 26 Dec 2023 18:54
Operator : MA/JU
Sample : PB158028BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK028

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019089.D
Acq On : 26 Dec 2023 18:54
Operator : MA/JU
Sample : PB158028BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK028

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc