

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019090.D
 Acq On : 26 Dec 2023 19:28
 Operator : MA/JU
 Sample : PB158031BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK031

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	36	rBV	49887	65751	1.77%	0.194%
2	3.664	94	98	112	rBV	590191	834558	22.41%	2.457%
3	3.987	150	153	159	rVB	9187	12241	0.33%	0.036%
4	6.987	657	663	677	rVB	618296	946689	25.42%	2.787%
5	7.152	684	691	704	rVB	510274	785772	21.10%	2.313%
6	7.340	716	723	733	rBV	609235	967124	25.97%	2.847%
7	7.810	796	803	812	rVV	509236	781528	20.99%	2.301%
8	8.528	918	925	940	rBV	711985	1146217	30.78%	3.375%
9	8.975	993	1001	1011	rBV	544412	895012	24.03%	2.635%
10	9.693	1116	1123	1137	rBV	433128	702147	18.85%	2.067%
11	10.234	1206	1215	1226	rBV	633173	1125790	30.23%	3.314%
12	10.604	1270	1278	1291	rVB	635403	1048148	28.15%	3.086%
13	10.751	1296	1303	1320	rBV	643830	1146731	30.79%	3.376%
14	12.198	1542	1549	1555	rBV2	10750	20092	0.54%	0.059%
15	13.357	1741	1746	1754	rVV2	3106	7289	0.20%	0.021%
16	13.428	1754	1758	1762	rVB7	2160	3726	0.10%	0.011%
17	13.863	1825	1832	1847	rBV	1089645	1554611	41.74%	4.577%
18	14.139	1872	1879	1892	rBV	1317386	1942796	52.17%	5.720%
19	14.445	1924	1931	1940	rBV	914069	1351642	36.29%	3.979%
20	14.669	1962	1969	1989	rBV	279655	664174	17.83%	1.955%
21	15.439	2090	2100	2113	rBV	1692240	2448686	65.75%	7.209%
22	15.563	2115	2121	2133	rBV	356432	555092	14.91%	1.634%
23	15.675	2138	2140	2146	rVB5	9095	14800	0.40%	0.044%
24	16.222	2228	2233	2238	rBV7	6830	11476	0.31%	0.034%
25	17.198	2392	2399	2409	rBV	1076321	1566233	42.06%	4.611%
26	17.298	2409	2416	2432	rVV	1745589	2559040	68.72%	7.534%
27	18.092	2549	2551	2556	rBV6	3118	4403	0.12%	0.013%
28	19.116	2721	2725	2730	rBV2	23483	32448	0.87%	0.096%
29	19.180	2733	2736	2740	rVV	20105	23946	0.64%	0.070%
30	19.533	2790	2796	2807	rBV	2227003	3077915	82.65%	9.062%
31	21.286	3090	3094	3103	rBV	1375880	1799927	48.33%	5.299%
32	23.492	3462	3469	3485	rVB2	1802997	3724087	100.00%	10.964%
33	23.639	3488	3494	3508	rVB	1043479	2146752	57.65%	6.320%




Sum of corrected areas: 33966843

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019090.D
Acq On : 26 Dec 2023 19:28
Operator : MA/JU
Sample : PB158031BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK031

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

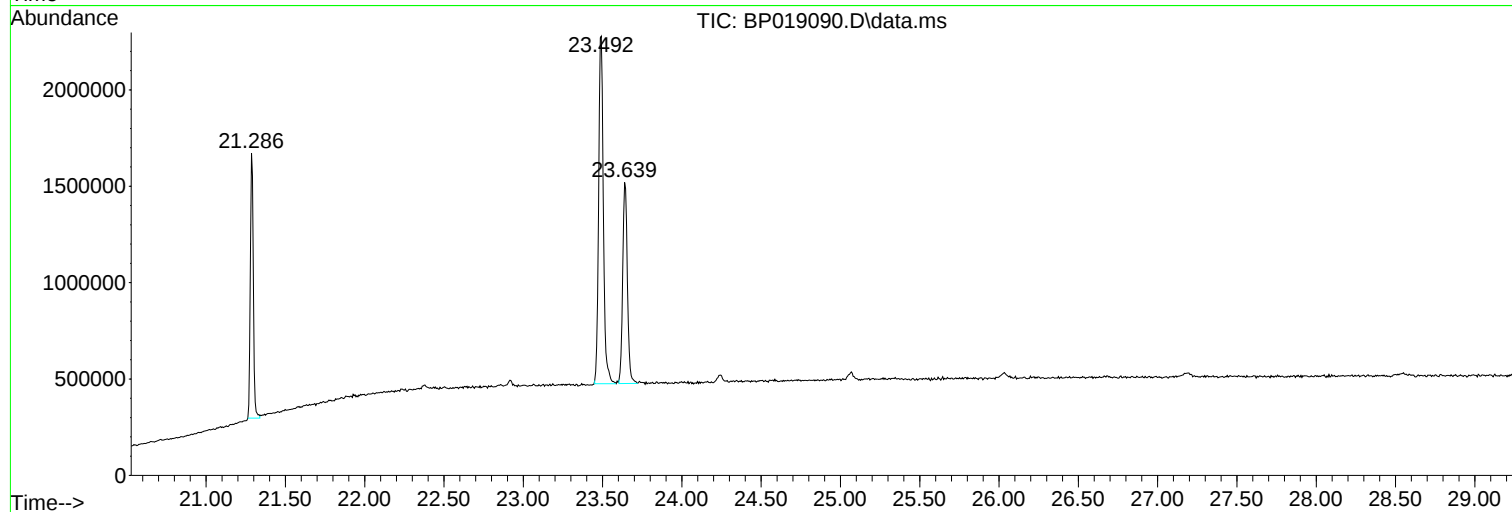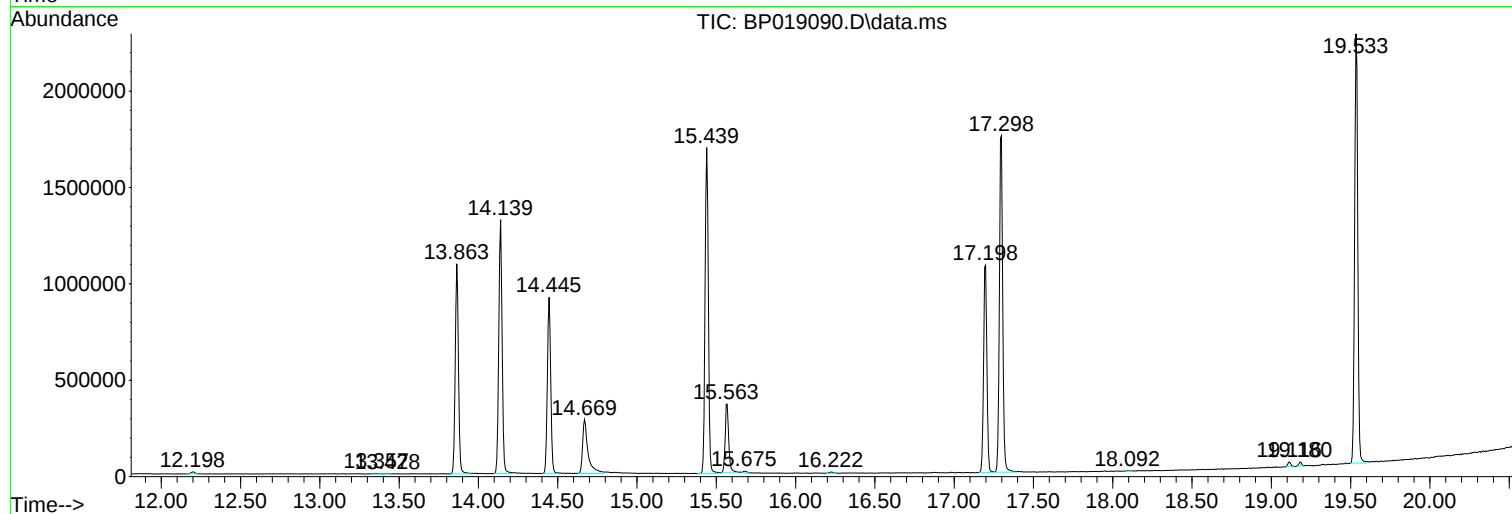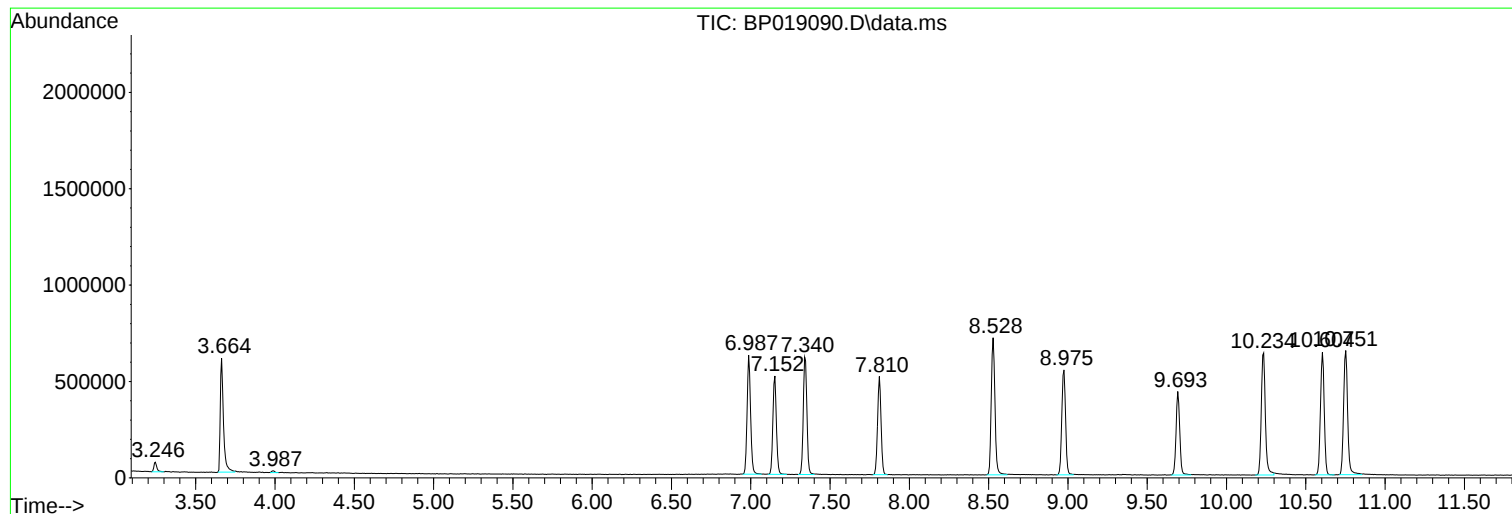

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019090.D
Acq On : 26 Dec 2023 19:28
Operator : MA/JU
Sample : PB158031BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK031

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019090.D
Acq On : 26 Dec 2023 19:28
Operator : MA/JU
Sample : PB158031BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK031

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------