

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019091.D
 Acq On : 26 Dec 2023 20:02
 Operator : MA/JU
 Sample : 05976-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7W0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	18	21	24	rBV3	11971	14215	0.32%	0.045%
2	3.246	24	27	34	rVB	32510	40050	0.90%	0.127%
3	3.669	95	99	115	rBV	148858	225554	5.07%	0.715%
4	3.987	150	153	160	rVB	9017	13407	0.30%	0.042%
5	4.434	226	229	238	rVB7	7943	14685	0.33%	0.047%
6	6.940	653	655	658	rBV4	4977	5618	0.13%	0.018%
7	6.987	658	663	671	rVB	91450	147985	3.33%	0.469%
8	7.152	684	691	704	rVB	429491	670978	15.08%	2.126%
9	7.340	717	723	734	rBV	376914	610003	13.71%	1.932%
10	7.810	795	803	812	rBV	492536	766394	17.23%	2.428%
11	8.528	918	925	936	rBV	267737	448043	10.07%	1.419%
12	8.975	991	1001	1011	rBV	466416	770021	17.31%	2.439%
13	9.381	1064	1070	1077	rVB	23880	38075	0.86%	0.121%
14	9.693	1116	1123	1133	rBV	344377	559188	12.57%	1.771%
15	10.234	1208	1215	1228	rBV	474545	856600	19.25%	2.714%
16	10.604	1271	1278	1288	rBV	609993	1009613	22.69%	3.198%
17	10.751	1295	1303	1316	rBV	457910	831304	18.69%	2.633%
18	11.875	1489	1494	1499	rVB2	13104	20383	0.46%	0.065%
19	12.198	1543	1549	1555	rBV3	10333	19810	0.45%	0.063%
20	13.275	1728	1732	1738	rVB9	3050	5968	0.13%	0.019%
21	13.345	1738	1744	1749	rBV5	10248	17990	0.40%	0.057%
22	13.863	1825	1832	1842	rBV	1005982	1394165	31.34%	4.417%
23	14.140	1872	1879	1896	rBV	1148785	1706552	38.36%	5.406%
24	14.445	1923	1931	1944	rBV	909482	1324160	29.76%	4.195%
25	14.681	1963	1971	1988	rBV2	35283	108634	2.44%	0.344%
26	15.439	2093	2100	2108	rBV	1593076	2259494	50.79%	7.158%
27	15.569	2115	2122	2135	rBV	387963	602270	13.54%	1.908%
28	15.675	2138	2140	2150	rVB6	9076	16511	0.37%	0.052%
29	16.228	2230	2234	2240	rBV8	5315	8289	0.19%	0.026%
30	16.610	2294	2299	2303	rBV8	3817	8243	0.19%	0.026%
31	17.010	2363	2367	2372	rVB3	11413	16169	0.36%	0.051%
32	17.198	2392	2399	2409	rBV	1101130	1590006	35.74%	5.037%
33	17.292	2409	2415	2428	rBV2	1925137	2802050	62.98%	8.877%
34	18.086	2546	2550	2559	rBV2	66748	99569	2.24%	0.315%
35	19.116	2721	2725	2730	rBV3	26312	35455	0.80%	0.112%
36	19.180	2733	2736	2740	rBV	25393	35841	0.81%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019091.D
Acq On : 26 Dec 2023 20:02
Operator : MA/JU
Sample : 05976-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.327	2757	2761	2765	rBV2	31670	43427	0.98%	0.138%
38	19.533	2790	2796	2811	rBV	2636863	3635591	81.72%	11.517%
39	21.286	3090	3094	3101	rBV	1543962	1978004	44.46%	6.266%
40	23.492	3462	3469	3485	rVB2	2223172	4448994	100.00%	14.094%
41	23.645	3489	3495	3506	rVB	1169937	2367304	53.21%	7.499%




Sum of corrected areas: 31566612

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019091.D
Acq On : 26 Dec 2023 20:02
Operator : MA/JU
Sample : 05976-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

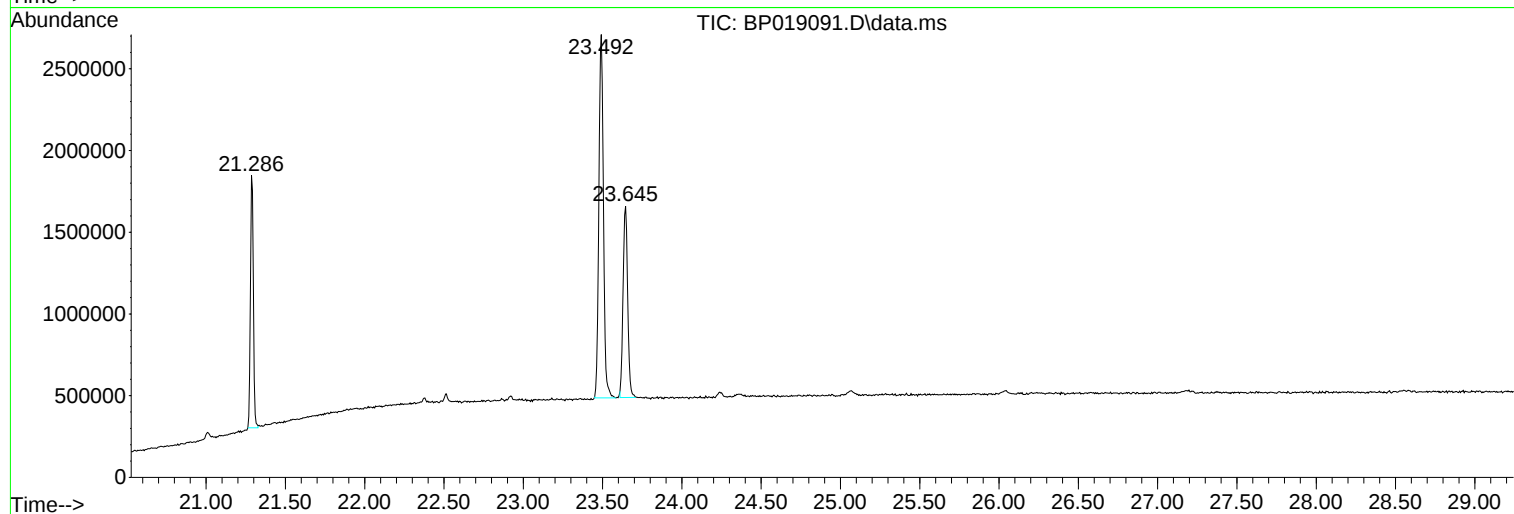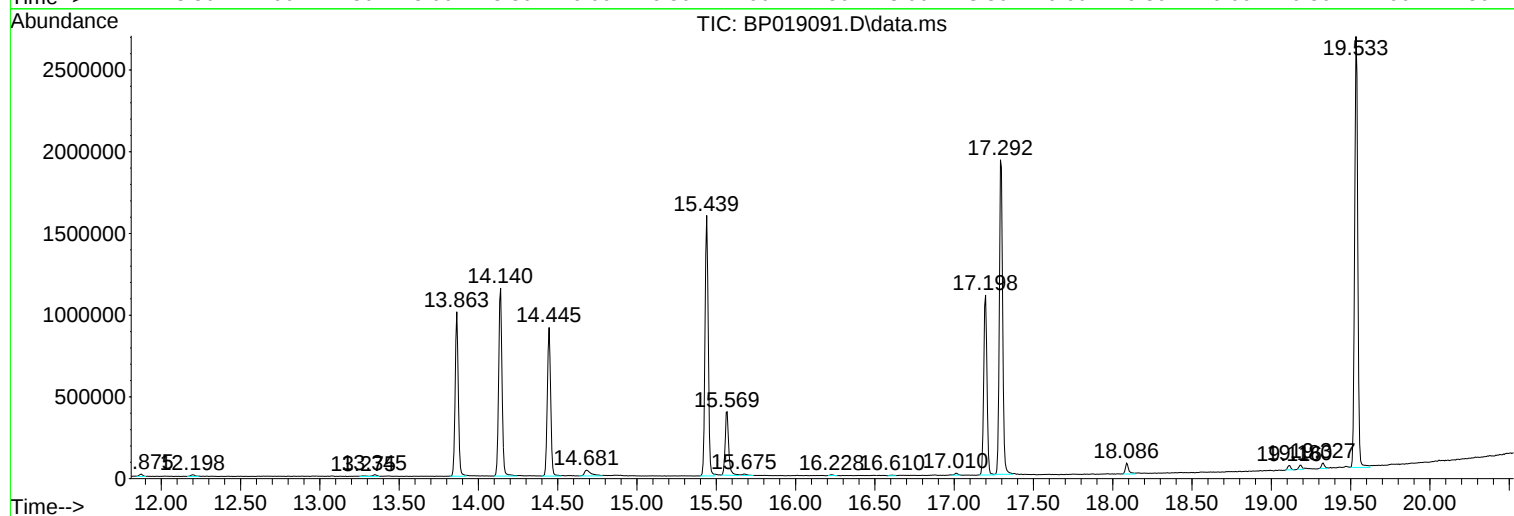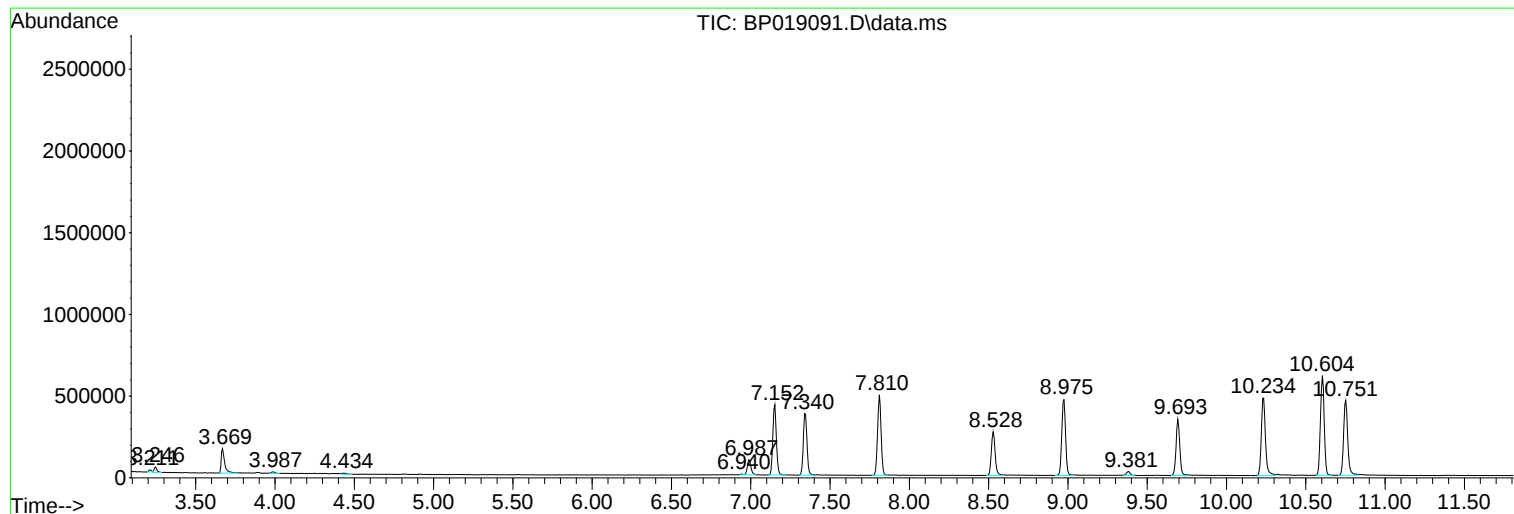

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019091.D
Acq On : 26 Dec 2023 20:02
Operator : MA/JU
Sample : 05976-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019091.D
Acq On : 26 Dec 2023 20:02
Operator : MA/JU
Sample : 05976-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------