

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019092.D
 Acq On : 26 Dec 2023 20:36
 Operator : MA/JU
 Sample : 05976-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7W1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	24	rBV4	12919	17641	0.30%	0.038%
2	3.246	24	27	31	rVB	32861	37133	0.64%	0.080%
3	3.670	96	99	110	rBV	70398	114993	1.99%	0.249%
4	3.987	149	153	159	rVB2	12067	18756	0.32%	0.041%
5	4.434	226	229	234	rVB6	5576	7388	0.13%	0.016%
6	6.946	650	656	658	rBV2	7070	10631	0.18%	0.023%
7	6.987	658	663	674	rVB	124471	197243	3.41%	0.427%
8	7.152	684	691	701	rBV	515671	799501	13.82%	1.733%
9	7.340	717	723	732	rBV	465726	756946	13.08%	1.640%
10	7.811	796	803	812	rBV	512622	802600	13.87%	1.739%
11	8.528	916	925	937	rBV	360273	583093	10.08%	1.264%
12	8.975	993	1001	1012	rBV	565601	931651	16.10%	2.019%
13	9.381	1064	1070	1076	rVB	27956	44995	0.78%	0.098%
14	9.693	1115	1123	1137	rBV	436022	711411	12.29%	1.542%
15	10.234	1204	1215	1229	rBV	607827	1089594	18.83%	2.361%
16	10.605	1271	1278	1287	rVB	679363	1104829	19.09%	2.394%
17	10.752	1294	1303	1321	rBV	445537	785279	13.57%	1.702%
18	11.869	1486	1493	1499	rBV2	12247	21315	0.37%	0.046%
19	12.199	1543	1549	1553	rBV3	11434	20169	0.35%	0.044%
20	13.075	1693	1698	1704	rVB2	6618	10945	0.19%	0.024%
21	13.346	1739	1744	1751	rBV6	8536	15451	0.27%	0.033%
22	13.863	1825	1832	1841	rBV	1409395	1916426	33.12%	4.153%
23	14.140	1871	1879	1893	rBV	1510588	2220526	38.37%	4.812%
24	14.251	1893	1898	1903	rVB4	6295	11025	0.19%	0.024%
25	14.445	1924	1931	1943	rBV	1041040	1552051	26.82%	3.364%
26	14.675	1965	1970	1984	rBV	66306	167572	2.90%	0.363%
27	15.440	2093	2100	2115	rBV	2094625	3045655	52.63%	6.601%
28	15.563	2115	2121	2135	rVV	613734	889484	15.37%	1.928%
29	15.675	2137	2140	2147	rVB3	9378	17643	0.30%	0.038%
30	16.134	2212	2218	2221	rBV8	3137	6293	0.11%	0.014%
31	16.228	2230	2234	2241	rVB6	8578	12338	0.21%	0.027%
32	17.016	2360	2368	2384	rBV	4183696	5787153	100.00%	12.542%
33	17.157	2388	2392	2393	rVV4	9504	11045	0.19%	0.024%
34	17.198	2393	2399	2409	rVB	1446759	2020790	34.92%	4.380%
35	17.298	2409	2416	2426	rBV	2550408	3772390	65.19%	8.176%
36	18.086	2545	2550	2555	rBV2	68774	95750	1.65%	0.208%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019092.D
Acq On : 26 Dec 2023 20:36
Operator : MA/JU
Sample : 05976-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.022	2705	2709	2713	rBV	54183	63392	1.10%	0.137%
38	19.110	2720	2724	2730	rBV3	41202	59818	1.03%	0.130%
39	19.181	2732	2736	2740	rBV	36233	53033	0.92%	0.115%
40	19.322	2757	2760	2766	rBV5	39910	57048	0.99%	0.124%
41	19.533	2790	2796	2807	rBV	3681580	4933240	85.24%	10.691%
42	21.286	3089	3094	3103	rBV	2086661	2653755	45.86%	5.751%
43	21.380	3107	3110	3114	rVV	130949	151040	2.61%	0.327%
44	23.492	3462	3469	3484	rVB	2950875	5681441	98.17%	12.313%
45	23.645	3488	3495	3505	rVB	1449639	2881395	49.79%	6.245%




Sum of corrected areas: 46141867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019092.D
Acq On : 26 Dec 2023 20:36
Operator : MA/JU
Sample : 05976-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

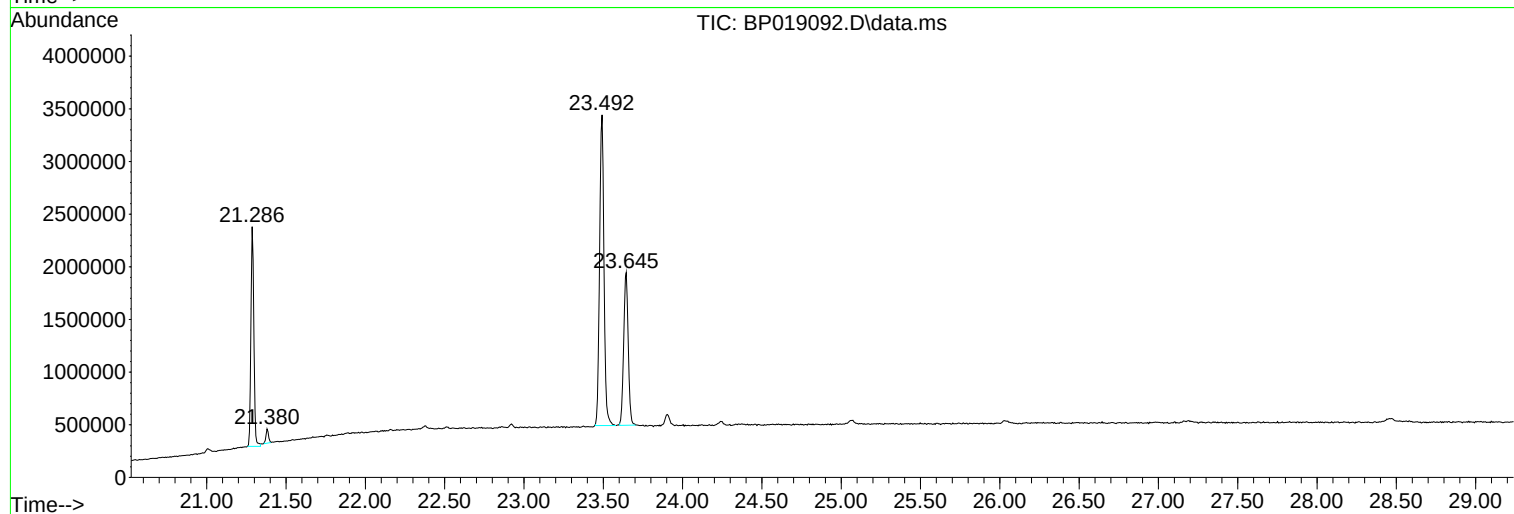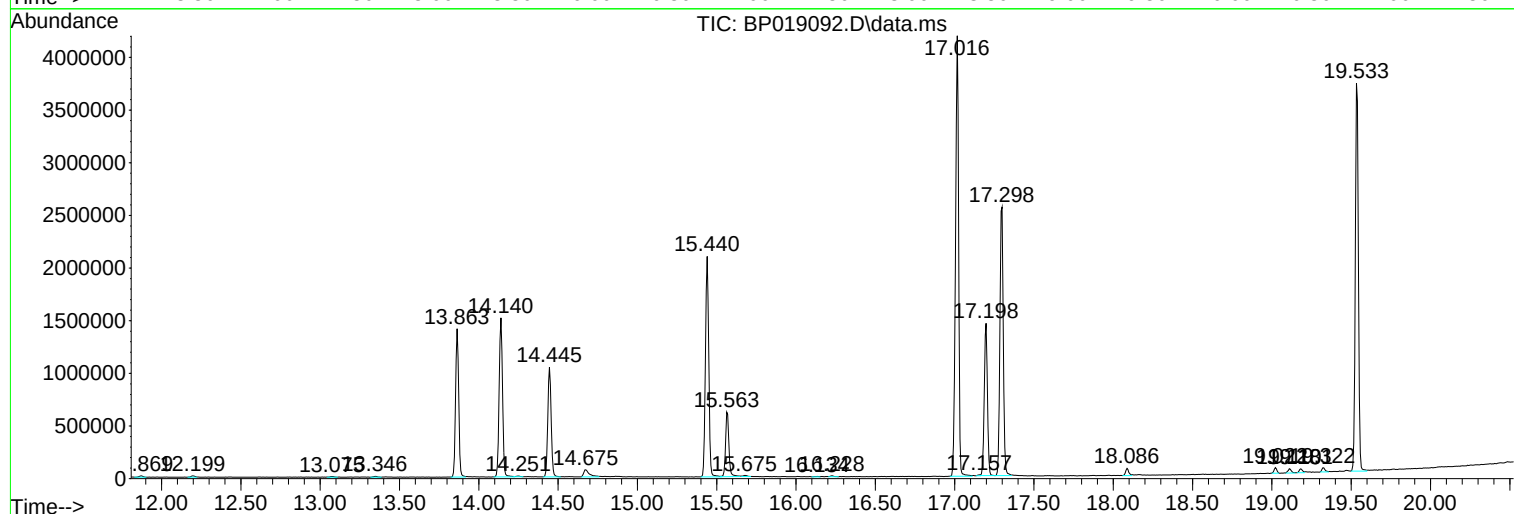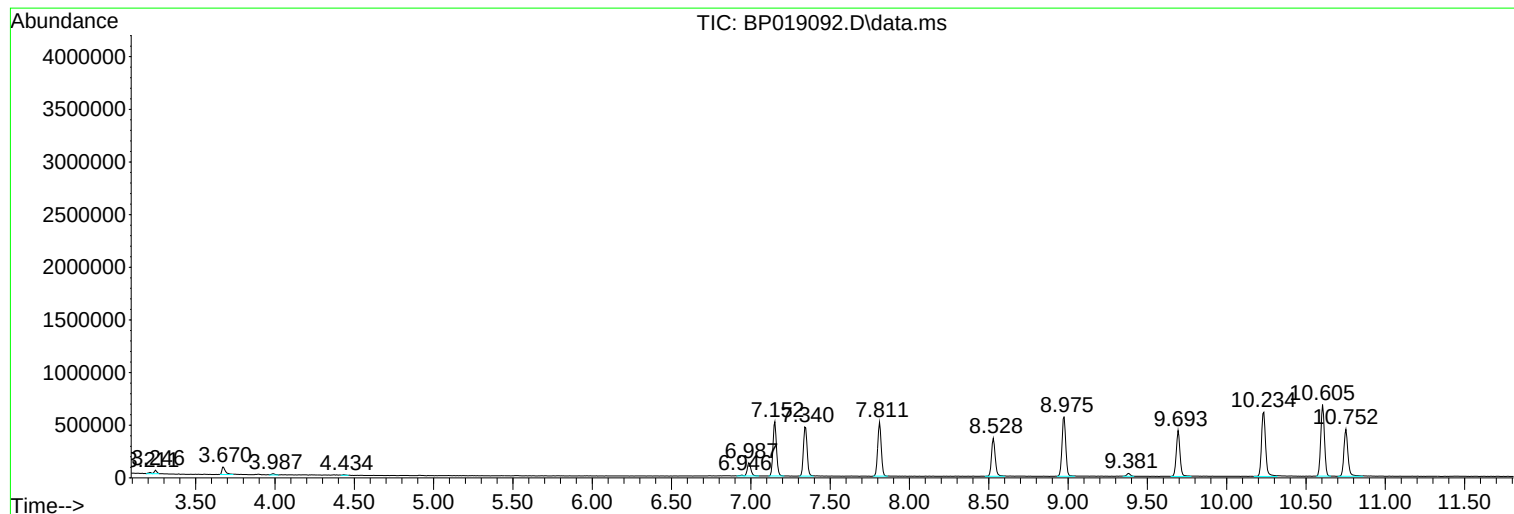

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019092.D
Acq On : 26 Dec 2023 20:36
Operator : MA/JU
Sample : 05976-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.016	57.28 ng/ul	5787150	Phenanthrene-d10	17.198

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	90
2			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	70
3			N-hexylbenzenesulfonamide	241	C12H19NO2S	007250-80-8	64
4			2-propenoic acid, 2-methyl-, 2-[...]	269	C12H15NO4S	1000401-71-8	64
5			N-Benzenesulfonyloxy-2,2-bis(tri...]	335	C10H7F6NO3S	055734-41-3	50

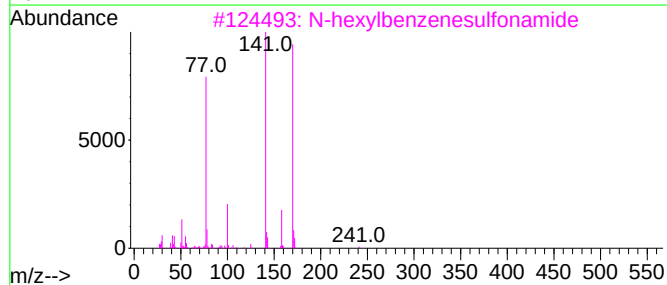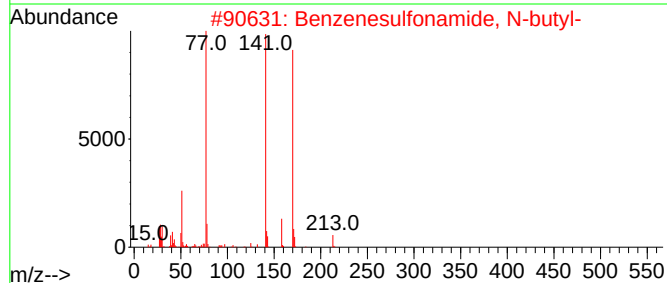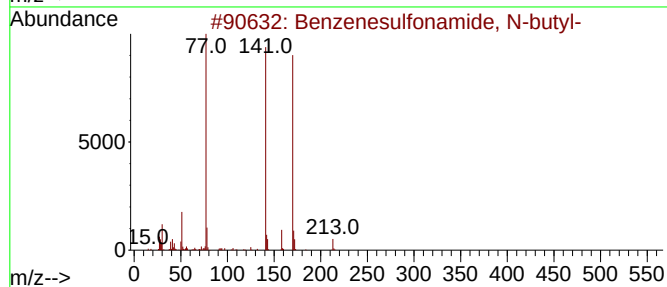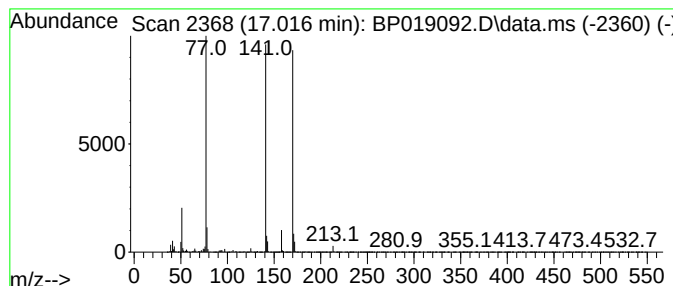

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019092.D
Acq On : 26 Dec 2023 20:36
Operator : MA/JU
Sample : 05976-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.016	57.3	ng/ul	5787150	4	17.198	2020790	20.0