

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019094.D
 Acq On : 26 Dec 2023 21:45
 Operator : MA/JU
 Sample : 05976-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7W3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	18	21	24	rBV2	16509	19589	0.32%	0.044%
2	3.246	24	27	37	rVB	34199	47776	0.78%	0.107%
3	3.670	96	99	116	rBV	112278	184077	3.01%	0.411%
4	3.987	150	153	159	rVB	9798	12620	0.21%	0.028%
5	6.987	657	663	673	rVB	98608	157386	2.58%	0.351%
6	7.152	681	691	702	rBV	488918	754525	12.35%	1.685%
7	7.340	716	723	734	rBV	418463	676348	11.07%	1.510%
8	7.811	796	803	812	rBV	481323	748421	12.25%	1.671%
9	8.528	918	925	938	rBV	300191	490139	8.02%	1.095%
10	8.975	992	1001	1012	rBV	528177	872981	14.29%	1.950%
11	9.381	1066	1070	1076	rVB6	4781	8135	0.13%	0.018%
12	9.693	1116	1123	1131	rBV	388733	632473	10.35%	1.412%
13	10.234	1207	1215	1227	rBV	554495	980972	16.06%	2.191%
14	10.605	1269	1278	1290	rBV	617198	1040483	17.03%	2.324%
15	10.752	1294	1303	1316	rBV	530983	925062	15.14%	2.066%
16	11.869	1489	1493	1499	rVB6	5038	7168	0.12%	0.016%
17	12.199	1542	1549	1555	rVB2	12071	20797	0.34%	0.046%
18	13.346	1739	1744	1749	rBV	16551	26530	0.43%	0.059%
19	13.863	1824	1832	1845	rBV	1386764	1872249	30.65%	4.181%
20	14.140	1870	1879	1888	rBV	1430549	2072595	33.92%	4.629%
21	14.446	1923	1931	1943	rBV	1003690	1473275	24.11%	3.290%
22	14.675	1963	1970	1985	rBV2	52657	145040	2.37%	0.324%
23	15.440	2093	2100	2112	rBV	1986472	2888906	47.29%	6.452%
24	15.563	2115	2121	2134	rVV	573843	859856	14.07%	1.920%
25	15.675	2137	2140	2147	rVB4	10011	17313	0.28%	0.039%
26	16.228	2228	2234	2238	rVB7	7773	11722	0.19%	0.026%
27	17.016	2360	2368	2383	rBV	4304599	6109418	100.00%	13.644%
28	17.198	2392	2399	2409	rVB	1290286	1889168	30.92%	4.219%
29	17.292	2409	2415	2429	rBV2	2537795	3661853	59.94%	8.178%
30	18.087	2546	2550	2556	rBV	82012	104124	1.70%	0.233%
31	19.022	2706	2709	2714	rVB3	18249	20590	0.34%	0.046%
32	19.110	2718	2724	2730	rBV3	44712	82766	1.35%	0.185%
33	19.181	2732	2736	2741	rBV	37216	56424	0.92%	0.126%
34	19.322	2757	2760	2767	rBV2	53547	71462	1.17%	0.160%
35	19.534	2790	2796	2804	rBV	3760130	4893203	80.09%	10.928%
36	21.286	3089	3094	3102	rBV	1928446	2451964	40.13%	5.476%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019094.D
Acq On : 26 Dec 2023 21:45
Operator : MA/JU
Sample : 05976-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.492	3461	3469	3481	rBV	2743174	5718427	93.60%	12.771%
38	23.645	3488	3495	3508	rVB	1356583	2771864	45.37%	6.190%




Sum of corrected areas: 44777701

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019094.D
Acq On : 26 Dec 2023 21:45
Operator : MA/JU
Sample : 05976-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

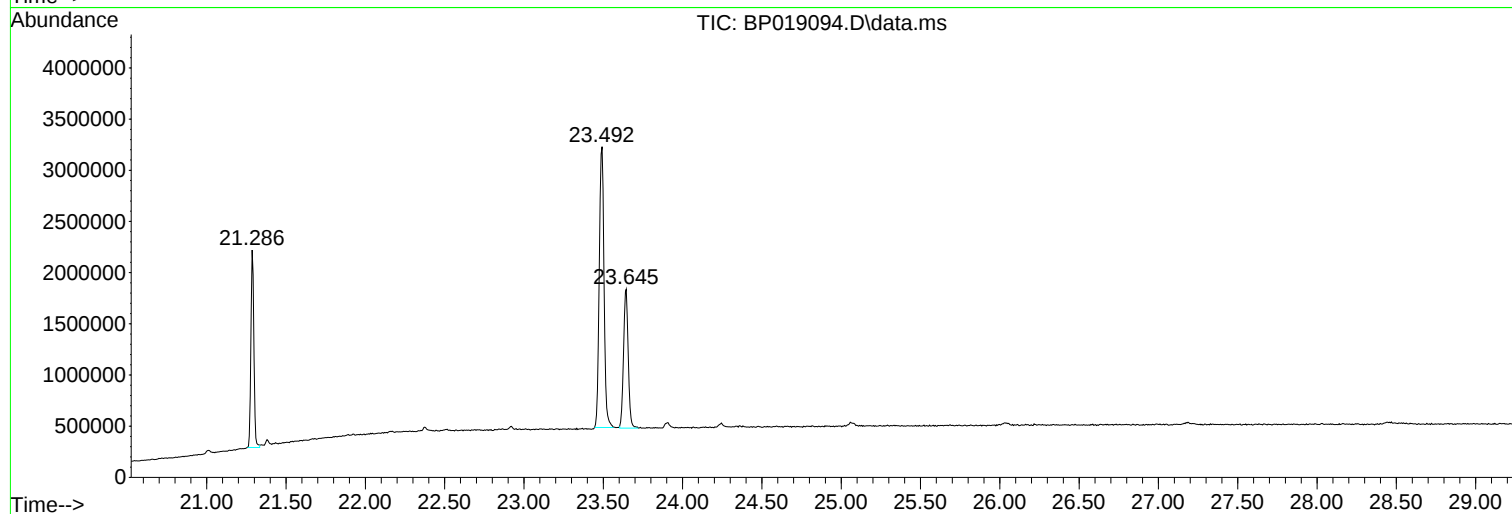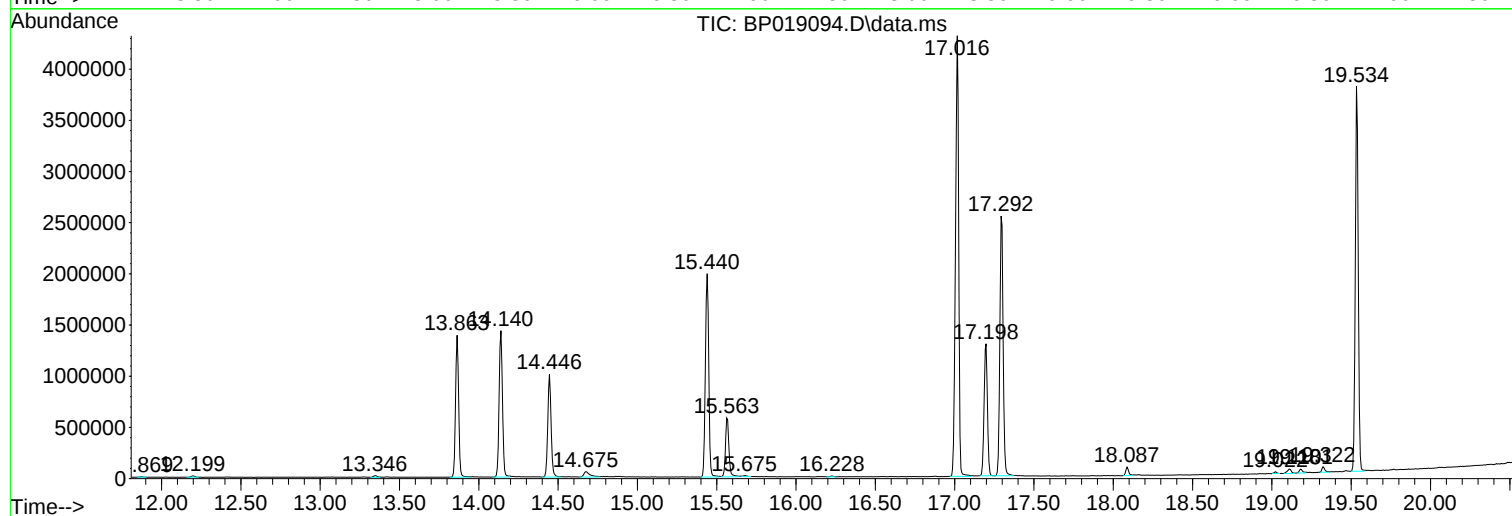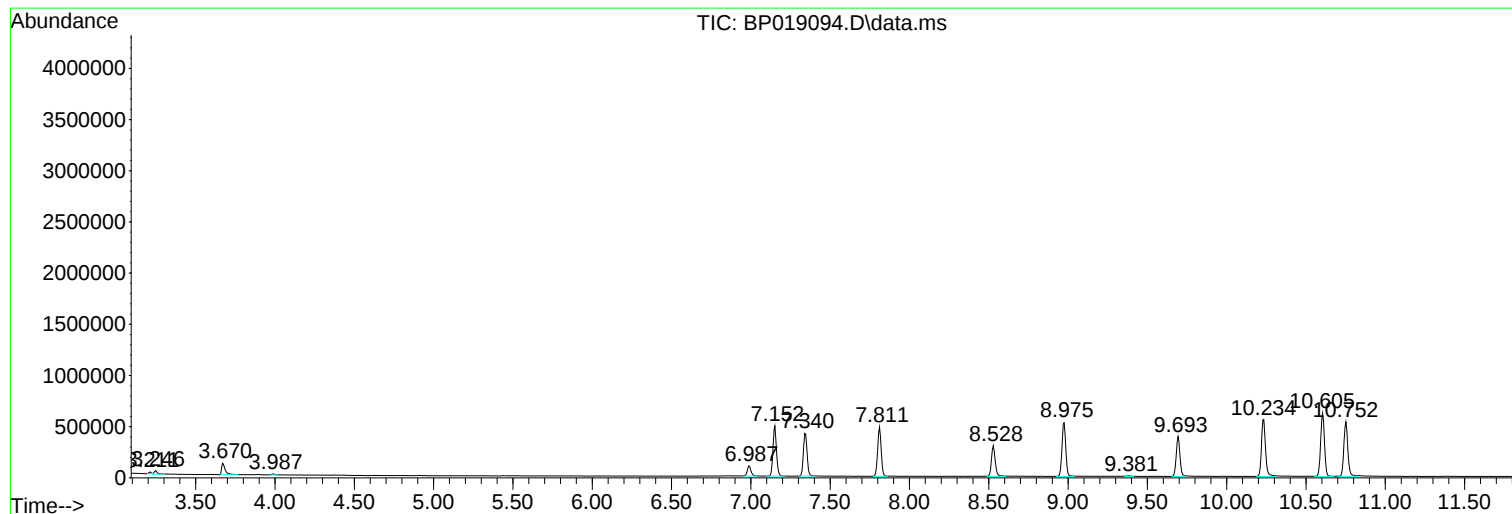

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019094.D
Acq On : 26 Dec 2023 21:45
Operator : MA/JU
Sample : 05976-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.016	64.68 ng/ul	6109420	Phenanthrene-d10	17.198

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	90
2			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	70
3			2-propenoic acid, 2-methyl-, 2-[...]	269	C12H15NO4S	1000401-71-8	64
4			N-hexylbenzenesulfonamide	241	C12H19NO2S	007250-80-8	64
5			N-Benzenesulfonyloxy-2,2-bis(tri...]	335	C10H7F6NO3S	055734-41-3	50

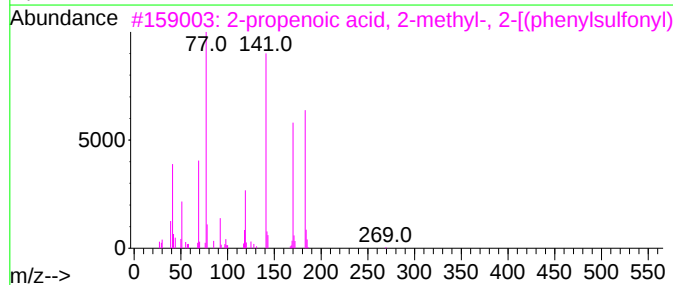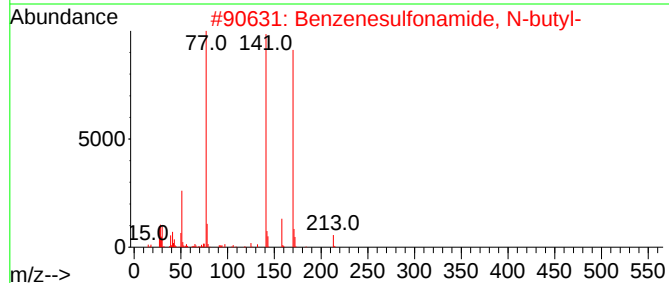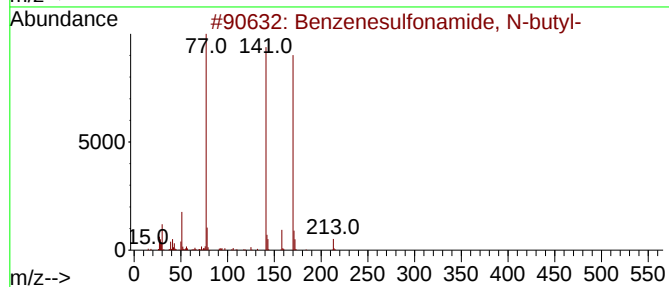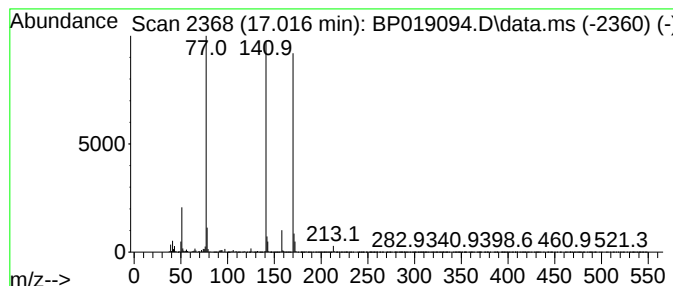

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019094.D
Acq On : 26 Dec 2023 21:45
Operator : MA/JU
Sample : 05976-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.016	64.7	ng/ul	6109420	4	17.198	1889170	20.0