

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019097.D
 Acq On : 26 Dec 2023 23:26
 Operator : MA/JU
 Sample : 05976-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	35	rVB	28232	38374	0.64%	0.091%
2	3.670	95	99	112	rBV	111121	175690	2.95%	0.416%
3	3.893	134	137	144	rVB2	6290	9704	0.16%	0.023%
4	3.993	150	154	162	rVB3	10286	16562	0.28%	0.039%
5	6.987	658	663	673	rVB	99143	161972	2.72%	0.384%
6	7.152	682	691	705	rBV	540269	844487	14.17%	2.001%
7	7.340	716	723	733	rBV	450073	728619	12.23%	1.726%
8	7.810	796	803	812	rBV	559768	868823	14.58%	2.058%
9	8.528	919	925	935	rBV	314560	508790	8.54%	1.205%
10	8.975	993	1001	1010	rBV	592538	980224	16.45%	2.322%
11	9.381	1063	1070	1076	rVB4	7070	14483	0.24%	0.034%
12	9.552	1093	1099	1105	rBV5	6144	10847	0.18%	0.026%
13	9.693	1112	1123	1135	rBV	448035	734318	12.32%	1.740%
14	10.228	1207	1214	1238	rBV	623588	1119025	18.78%	2.651%
15	10.604	1270	1278	1285	rBV	725614	1204622	20.22%	2.854%
16	10.752	1294	1303	1316	rBV	566890	985745	16.54%	2.335%
17	11.375	1404	1409	1415	rBV6	4024	8892	0.15%	0.021%
18	12.198	1544	1549	1555	rVB	13452	21768	0.37%	0.052%
19	13.269	1727	1731	1735	rVB5	5130	6559	0.11%	0.016%
20	13.345	1740	1744	1748	rBV7	5030	8281	0.14%	0.020%
21	13.863	1825	1832	1847	rBV	1442501	2000273	33.57%	4.739%
22	14.140	1869	1879	1893	rBV	1624496	2385788	40.04%	5.652%
23	14.445	1924	1931	1947	rBV	1160622	1688572	28.34%	4.000%
24	14.681	1965	1971	1983	rBV3	43584	112227	1.88%	0.266%
25	14.869	1997	2003	2010	rVB3	7052	15721	0.26%	0.037%
26	15.440	2093	2100	2115	rBV	2268187	3251768	54.57%	7.703%
27	15.563	2115	2121	2136	rVV	604417	917268	15.39%	2.173%
28	15.681	2136	2141	2147	rVB	12181	23887	0.40%	0.057%
29	16.222	2229	2233	2243	rBV7	8400	13832	0.23%	0.033%
30	16.875	2339	2344	2349	rBV8	4219	8297	0.14%	0.020%
31	17.010	2363	2367	2373	rVB4	11839	17941	0.30%	0.043%
32	17.192	2391	2398	2408	rBV	1521386	2134142	35.82%	5.056%
33	17.292	2409	2415	2438	rVB	2774329	3976187	66.73%	9.420%
34	17.963	2526	2529	2536	rVB8	5925	7992	0.13%	0.019%
35	18.086	2545	2550	2558	rBV2	88198	127379	2.14%	0.302%
36	19.110	2720	2724	2729	rBV3	42778	59172	0.99%	0.140%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019097.D
Acq On : 26 Dec 2023 23:26
Operator : MA/JU
Sample : 05976-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.180	2732	2736	2740	rBV	39097	51293	0.86%	0.122%
38	19.322	2756	2760	2765	rBV2	46310	70735	1.19%	0.168%
39	19.533	2790	2796	2803	rBV	3975226	5186798	87.05%	12.287%
40	19.763	2832	2835	2839	rBV4	20126	27637	0.46%	0.065%
41	21.286	3089	3094	3104	rBV	2184201	2745351	46.07%	6.504%
42	23.492	3462	3469	3482	rVB2	3058313	5958455	100.00%	14.116%
43	23.639	3488	3494	3505	rVB	1454915	2983629	50.07%	7.068%




Sum of corrected areas: 42212129

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019097.D
Acq On : 26 Dec 2023 23:26
Operator : MA/JU
Sample : 05976-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

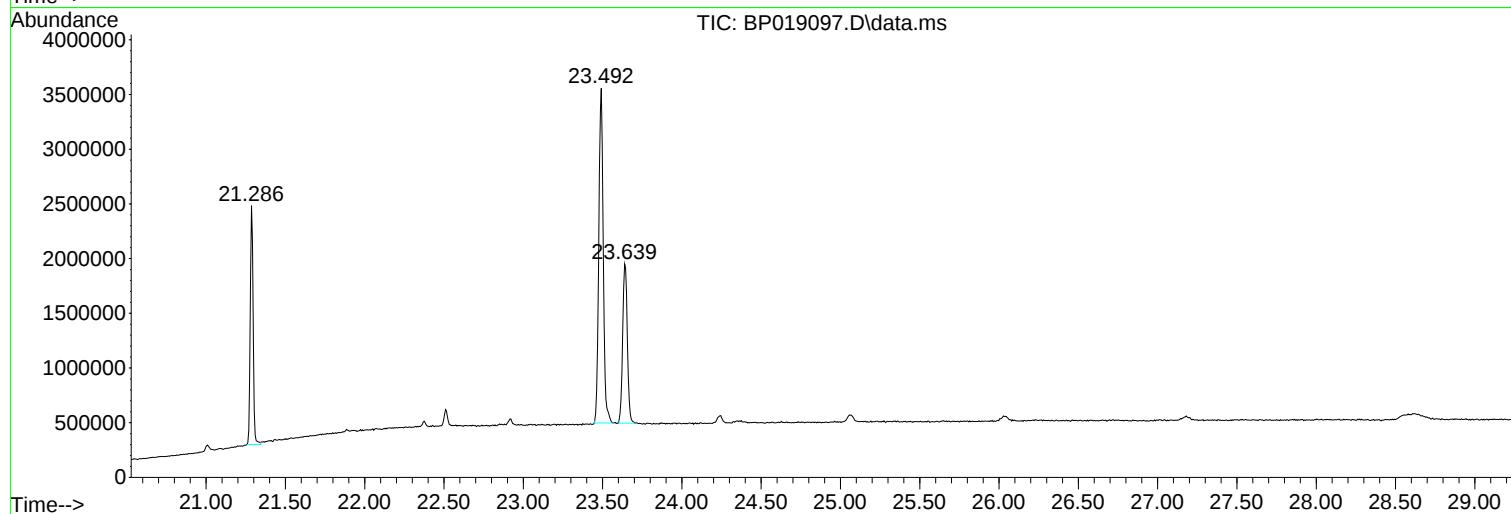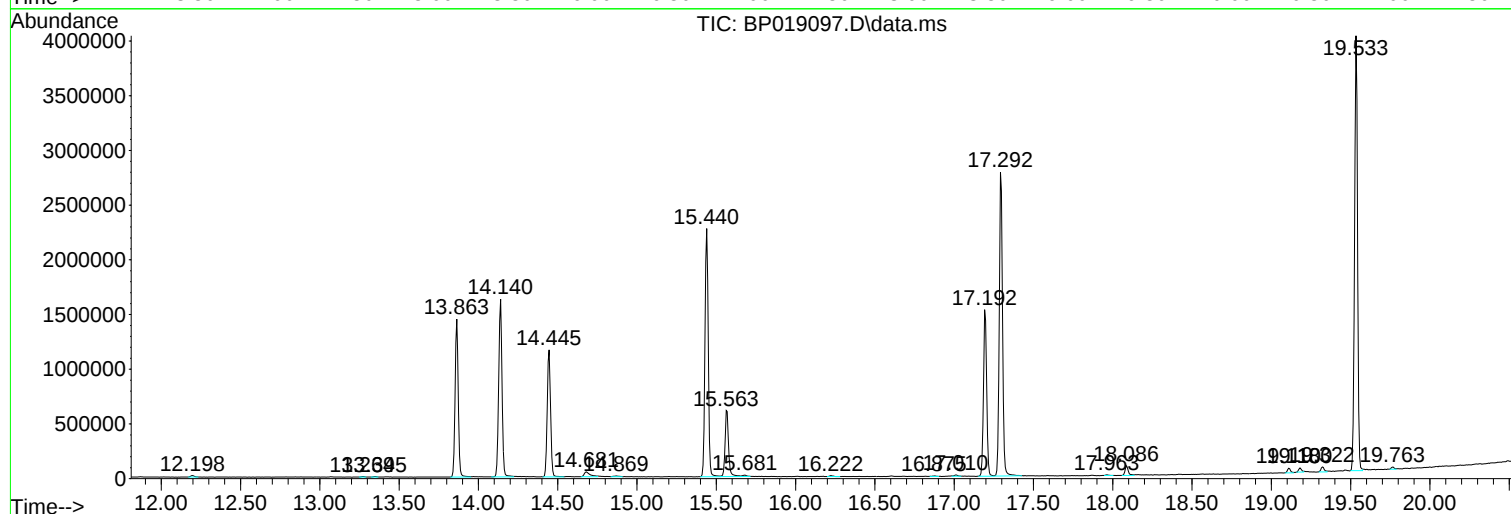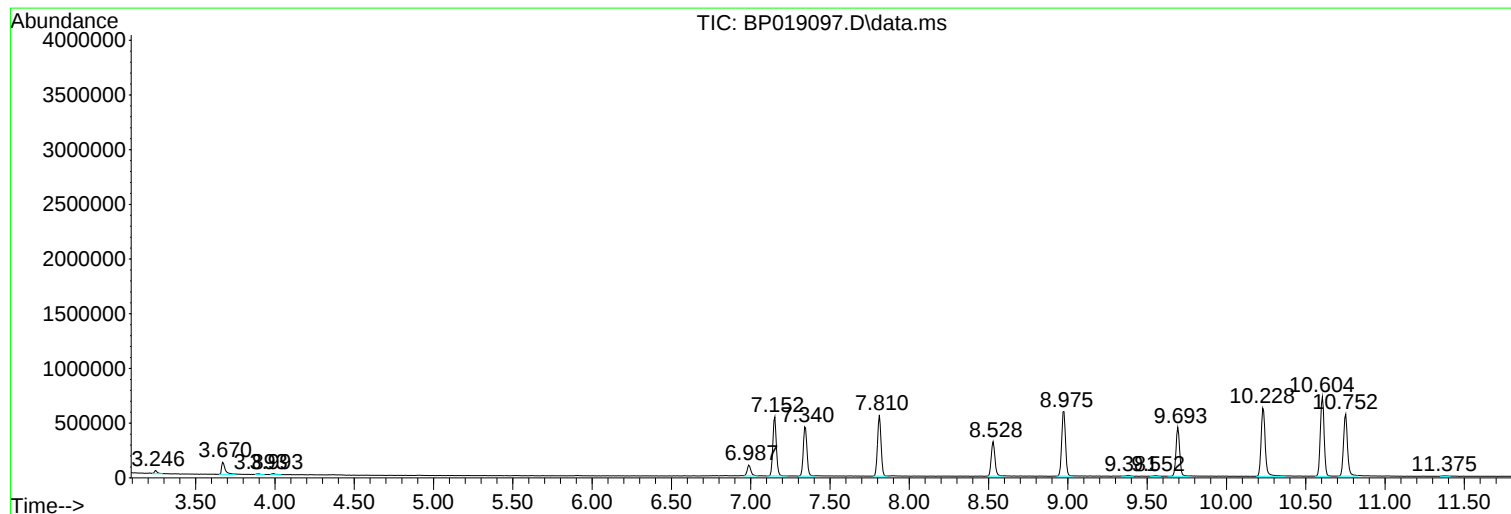

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019097.D
Acq On : 26 Dec 2023 23:26
Operator : MA/JU
Sample : 05976-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019097.D
Acq On : 26 Dec 2023 23:26
Operator : MA/JU
Sample : 05976-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc