

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019098.D
 Acq On : 27 Dec 2023 00:00
 Operator : MA/JU
 Sample : 05976-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	35	rVB	33821	45384	0.99%	0.138%
2	3.669	96	99	115	rBV	103317	164183	3.59%	0.501%
3	3.987	149	153	158	rVB	11698	16375	0.36%	0.050%
4	4.422	225	227	232	rVB6	3901	4743	0.10%	0.014%
5	6.987	658	663	672	rVB	84203	135068	2.95%	0.412%
6	7.152	683	691	702	rBV	466511	731688	15.98%	2.231%
7	7.340	716	723	733	rBV	392217	635309	13.87%	1.937%
8	7.810	795	803	812	rBV	576877	876010	19.13%	2.671%
9	8.528	918	925	936	rBV	262937	428179	9.35%	1.306%
10	8.975	992	1001	1015	rBV	494637	819104	17.89%	2.498%
11	9.381	1065	1070	1075	rVB7	6691	11351	0.25%	0.035%
12	9.557	1095	1100	1102	rBV5	3373	4861	0.11%	0.015%
13	9.693	1116	1123	1131	rBV	370034	588821	12.86%	1.795%
14	10.234	1205	1215	1232	rBV	501398	919376	20.08%	2.803%
15	10.604	1268	1278	1289	rBV	684161	1125792	24.59%	3.433%
16	10.751	1295	1303	1320	rBV	470955	854395	18.66%	2.605%
17	11.875	1488	1494	1500	rVB10	3955	9063	0.20%	0.028%
18	12.198	1544	1549	1556	rBV5	10641	20736	0.45%	0.063%
19	13.263	1728	1730	1737	rVB8	3225	5340	0.12%	0.016%
20	13.345	1740	1744	1748	rBV5	4920	7718	0.17%	0.024%
21	13.863	1823	1832	1845	rBV	1036801	1462040	31.93%	4.458%
22	14.139	1870	1879	1893	rBV	1216471	1820879	39.77%	5.552%
23	14.445	1923	1931	1946	rBV	939754	1413162	30.86%	4.309%
24	14.686	1965	1972	1985	rBV2	25637	79583	1.74%	0.243%
25	15.439	2093	2100	2114	rBV	1658057	2405912	52.54%	7.336%
26	15.569	2116	2122	2132	rVV	393125	579564	12.66%	1.767%
27	15.681	2137	2141	2147	rVB4	8656	15394	0.34%	0.047%
28	16.222	2229	2233	2240	rVB6	5478	10550	0.23%	0.032%
29	17.016	2365	2368	2372	rVB5	4279	5670	0.12%	0.017%
30	17.198	2392	2399	2409	rBV	1131960	1662353	36.30%	5.069%
31	17.292	2409	2415	2434	rVV	1954366	2857228	62.40%	8.712%
32	18.086	2546	2550	2558	rBV2	53956	77441	1.69%	0.236%
33	19.110	2721	2724	2728	rVB	29675	33752	0.74%	0.103%
34	19.180	2732	2736	2743	rBV	26466	48807	1.07%	0.149%
35	19.322	2757	2760	2765	rBV6	25555	29638	0.65%	0.090%
36	19.533	2790	2796	2804	rBV	2926876	3648969	79.69%	11.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019098.D
Acq On : 27 Dec 2023 00:00
Operator : MA/JU
Sample : 05976-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	21.286	3089	3094	3103	rBV	1676095	2167945	47.34%	6.610%
38	23.492	3462	3469	3481	rVB	2184664	4579087	100.00%	13.962%
39	23.639	3488	3494	3504	rVB	1235176	2494800	54.48%	7.607%




Sum of corrected areas: 32796270

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019098.D
Acq On : 27 Dec 2023 00:00
Operator : MA/JU
Sample : 05976-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

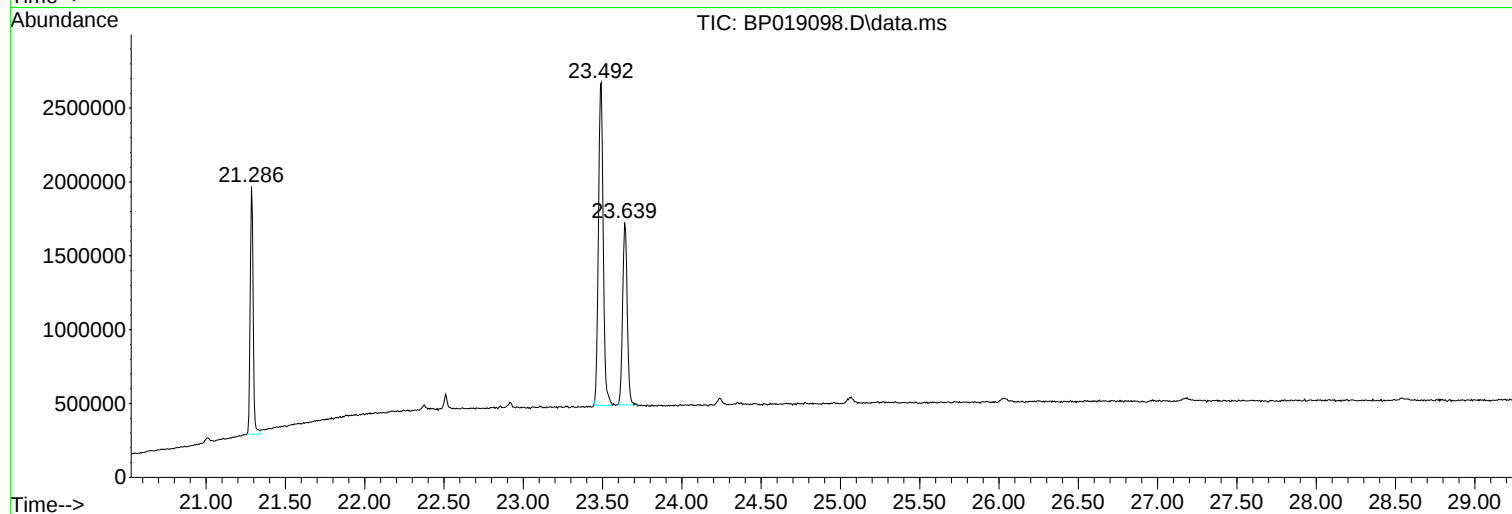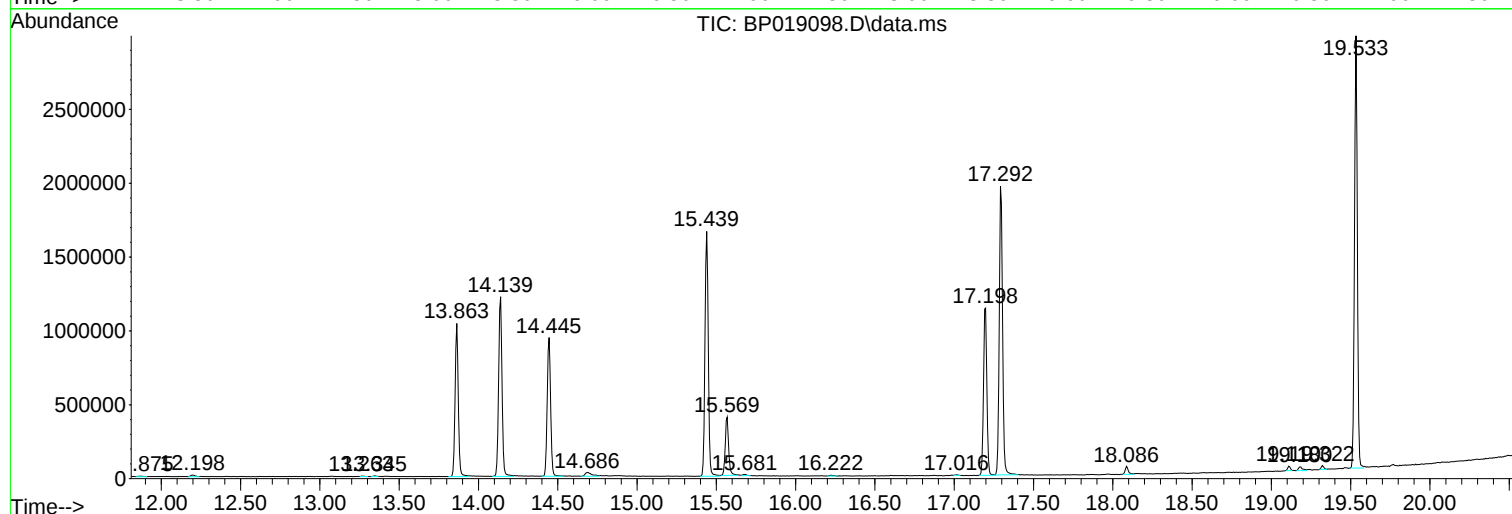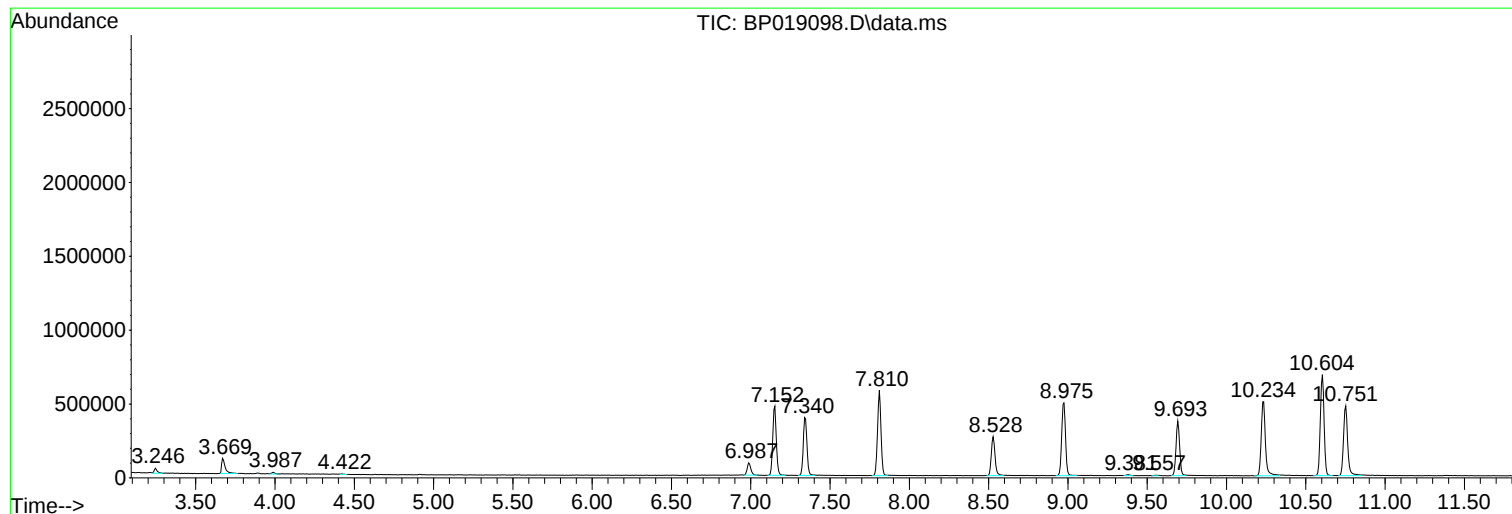

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019098.D
Acq On : 27 Dec 2023 00:00
Operator : MA/JU
Sample : 05976-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019098.D
Acq On : 27 Dec 2023 00:00
Operator : MA/JU
Sample : 05976-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc