

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019103.D
 Acq On : 27 Dec 2023 02:50
 Operator : MA/JU
 Sample : PB158030BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK030

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	37	rVB	55700	68785	1.57%	0.184%
2	3.664	94	98	115	rBV	609433	897816	20.51%	2.401%
3	3.987	150	153	159	rVB3	9322	11741	0.27%	0.031%
4	6.987	656	663	679	rVB	639547	1008611	23.04%	2.697%
5	7.152	684	691	700	rVB	522564	822310	18.78%	2.199%
6	7.340	716	723	733	rBV	657846	1022991	23.37%	2.735%
7	7.811	796	803	810	rBV	523094	829513	18.95%	2.218%
8	8.528	918	925	940	rBV	735433	1210132	27.64%	3.236%
9	8.969	992	1000	1015	rBV	570544	944159	21.57%	2.525%
10	9.693	1115	1123	1133	rBV	450763	732875	16.74%	1.960%
11	10.228	1206	1214	1227	rBV	687582	1206415	27.56%	3.226%
12	10.605	1269	1278	1285	rBV	662853	1107066	25.29%	2.960%
13	10.752	1294	1303	1313	rBV	661684	1204560	27.52%	3.221%
14	12.199	1542	1549	1558	rBV	12429	24752	0.57%	0.066%
15	13.346	1737	1744	1752	rBV9	6953	13203	0.30%	0.035%
16	13.416	1752	1756	1761	rBV8	2461	5170	0.12%	0.014%
17	13.863	1825	1832	1844	rBV	1166171	1638441	37.43%	4.381%
18	14.140	1872	1879	1890	rBV	1356484	2030878	46.39%	5.430%
19	14.446	1923	1931	1941	rBV	937333	1411436	32.24%	3.774%
20	14.669	1961	1969	1990	rBV	313019	743230	16.98%	1.987%
21	15.440	2093	2100	2114	rBV	1841229	2613536	59.70%	6.988%
22	15.563	2115	2121	2136	rVV	437501	657654	15.02%	1.759%
23	15.675	2137	2140	2148	rVB4	9039	16970	0.39%	0.045%
24	16.222	2229	2233	2238	rVB6	7744	10612	0.24%	0.028%
25	16.875	2341	2344	2349	rVB7	3655	5634	0.13%	0.015%
26	17.198	2392	2399	2409	rBV	1180233	1721866	39.33%	4.604%
27	17.292	2409	2415	2432	rVV	2008124	2830980	64.67%	7.570%
28	19.110	2721	2724	2729	rBV3	24573	31547	0.72%	0.084%
29	19.181	2733	2736	2740	rVB2	21279	27672	0.63%	0.074%
30	19.533	2790	2796	2807	rBV	2767762	3613931	82.56%	9.663%
31	21.286	3090	3094	3103	rBV	1650342	2104766	48.08%	5.628%
32	23.492	3462	3469	3486	rVB2	2107381	4377508	100.00%	11.705%
33	23.639	3488	3494	3506	rVB	1198238	2451042	55.99%	6.554%




Sum of corrected areas: 37397802

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019103.D
Acq On : 27 Dec 2023 02:50
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

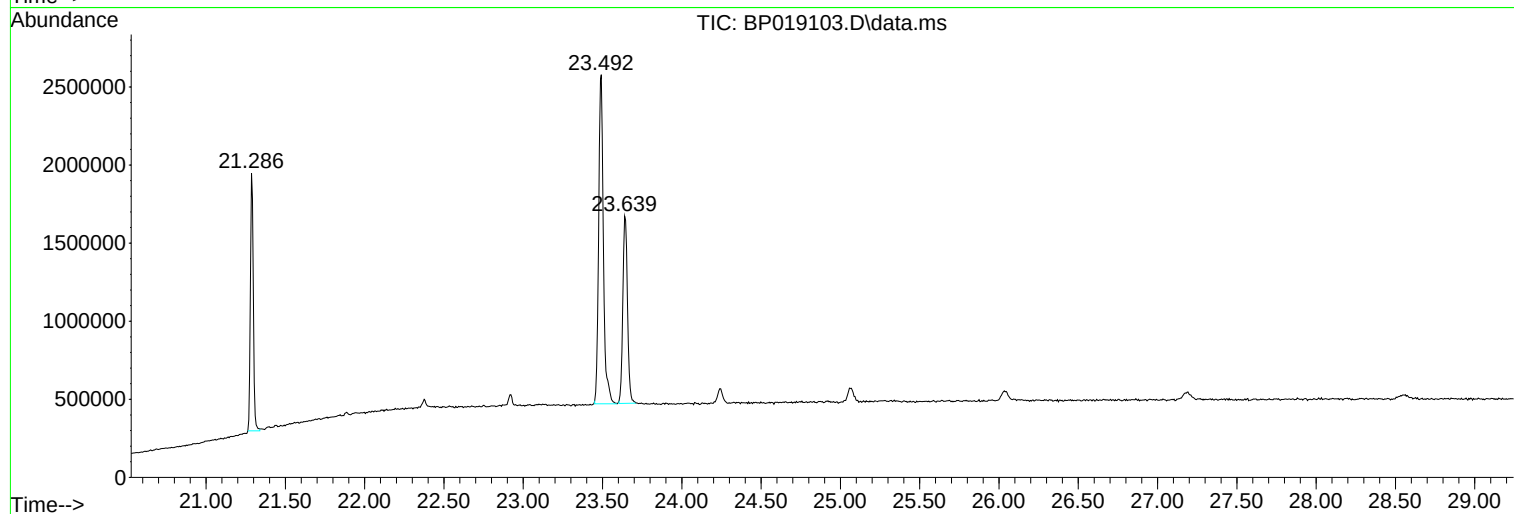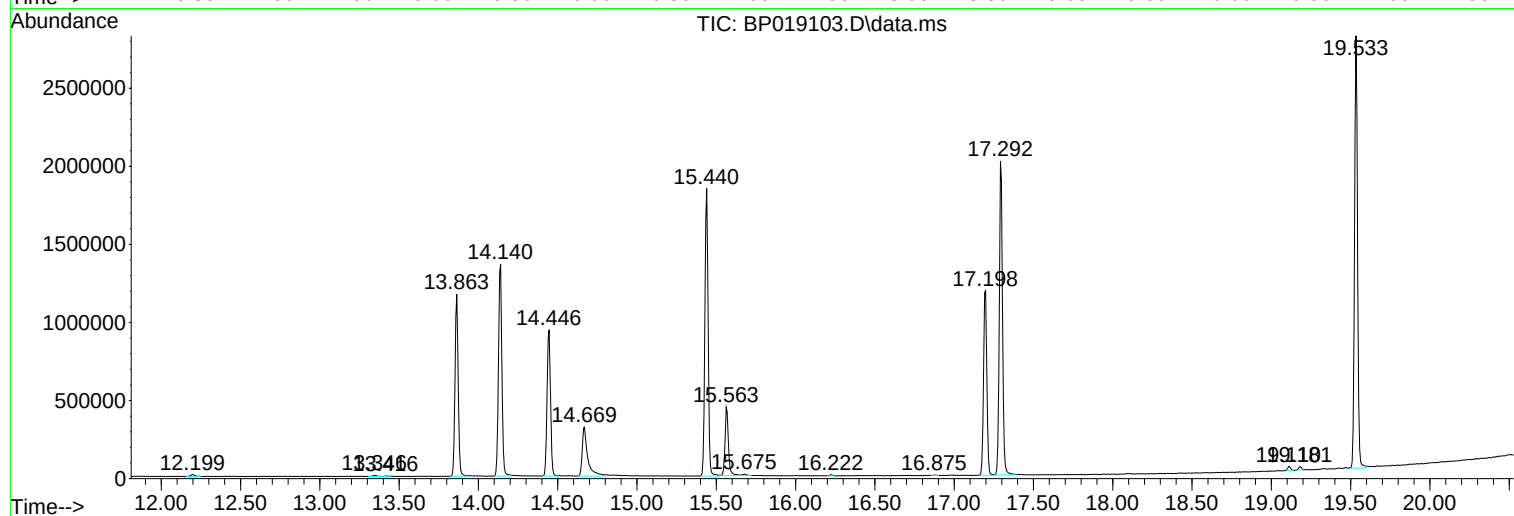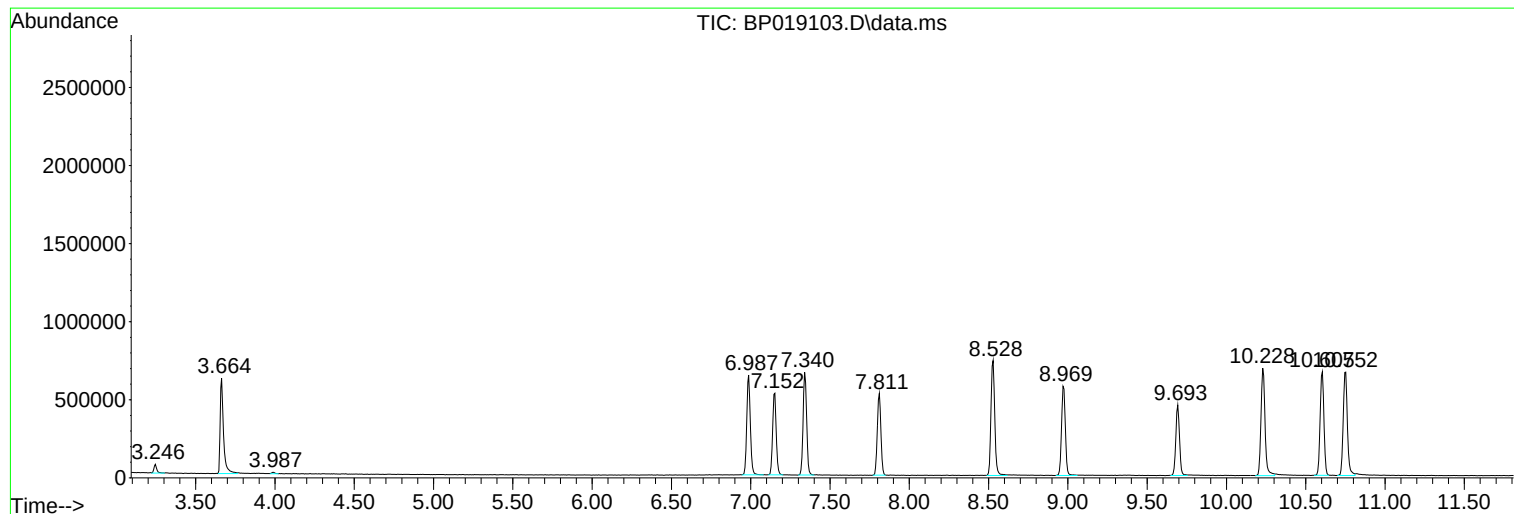

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019103.D
Acq On : 27 Dec 2023 02:50
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019103.D
Acq On : 27 Dec 2023 02:50
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc