

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
 Data File : BP019105.D
 Acq On : 27 Dec 2023 03:58
 Operator : MA/JU
 Sample : PB158050BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	35	rVB	52620	65489	1.46%	0.163%
2	3.664	94	98	113	rBV	622260	907690	20.28%	2.263%
3	3.987	149	153	158	rVB	11087	15224	0.34%	0.038%
4	6.987	656	663	676	rBV	641544	1020614	22.80%	2.545%
5	7.146	684	690	703	rVB	540958	849782	18.98%	2.119%
6	7.340	716	723	735	rBV	674318	1052869	23.52%	2.625%
7	7.810	795	803	811	rBV	581398	930848	20.80%	2.321%
8	8.522	917	924	939	rBV	739444	1241225	27.73%	3.095%
9	8.969	989	1000	1010	rBV	583132	968598	21.64%	2.415%
10	9.428	1074	1078	1082	rVB7	2230	4562	0.10%	0.011%
11	9.693	1112	1123	1131	rBV	466763	760980	17.00%	1.898%
12	10.228	1206	1214	1230	rBV	728916	1257719	28.10%	3.136%
13	10.604	1270	1278	1285	rBV	746204	1247500	27.87%	3.111%
14	10.746	1294	1302	1320	rBV	702472	1273701	28.45%	3.176%
15	12.193	1544	1548	1556	rBV3	12190	23185	0.52%	0.058%
16	13.345	1737	1744	1750	rVV5	8509	16194	0.36%	0.040%
17	13.863	1825	1832	1844	rBV	1242591	1714709	38.31%	4.276%
18	14.139	1871	1879	1893	rBV	1420402	2140670	47.82%	5.338%
19	14.445	1922	1931	1940	rBV	1079697	1612091	36.01%	4.020%
20	14.663	1961	1968	1991	rBV	340081	795054	17.76%	1.983%
21	15.439	2091	2100	2113	rBV	1905202	2738191	61.17%	6.828%
22	15.563	2115	2121	2136	rVV	463581	708254	15.82%	1.766%
23	15.675	2137	2140	2151	rVB6	11296	22901	0.51%	0.057%
24	16.222	2228	2233	2238	rVB5	7176	12097	0.27%	0.030%
25	16.875	2340	2344	2348	rVB7	3741	6580	0.15%	0.016%
26	16.981	2357	2362	2365	rBV5	2599	4608	0.10%	0.011%
27	17.198	2392	2399	2409	rBV	1380093	2004114	44.77%	4.997%
28	17.292	2409	2415	2432	rVV2	2059275	3002869	67.08%	7.488%
29	19.110	2721	2724	2731	rVB3	28302	39023	0.87%	0.097%
30	19.180	2732	2736	2744	rBV	26674	45823	1.02%	0.114%
31	19.533	2790	2796	2806	rBV	2866405	3800505	84.90%	9.477%
32	21.286	3089	3094	3101	rBV	2027240	2520205	56.30%	6.284%
33	23.492	3462	3469	3481	rVB2	2082676	4476262	100.00%	11.162%
34	23.639	3488	3494	3505	rVB	1386985	2822803	63.06%	7.039%

Sum of corrected areas: 40102939




Instrument :
BNA_P
ClientSampleId :
SBLK050

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019105.D
Acq On : 27 Dec 2023 03:58
Operator : MA/JU
Sample : PB158050BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK050

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

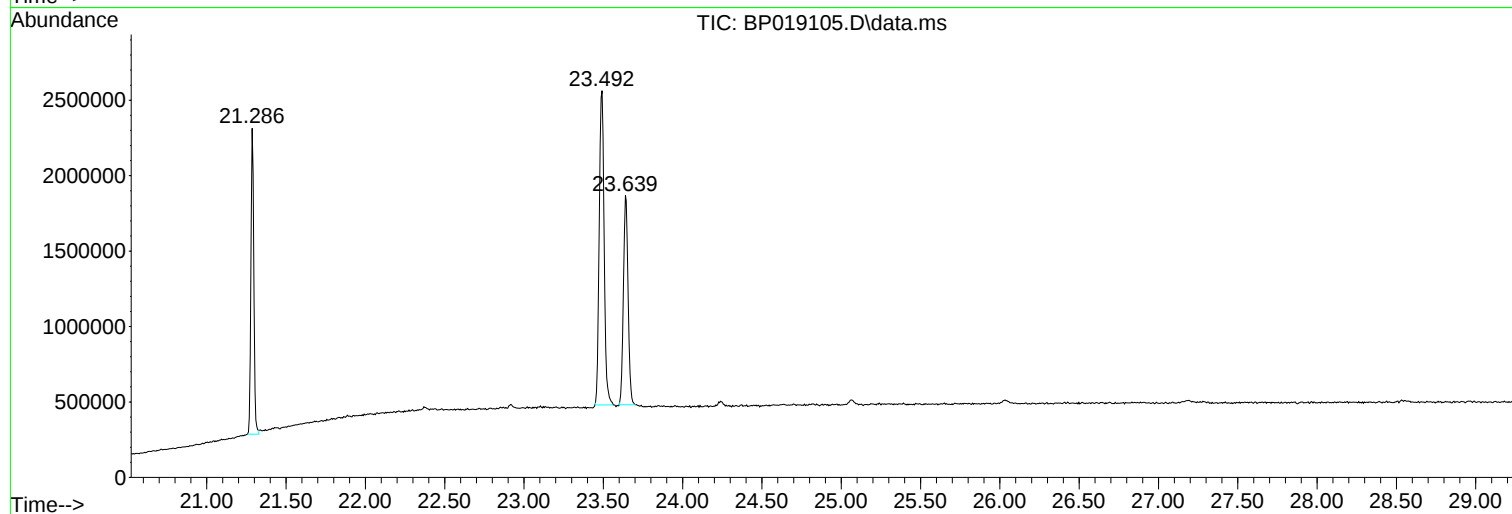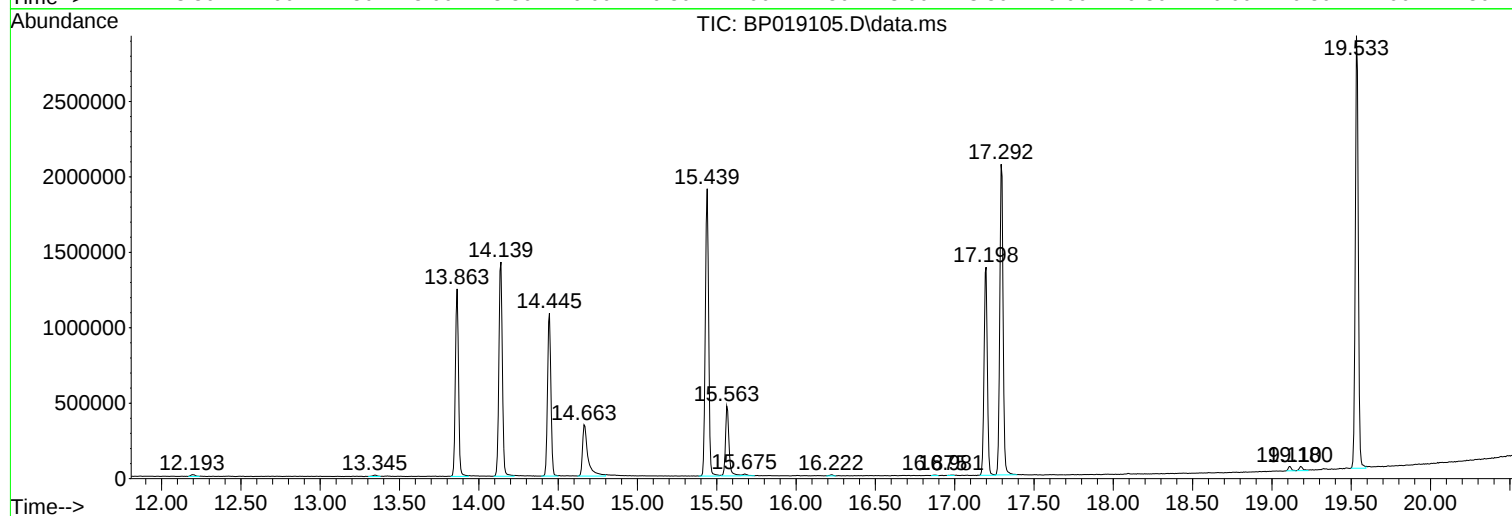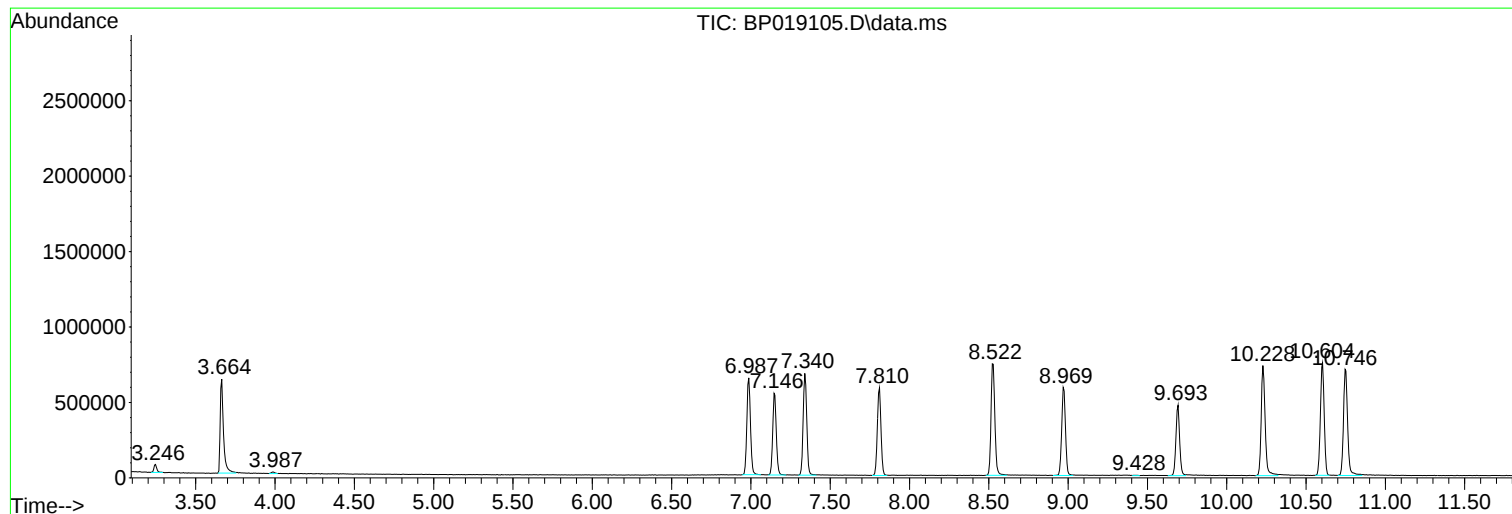

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019105.D
Acq On : 27 Dec 2023 03:58
Operator : MA/JU
Sample : PB158050BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK050

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019105.D
Acq On : 27 Dec 2023 03:58
Operator : MA/JU
Sample : PB158050BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK050

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc