
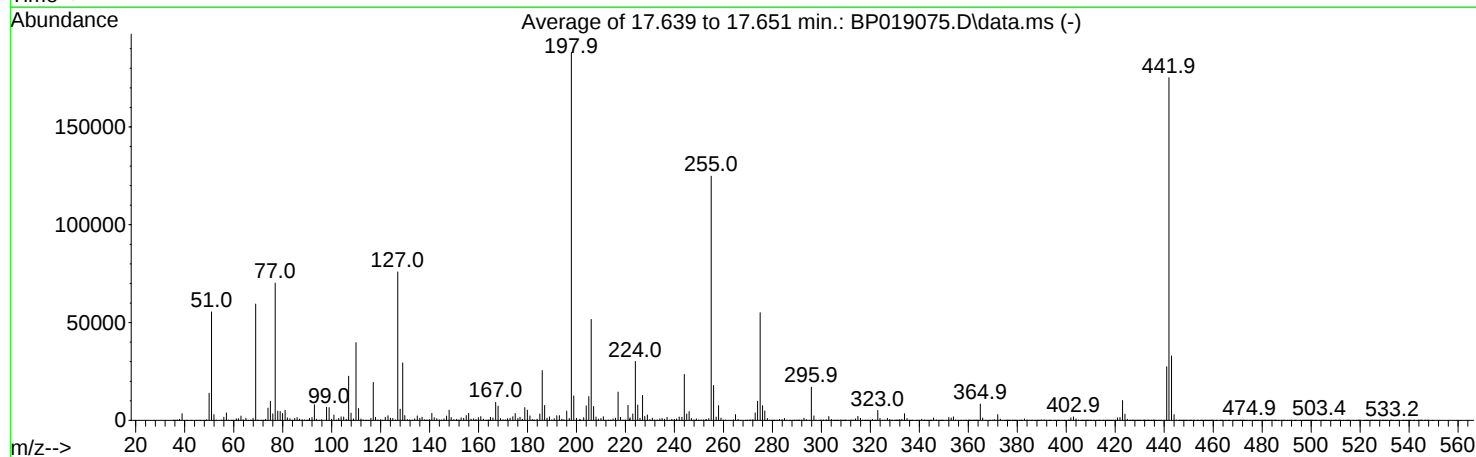


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122623\
Data File : BP019075.D
Acq On : 26 Dec 2023 10:19
Operator : MA/JU
Sample : DFTPP694
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP694

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Dec 26 22:20:53 2023

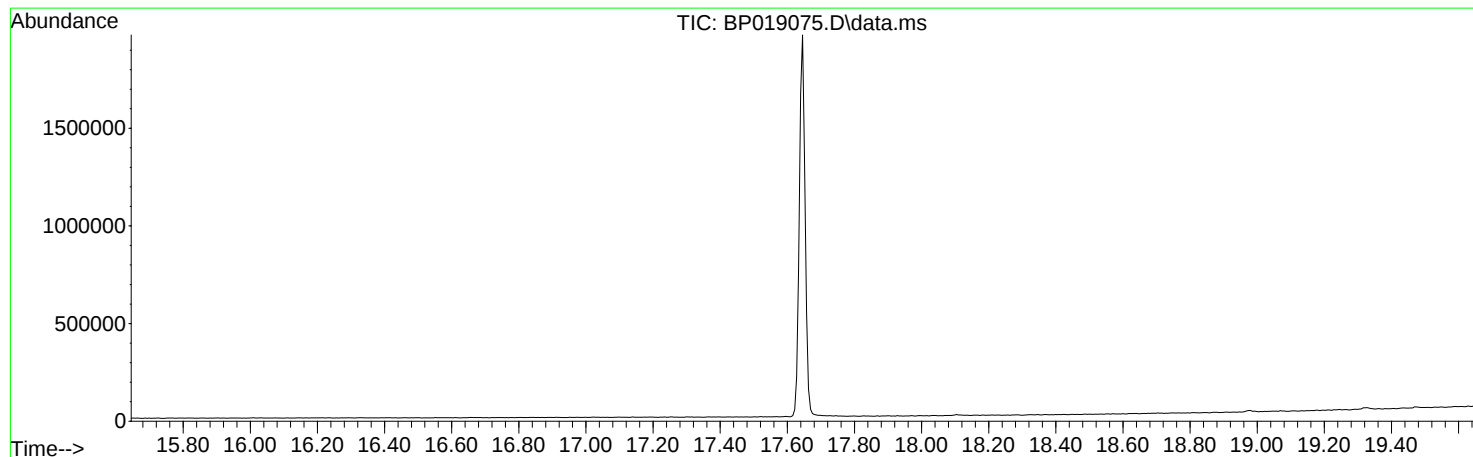

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	55468	PASS
68	69	0.00	2	1.9	1103	PASS
69	198	0.00	100	31.6	59468	PASS
70	69	0.00	2	0.4	253	PASS
127	198	10	80	40.4	75880	PASS
197	198	0.00	2	0.5	1029	PASS
198	198	100	100	100.0	188053	PASS
199	198	5	9	6.7	12527	PASS
275	198	10	60	29.3	55023	PASS
365	198	1	100	4.4	8347	PASS
441	198	0.01	100	14.6	27422	PASS
442	198	50	100	93.2	175228	PASS
443	442	15	24	18.8	32968	PASS

m/z	Abundance
35.00	24.0
35.80	57.0
36.80	24.0
37.50	20.0
37.90	17.0
38.90	138.0
40.00	1198.0
41.00	167.0
42.00	151.0
43.10	146.0
44.00	2951.0
45.00	156.0
45.80	17.0
47.00	110.0
48.00	32.0
48.90	363.0
50.00	55.0
50.90	180.0
51.90	27.0
52.60	21.0
53.10	11.0
53.80	85.0
55.10	167.0
55.90	85.0
57.00	120.0
58.00	14.0
58.90	82.0
59.90	14.0
60.60	18.0
61.10	3.0
61.80	16.0
62.80	20.0
63.70	39.0
64.70	11.0
65.40	10.0
65.90	12.0
66.90	81.0
67.90	44.0
69.20	49.0
69.80	12.0
70.20	14.0
71.20	37.0
72.00	11.0
73.00	544.0
74.00	150.0
75.00	118.0
75.90	28.0
76.90	137.0
78.10	160.0
78.90	108.0
79.90	27.0
81.00	82.0
82.00	16.0
83.10	93.0
83.80	207.0
84.70	8.0
85.90	205.0
86.80	36.0
87.90	54.0
89.20	46.0
90.10	12.0
91.00	143.0
92.00	60.0
92.90	48.0
94.10	10.0
94.90	86.0
95.80	127.0
96.70	211.0
98.70	7.0
99.10	7.0
100.40	5.0
101.10	19.0
102.00	26.0
102.90	116.0
103.90	17.0
104.90	45.0
105.90	18.0
106.80	34.0
108.00	12.0
108.80	15.0
109.30	12.0
109.90	16.0
110.80	6.0
111.20	12.0
112.10	16.0
112.90	4.0
114.00	15.0
114.90	25.0
116.00	49.0
117.10	50.0
118.00	46.0
118.80	63.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

119.90	9.0
121.10	15.0
121.80	23.0
122.50	8.0
124.00	21.0
125.20	8.0
126.10	7.0
127.30	10.0
128.10	21.0
129.00	60.0
129.90	2.0
130.60	14.0
131.10	13.0
131.90	31.0
132.90	127.0
133.10	127.0
134.00	30.0
135.00	286.0
136.00	22.0
136.80	52.0
137.60	2.0
138.20	13.0
138.70	4.0
139.30	7.0
140.00	15.0
140.90	16.0
142.60	8.0
144.90	40.0
146.00	5.0
147.00	267.0
148.20	9.0
148.70	71.0
150.00	16.0
151.10	10.0
152.40	5.0
153.00	21.0
154.10	5.0
154.90	8.0
155.30	7.0
155.90	20.0
156.90	13.0
158.00	13.0
159.00	13.0
160.80	36.0
162.90	170.0
163.70	14.0
164.90	86.0
165.80	5.0
166.50	11.0
167.30	18.0
168.10	17.0
168.60	5.0
169.10	18.0
169.70	4.0
170.50	8.0
171.00	22.0
171.80	9.0
172.90	20.0
174.30	7.0
174.80	8.0
175.80	86.0
176.90	126.0
177.90	49.0
178.80	59.0
179.80	1.0
181.00	15.0
182.00	20.0
183.20	1.0
183.80	5.0
184.60	2.0
185.20	24.0
187.20	19.0
188.30	9.0
189.10	13.0
190.00	44.0
190.90	348.0
191.90	99.0
193.00	498.0
193.80	83.0
195.00	27.0
196.00	12.0
196.40	9.0
198.20	5.0
199.20	10.0
199.60	13.0
200.70	18.0
202.00	17.0
202.80	26.0
203.30	7.0
204.10	9.0
204.60	11.0
205.70	16.0
207.00	3118.0
208.00	695.0
209.00	416.0
209.90	70.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

211.00	42.0
211.70	1.0
212.10	4.0
213.00	8.0
214.10	4.0
215.20	4.0
216.00	0.0
216.70	4.0
217.50	1.0
218.10	15.0
218.90	14.0
219.30	15.0
220.20	21.0
221.00	279.0
222.00	41.0
222.70	63.0
223.70	5.0
224.20	7.0
225.10	15.0
225.80	7.0
226.20	4.0
227.80	13.0
228.50	0.0
229.30	16.0
230.90	11.0
232.20	2.0
232.70	3.0
233.80	8.0
234.20	11.0
235.10	1.0
235.60	3.0
237.20	25.0
238.10	18.0
238.90	24.0
240.50	9.0
241.10	17.0
241.90	11.0
242.60	2.0
243.50	6.0
244.10	6.0
245.50	16.0
246.60	18.0
247.60	7.0
249.00	141.0
250.00	25.0
250.90	73.0
252.30	6.0
253.00	32.0
254.00	17.0
256.30	4.0
257.50	1.0
258.00	2.0
258.60	1.0
259.40	4.0
260.20	18.0
260.90	7.0
261.90	14.0
262.80	14.0
263.80	6.0
264.90	140.0
265.80	12.0
267.00	202.0
267.80	83.0
268.90	26.0
270.10	17.0
270.70	7.0
271.20	13.0
272.10	4.0
273.10	2.0
273.50	2.0
275.20	20.0
276.90	6.0
278.80	16.0
279.90	17.0
281.00	756.0
281.80	201.0
282.90	181.0
284.70	9.0
286.10	11.0
287.60	4.0
287.90	4.0
288.60	2.0
289.30	18.0
290.00	2.0
290.70	3.0
291.90	0.0
292.50	15.0
293.80	4.0
295.10	55.0
295.80	19.0
296.70	1.0
297.30	14.0
298.10	0.0
298.90	14.0
300.20	1.0
300.80	11.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

302.00	3.0
303.30	3.0
304.10	2.0
304.90	5.0
306.30	3.0
307.10	4.0
307.80	4.0
308.80	6.0
309.30	4.0
309.80	9.0
311.10	3.0
312.20	0.0
312.70	4.0
313.90	19.0
314.50	3.0
315.20	0.0
315.80	20.0
317.00	1.0
317.50	2.0
318.00	1.0
318.70	2.0
319.10	4.0
320.10	1.0
320.80	4.0
321.90	1.0
322.70	16.0
323.60	7.0
324.50	6.0
325.00	11.0
325.90	13.0
327.00	59.0
327.80	6.0
328.50	8.0
329.10	13.0
329.60	3.0
330.30	3.0
331.00	3.0
331.70	4.0
332.80	5.0
333.60	2.0
334.70	5.0
335.90	1.0
336.50	3.0
337.50	3.0
338.00	3.0
339.00	7.0
339.90	2.0
340.90	128.0
342.00	23.0
343.10	15.0
344.00	11.0
345.80	4.0
346.70	0.0
347.40	8.0
348.20	2.0
349.10	4.0
349.80	0.0
350.50	4.0
352.00	7.0
352.50	11.0
353.80	4.0
354.90	269.0
356.00	71.0
356.80	50.0
357.60	12.0
358.10	6.0
359.10	2.0
360.00	2.0
360.60	1.0
361.50	4.0
362.10	3.0
362.80	2.0
363.20	3.0
365.00	5.0
366.20	22.0
367.60	10.0
368.00	19.0
369.10	39.0
370.30	0.0
370.80	2.0
371.30	15.0
372.70	4.0
373.70	5.0
374.30	4.0
375.30	4.0
375.90	3.0
376.80	4.0
377.40	6.0
378.80	4.0
379.60	0.0
380.60	3.0
381.60	3.0
382.10	4.0
383.70	4.0
384.80	5.0
385.30	2.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

386.10	1.0
386.80	23.0
387.70	17.0
388.30	9.0
389.00	0.0
389.90	3.0
390.50	11.0
391.70	4.0
393.30	3.0
394.50	7.0
395.50	1.0
396.40	11.0
397.40	1.0
397.80	3.0
398.60	9.0
399.20	9.0
399.90	15.0
400.60	1.0
401.10	63.0
401.80	12.0
402.70	12.0
404.10	4.0
405.50	4.0
406.10	1.0
407.20	3.0
408.40	2.0
408.90	2.0
410.60	8.0
411.70	5.0
413.00	18.0
413.60	4.0
414.80	48.0
415.30	13.0
415.80	10.0
416.20	7.0
417.10	8.0
418.20	3.0
418.80	2.0
419.90	6.0
421.60	6.0
422.40	11.0
423.00	3.0
423.80	1.0
424.60	3.0
425.30	5.0
425.90	4.0
427.50	3.0
427.90	10.0
429.10	17.0
431.00	20.0
432.50	3.0
433.10	4.0
434.20	4.0
434.70	1.0
435.60	6.0
436.90	5.0
437.40	3.0
438.20	2.0
439.00	3.0
440.30	4.0
441.20	2.0
441.80	4.0
442.80	11.0
443.40	3.0
444.20	1.0
444.80	2.0
445.30	2.0
446.60	3.0
447.30	0.0
447.90	1.0
448.40	2.0
449.70	3.0
450.50	0.0
451.20	3.0
451.70	1.0
452.80	5.0
454.10	2.0
454.60	3.0
455.20	0.0
456.10	4.0
457.40	3.0
459.20	4.0
460.10	5.0
460.60	2.0
461.80	14.0
462.50	9.0
463.80	5.0
464.50	21.0
465.40	4.0
466.80	3.0
467.20	2.0
468.70	5.0
470.10	3.0
470.80	1.0
471.80	4.0
473.00	14.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

474.40	11.0
475.20	13.0
475.70	7.0
476.40	10.0
477.60	2.0
478.00	3.0
479.50	6.0
481.40	12.0
482.70	3.0
483.90	1.0
484.40	14.0
485.90	4.0
486.80	2.0
487.50	9.0
488.70	28.0
489.20	19.0
490.10	2.0
490.90	2.0
492.20	5.0
493.20	2.0
493.80	3.0
494.80	6.0
495.60	3.0
496.90	3.0
498.50	4.0
500.10	3.0
500.60	2.0
501.00	2.0
501.70	5.0
502.70	2.0
503.30	3.0
503.80	1.0
505.00	5.0
505.70	1.0
506.40	4.0
507.60	2.0
508.20	3.0
509.20	3.0
509.70	3.0
510.70	5.0
511.30	3.0
511.90	1.0
512.60	4.0
513.40	1.0
514.30	3.0
516.00	5.0
516.90	3.0
517.40	5.0
517.80	7.0
518.80	20.0
520.20	4.0
520.70	4.0
522.00	11.0
523.60	3.0
524.00	1.0
525.20	4.0
526.90	9.0
527.90	2.0
528.40	3.0
530.30	5.0
531.00	1.0
531.60	5.0
532.90	4.0
533.60	2.0
535.00	20.0
535.70	1.0
536.40	4.0
537.00	1.0
537.90	4.0
539.50	4.0
541.00	5.0
542.40	4.0
542.90	2.0
543.50	1.0
544.10	5.0
545.30	2.0
545.60	2.0
546.60	1.0
547.30	5.0
548.20	2.0
548.70	24.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

m/z	Abundance
35.30	23.0
36.00	107.0
37.00	319.0
37.90	715.0
39.00	4302.0
39.90	1103.0
41.00	224.0
41.90	175.0
42.90	125.0
43.90	2852.0
44.90	197.0
45.70	17.0
46.90	78.0
48.00	139.0
49.00	838.0
50.00	15770.0
51.00	64584.0
52.00	3704.0
52.90	205.0
54.00	29.0
54.90	430.0
56.00	1999.0
57.00	4427.0
57.90	220.0
58.90	66.0
60.00	66.0
61.10	871.0
62.00	1052.0
63.00	2753.0
63.90	345.0
65.00	1461.0
65.90	108.0
66.80	124.0
68.00	1273.0
69.00	68296.0
69.90	259.0
71.00	102.0
71.90	62.0
73.00	1157.0
74.00	7188.0
75.00	11729.0
76.00	3539.0
77.00	80824.0
78.00	5688.0
79.00	5556.0
80.00	4119.0
81.00	5685.0
82.00	1797.0
82.90	1169.0
83.90	378.0
85.00	1044.0
86.00	1921.0
86.90	894.0
87.90	458.0
88.90	328.0
89.90	24.0
90.90	1209.0
91.90	1533.0
93.00	9183.0
93.90	628.0
95.00	211.0
95.90	561.0
98.00	7804.0
99.00	7676.0
99.90	617.0
100.90	3185.0
102.00	99.0
103.00	1391.0
103.90	2127.0
104.90	1853.0
106.10	599.0
107.00	25008.0
107.90	4052.0
108.90	763.0
110.00	43624.0
111.00	6797.0
111.90	681.0
112.90	384.0
113.90	18.0
114.90	99.0
116.00	1402.0
117.00	21440.0
117.90	1774.0
118.90	356.0
119.90	294.0
121.00	149.0
121.90	1622.0
123.00	2552.0
124.00	1510.0
125.00	1192.0
126.10	402.0
127.00	83080.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

128.00	6557.0
129.00	33088.0
130.00	2622.0
130.90	539.0
131.90	269.0
132.90	368.0
133.90	943.0
135.00	2754.0
136.00	1186.0
137.00	1989.0
138.00	387.0
138.90	179.0
140.00	566.0
141.00	4081.0
141.90	1583.0
143.00	832.0
144.00	378.0
144.90	286.0
145.90	1096.0
147.00	2805.0
148.00	5550.0
148.90	1524.0
149.90	409.0
151.10	780.0
151.80	297.0
152.90	1435.0
153.90	1380.0
155.00	2331.0
156.00	3636.0
157.00	578.0
158.00	816.0
158.90	699.0
160.00	1455.0
161.00	2131.0
162.10	572.0
162.90	313.0
163.70	155.0
164.20	107.0
164.90	1694.0
165.90	1121.0
167.00	9103.0
168.00	8674.0
168.90	951.0
169.90	388.0
171.00	264.0
171.90	968.0
173.00	1181.0
173.90	1977.0
175.00	3957.0
176.10	711.0
177.00	1774.0
177.80	644.0
178.90	6943.0
180.00	6005.0
181.00	2482.0
182.00	359.0
182.90	217.0
184.10	498.0
185.00	3296.0
186.00	26400.0
187.00	7989.0
188.00	1126.0
188.90	1997.0
189.90	339.0
190.90	1271.0
192.00	2432.0
193.00	2767.0
194.10	574.0
194.90	412.0
196.00	4910.0
197.10	1088.0
197.90	189760.0
198.90	12496.0
200.00	1034.0
201.40	995.0
202.90	1481.0
204.00	7575.0
205.00	12722.0
206.00	52192.0
207.00	10770.0
208.00	2263.0
208.90	1081.0
210.10	997.0
211.00	1992.0
212.90	298.0
214.00	60.0
215.00	590.0
216.00	1048.0
217.00	14828.0
218.00	1708.0
218.90	163.0
219.10	168.0
220.10	402.0
221.00	7519.0
221.70	1933.0
222.90	3302.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

224.00	30384.0
225.00	8096.0
226.00	1048.0
227.00	13073.0
228.00	2480.0
228.90	2553.0
230.00	426.0
231.00	1067.0
231.90	223.0
232.90	227.0
233.90	863.0
235.00	1077.0
235.90	464.0
236.90	1737.0
238.00	255.0
239.00	666.0
240.00	361.0
240.90	659.0
242.00	1514.0
243.00	1526.0
244.00	22552.0
245.00	3363.0
246.00	4184.0
246.90	928.0
247.90	282.0
248.90	927.0
249.80	197.0
250.90	373.0
252.00	179.0
252.80	541.0
254.00	865.0
255.00	118728.0
256.00	17968.0
257.00	1990.0
258.00	7506.0
259.00	1129.0
260.00	221.0
260.80	167.0
262.00	3.0
263.00	47.0
264.00	215.0
264.90	2873.0
266.10	443.0
266.90	273.0
267.80	118.0
268.90	57.0
269.80	117.0
270.90	372.0
271.90	388.0
272.90	3795.0
274.00	9314.0
275.00	51608.0
276.00	7572.0
277.00	4784.0
277.90	940.0
278.90	271.0
280.10	27.0
280.90	819.0
281.90	400.0
283.00	713.0
284.10	393.0
285.00	1043.0
285.90	141.0
287.00	27.0
288.00	60.0
288.80	135.0
289.90	161.0
290.70	104.0
291.00	103.0
292.00	219.0
292.90	980.0
293.90	451.0
296.00	16066.0
296.90	2512.0
297.80	171.0
298.90	23.0
300.90	260.0
302.00	431.0
303.00	1760.0
304.10	502.0
304.80	94.0
306.10	14.0
306.80	17.0
308.00	314.0
308.70	198.0
309.20	140.0
309.80	162.0
311.00	68.0
312.20	6.0
312.90	243.0
313.90	578.0
314.90	1990.0
316.00	917.0
316.80	77.0
317.00	81.0
317.90	9.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

318.50	14.0
319.10	19.0
319.90	31.0
320.80	376.0
321.90	254.0
323.00	4704.0
324.00	1059.0
325.10	94.0
325.90	129.0
327.00	1036.0
328.00	331.0
329.00	92.0
329.80	14.0
330.30	12.0
330.90	16.0
331.90	348.0
333.00	508.0
333.90	2844.0
335.00	951.0
335.90	137.0
336.70	3.0
337.90	6.0
338.90	46.0
339.90	103.0
341.00	477.0
341.80	112.0
342.70	57.0
343.00	59.0
343.70	11.0
344.30	6.0
345.90	1197.0
346.90	322.0
347.80	28.0
349.00	21.0
350.00	76.0
351.00	130.0
352.10	1270.0
353.00	1113.0
354.00	1615.0
354.80	394.0
355.90	110.0
356.90	121.0
358.00	14.0
358.90	135.0
359.90	12.0
360.40	5.0
361.10	11.0
361.90	6.0
363.00	20.0
363.90	24.0
364.90	7260.0
365.90	955.0
367.10	38.0
368.00	8.0
368.60	4.0
370.00	101.0
370.80	326.0
372.00	2547.0
373.00	733.0
373.80	102.0
375.20	1.0
375.90	22.0
376.80	90.0
377.90	7.0
378.70	25.0
379.70	14.0
380.40	3.0
380.80	3.0
381.40	5.0
382.90	715.0
384.00	255.0
384.90	66.0
385.50	13.0
386.00	21.0
386.80	11.0
387.90	14.0
388.20	17.0
389.00	10.0
389.90	163.0
390.90	334.0
392.00	164.0
393.10	21.0
394.70	20.0
396.40	15.0
397.00	25.0
397.80	2.0
398.40	4.0
399.10	9.0
399.80	20.0
400.90	229.0
401.90	1062.0
402.90	1270.0
404.00	608.0
405.00	276.0
406.00	23.0
406.90	12.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

407.60	4.0
408.10	19.0
408.90	17.0
409.90	21.0
410.50	6.0
412.30	6.0
413.20	0.0
413.90	4.0
415.10	127.0
415.90	16.0
417.20	16.0
418.50	13.0
419.10	6.0
419.90	49.0
420.90	975.0
421.90	1335.0
423.00	8042.0
424.00	2902.0
424.90	445.0
425.80	2.0
426.20	4.0
427.00	14.0
428.20	11.0
429.20	46.0
429.90	18.0
431.20	4.0
431.70	3.0
432.30	11.0
434.50	8.0
435.50	19.0
436.60	12.0
437.60	89.0
438.80	64.0
439.90	220.0
441.00	22112.0
442.00	137664.0
443.00	26520.0
444.00	2519.0
445.10	71.0
446.20	1.0
447.00	11.0
448.50	7.0
450.00	5.0
450.70	1.0
451.80	4.0
452.40	0.0
453.40	22.0
454.60	8.0
455.00	14.0
456.40	4.0
457.20	2.0
457.80	3.0
459.50	5.0
460.30	0.0
461.00	13.0
461.70	14.0
462.30	2.0
462.80	2.0
463.50	2.0
464.10	4.0
465.40	2.0
466.10	3.0
466.50	1.0
468.00	8.0
468.50	2.0
468.80	2.0
471.00	7.0
471.90	10.0
472.60	3.0
473.60	3.0
474.80	22.0
475.30	19.0
475.90	12.0
476.90	11.0
477.90	6.0
478.40	5.0
479.40	2.0
480.10	14.0
481.00	1.0
481.50	3.0
483.00	3.0
483.70	0.0
484.40	1.0
485.00	14.0
486.50	11.0
487.80	3.0
488.70	12.0
489.30	2.0
490.20	14.0
491.00	8.0
492.20	9.0
492.90	22.0
493.50	1.0
494.00	3.0
495.30	1.0
495.80	3.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

496.40	15.0
497.50	4.0
498.40	2.0
498.80	2.0
499.80	0.0
500.40	2.0
502.10	10.0
503.50	7.0
504.20	3.0
505.10	4.0
505.80	7.0
506.50	3.0
507.00	3.0
508.30	4.0
509.00	0.0
509.90	4.0
511.40	12.0
512.40	1.0
513.00	2.0
513.60	0.0
514.50	6.0
515.60	9.0
516.10	5.0
517.10	1.0
517.80	5.0
519.20	5.0
520.90	4.0
522.20	2.0
522.70	2.0
524.10	5.0
524.90	1.0
525.70	4.0
527.10	4.0
527.90	5.0
528.50	3.0
529.00	6.0
530.00	5.0
531.60	3.0
532.20	3.0
533.20	17.0
534.40	11.0
535.10	3.0
536.30	4.0
537.30	15.0
538.40	18.0
539.40	7.0
540.00	4.0
541.00	10.0
541.70	2.0
543.00	3.0
543.80	2.0
544.50	3.0
545.20	1.0
546.20	5.0
547.20	7.0
547.70	3.0
548.80	6.0
549.30	6.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

m/z	Abundance
35.90	102.0
37.00	393.0
38.00	698.0
39.00	3797.0
40.00	1116.0
41.00	275.0
41.80	25.0
43.10	110.0
44.00	3020.0
44.90	192.0
46.10	12.0
46.90	88.0
47.90	168.0
48.90	677.0
50.00	17296.0
51.00	65224.0
52.00	3229.0
52.90	155.0
53.90	87.0
55.00	372.0
56.00	1985.0
57.00	4617.0
57.90	301.0
59.00	128.0
59.90	75.0
61.00	1082.0
62.00	1088.0
63.00	2558.0
63.90	408.0
65.00	1338.0
66.00	152.0
66.80	240.0
68.00	1318.0
69.00	69440.0
70.00	336.0
71.00	40.0
71.90	89.0
73.00	1131.0
74.00	7496.0
75.00	10940.0
76.00	4359.0
77.00	82016.0
78.00	5739.0
79.00	5347.0
80.00	4130.0
81.00	5930.0
81.90	1264.0
83.00	1141.0
83.90	313.0
84.90	1190.0
85.90	1949.0
87.00	831.0
87.80	442.0
88.90	197.0
90.00	27.0
91.00	1361.0
92.00	1976.0
93.00	8856.0
93.90	848.0
95.00	226.0
96.00	563.0
96.90	263.0
97.90	8007.0
98.90	7372.0
100.00	648.0
101.00	3321.0
102.00	247.0
102.90	1086.0
104.00	2012.0
105.00	2398.0
105.90	685.0
107.00	27272.0
108.00	4322.0
109.00	848.0
110.00	47928.0
111.00	7096.0
112.00	900.0
113.00	305.0
113.90	30.0
114.80	186.0
116.00	1329.0
117.00	22800.0
118.00	1925.0
119.00	352.0
120.00	457.0
120.80	136.0
122.00	1925.0
123.00	2588.0
124.00	1474.0
124.90	1135.0
127.00	89704.0
128.00	6750.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

129.00	34656.0
129.90	3063.0
130.90	444.0
131.90	279.0
132.80	449.0
133.90	983.0
135.00	3141.0
136.00	1116.0
137.00	1968.0
138.00	510.0
139.00	136.0
140.00	446.0
141.00	4519.0
141.90	1645.0
143.00	1156.0
144.00	283.0
145.00	335.0
145.90	740.0
147.00	2580.0
147.90	6094.0
148.90	1806.0
149.90	473.0
151.10	609.0
152.00	486.0
152.90	1519.0
154.00	1183.0
155.00	2882.0
156.00	4397.0
156.90	804.0
157.90	932.0
159.00	605.0
160.00	1680.0
161.00	2416.0
161.90	939.0
162.80	333.0
163.90	304.0
164.90	1797.0
166.00	1687.0
167.00	11331.0
168.00	8101.0
169.00	1061.0
170.10	422.0
170.80	429.0
171.90	1032.0
172.90	1297.0
174.00	2265.0
175.00	4041.0
176.00	1278.0
177.00	2005.0
177.90	700.0
178.90	8063.0
180.00	5816.0
181.00	2670.0
182.00	513.0
182.80	320.0
183.90	962.0
185.00	3883.0
186.00	30168.0
187.00	8494.0
188.00	1307.0
189.00	2071.0
189.90	441.0
190.90	1140.0
192.00	2846.0
193.00	3730.0
194.00	825.0
194.90	439.0
196.00	5396.0
197.00	1185.0
197.90	224320.0
198.90	15544.0
200.00	1542.0
201.50	858.0
203.00	1731.0
204.00	9324.0
205.00	14282.0
206.00	61424.0
207.00	11685.0
207.90	2823.0
208.90	1227.0
210.00	1191.0
210.90	2261.0
213.10	187.0
213.90	108.0
215.00	992.0
215.90	1514.0
216.90	17056.0
217.90	1860.0
218.80	190.0
221.00	9786.0
221.90	2605.0
223.00	3768.0
224.00	35728.0
225.00	9404.0
226.00	1198.0
227.00	14756.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

227.90	2321.0
228.90	3573.0
229.90	524.0
231.00	1408.0
232.00	284.0
233.00	330.0
234.00	834.0
234.90	1370.0
235.90	704.0
237.00	1738.0
237.80	205.0
238.90	704.0
240.00	715.0
240.90	1025.0
242.00	2277.0
243.00	1944.0
244.00	28272.0
245.00	3856.0
246.00	5170.0
246.90	1270.0
247.80	270.0
248.90	1062.0
250.00	334.0
250.80	247.0
251.90	415.0
253.00	810.0
254.00	981.0
255.00	149824.0
256.00	21272.0
257.00	2055.0
258.00	9118.0
259.00	1393.0
259.80	270.0
261.00	286.0
261.90	17.0
262.80	108.0
264.10	382.0
265.00	4003.0
265.90	511.0
267.00	248.0
267.90	97.0
268.80	67.0
269.80	235.0
270.90	451.0
272.10	390.0
273.00	4441.0
273.90	11903.0
275.00	66952.0
276.00	9316.0
277.00	5800.0
277.90	1051.0
279.00	177.0
280.20	26.0
281.00	853.0
281.90	433.0
282.90	675.0
284.10	483.0
285.00	1072.0
285.90	194.0
286.80	14.0
288.00	76.0
289.00	98.0
290.10	242.0
290.90	254.0
291.90	341.0
292.90	1445.0
293.90	377.0
295.90	20056.0
296.90	2564.0
297.80	178.0
298.90	19.0
299.60	3.0
300.90	310.0
302.00	316.0
303.00	2381.0
303.90	668.0
304.90	113.0
305.70	22.0
306.70	11.0
308.00	331.0
308.90	120.0
310.00	235.0
311.00	104.0
311.70	31.0
313.00	179.0
314.00	924.0
314.90	2147.0
316.00	1267.0
316.80	250.0
317.60	17.0
318.90	23.0
319.80	83.0
320.90	504.0
322.10	251.0
323.00	6164.0
323.90	1040.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

325.10	120.0
325.90	183.0
327.00	1237.0
328.00	646.0
329.00	144.0
329.80	8.0
330.50	4.0
331.10	25.0
331.90	479.0
332.90	569.0
334.00	4476.0
335.00	1062.0
335.90	195.0
337.00	7.0
337.60	1.0
338.70	115.0
339.90	112.0
341.10	918.0
342.00	238.0
342.70	70.0
343.70	27.0
344.80	19.0
345.90	1513.0
347.00	304.0
347.70	49.0
348.50	16.0
349.20	6.0
350.00	72.0
350.90	133.0
352.00	1847.0
353.00	1561.0
354.00	2369.0
355.00	494.0
356.00	133.0
356.80	76.0
358.00	36.0
359.10	148.0
360.10	19.0
361.10	12.0
361.70	12.0
362.00	9.0
363.40	22.0
364.90	9542.0
365.90	1624.0
366.90	108.0
369.10	41.0
370.00	123.0
370.80	477.0
372.00	3543.0
373.10	755.0
373.90	106.0
374.70	20.0
375.40	3.0
376.20	15.0
377.00	171.0
378.10	8.0
378.80	16.0
379.50	4.0
381.30	15.0
383.00	1042.0
383.80	220.0
385.00	76.0
386.00	13.0
387.10	9.0
387.60	4.0
389.90	294.0
391.00	305.0
392.00	267.0
393.00	8.0
393.60	1.0
394.80	37.0
395.50	12.0
396.50	22.0
397.00	30.0
397.60	3.0
398.90	18.0
399.90	1.0
400.70	126.0
401.10	204.0
401.90	1410.0
403.00	2067.0
404.00	845.0
404.90	161.0
405.80	27.0
406.40	25.0
407.00	18.0
407.90	6.0
408.50	13.0
409.50	7.0
410.00	10.0
411.00	12.0
412.90	3.0
414.90	132.0
416.00	18.0
417.10	7.0
417.50	14.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

418.90	19.0
420.00	42.0
421.00	1623.0
422.00	1476.0
423.00	12701.0
424.00	3812.0
424.90	805.0
425.80	11.0
426.80	6.0
427.20	5.0
427.90	12.0
428.80	19.0
429.20	57.0
430.10	16.0
430.80	6.0
432.00	24.0
432.60	0.0
433.40	6.0
434.10	0.0
434.90	2.0
435.60	22.0
436.60	5.0
437.10	11.0
437.60	59.0
438.10	13.0
438.90	163.0
441.00	33032.0
442.00	209152.0
443.00	39352.0
444.00	3550.0
444.90	169.0
445.90	20.0
447.50	3.0
448.30	1.0
449.30	13.0
450.60	3.0
451.40	1.0
452.20	3.0
453.70	4.0
454.60	2.0
455.40	14.0
456.80	3.0
458.30	17.0
458.90	7.0
459.70	5.0
460.10	7.0
460.80	1.0
461.30	1.0
462.40	11.0
463.60	11.0
464.10	0.0
464.80	4.0
465.60	0.0
466.10	4.0
467.30	1.0
467.90	4.0
468.50	1.0
469.90	14.0
470.70	3.0
471.20	4.0
472.20	3.0
472.90	11.0
473.20	8.0
474.20	4.0
474.90	24.0
476.10	28.0
476.90	18.0
477.30	13.0
477.90	11.0
479.10	6.0
480.10	3.0
480.60	4.0
481.90	3.0
483.70	4.0
485.20	5.0
486.60	2.0
487.60	1.0
488.40	4.0
488.90	2.0
489.40	1.0
490.00	4.0
491.10	11.0
491.80	3.0
493.50	14.0
494.80	3.0
495.40	2.0
496.20	4.0
497.80	5.0
498.40	9.0
499.10	13.0
499.60	4.0
501.10	3.0
502.60	4.0
503.40	12.0
504.30	10.0
505.00	12.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

505.70	4.0
507.00	11.0
508.10	0.0
508.80	3.0
510.10	2.0
510.60	2.0
511.90	4.0
513.50	2.0
514.30	2.0
515.10	4.0
515.90	2.0
516.70	3.0
517.10	3.0
517.70	1.0
518.30	5.0
519.10	13.0
519.50	9.0
519.80	8.0
521.50	10.0
522.70	5.0
523.10	4.0
524.60	3.0
526.10	4.0
526.90	2.0
527.70	3.0
529.30	5.0
530.30	21.0
531.00	5.0
532.30	3.0
532.60	3.0
533.70	2.0
534.20	4.0
535.20	9.0
535.70	5.0
537.50	8.0
539.10	9.0
540.30	4.0
541.00	1.0
541.90	4.0
542.70	1.0
543.50	5.0
544.30	1.0
545.00	4.0
546.20	2.0
546.70	3.0
548.20	4.0
549.10	2.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

m/z	Abundance
35.90	66.0
37.00	175.0
38.00	446.0
39.00	2679.0
40.00	955.0
41.00	160.0
41.90	64.0
42.90	158.0
44.00	2663.0
45.00	229.0
46.90	65.0
47.80	64.0
49.00	649.0
50.00	8879.0
51.00	37136.0
52.00	1987.0
52.90	100.0
54.00	80.0
54.80	264.0
56.00	1203.0
57.00	2921.0
58.00	112.0
59.00	56.0
60.00	115.0
61.00	474.0
62.10	604.0
63.00	1482.0
63.90	336.0
65.00	755.0
66.00	136.0
67.00	172.0
67.90	851.0
69.00	40816.0
69.90	199.0
71.00	64.0
71.90	24.0
73.00	1036.0
74.00	4589.0
75.00	7207.0
76.00	2165.0
77.00	48176.0
78.00	3416.0
79.00	3094.0
80.00	2390.0
81.00	4022.0
82.00	860.0
82.90	582.0
83.90	464.0
85.00	829.0
86.00	1070.0
86.90	454.0
88.00	182.0
88.90	192.0
89.70	18.0
91.00	892.0
92.00	1106.0
93.00	6262.0
94.00	263.0
94.90	163.0
95.90	311.0
98.00	4435.0
99.00	4517.0
100.00	360.0
101.00	1770.0
102.00	123.0
102.90	871.0
103.90	1329.0
105.00	1150.0
106.00	415.0
107.00	15545.0
108.00	2614.0
108.90	559.0
110.00	27672.0
110.90	4391.0
111.90	622.0
112.80	202.0
114.00	37.0
115.00	138.0
115.90	690.0
116.90	13968.0
118.00	1030.0
118.90	287.0
120.10	235.0
120.80	71.0
122.00	1138.0
123.00	1884.0
124.00	599.0
125.00	756.0
126.10	307.0
127.00	54856.0
127.90	3964.0
129.00	20560.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

129.90	1747.0
130.90	397.0
131.80	244.0
133.00	363.0
134.00	524.0
135.00	1932.0
136.00	1054.0
137.00	1165.0
137.90	159.0
138.60	118.0
139.00	171.0
139.90	335.0
140.90	2364.0
142.00	914.0
142.90	680.0
144.10	145.0
144.70	325.0
146.00	579.0
146.90	1948.0
147.90	4047.0
148.90	980.0
150.00	301.0
151.20	373.0
152.90	1048.0
154.00	740.0
155.00	2059.0
156.00	2797.0
157.00	537.0
157.90	694.0
158.90	327.0
159.90	1117.0
160.90	1547.0
161.90	595.0
163.10	182.0
164.00	171.0
164.90	1439.0
165.90	1017.0
167.00	7278.0
168.00	5113.0
168.90	723.0
170.00	213.0
170.90	244.0
171.90	624.0
173.00	990.0
173.90	1517.0
175.00	2651.0
176.00	900.0
177.00	1519.0
178.00	460.0
179.00	4945.0
180.00	3937.0
180.90	1891.0
181.90	315.0
182.40	270.0
184.00	469.0
185.00	2623.0
186.00	19752.0
187.00	6343.0
187.90	909.0
189.00	1302.0
189.80	202.0
190.90	1235.0
192.00	2187.0
193.00	2408.0
194.00	533.0
194.90	197.0
196.00	4046.0
197.00	815.0
197.90	150080.0
198.90	9542.0
200.10	678.0
201.20	847.0
201.70	366.0
202.90	1019.0
204.00	5370.0
205.00	9635.0
206.00	41272.0
207.00	8191.0
208.00	2219.0
209.00	908.0
210.00	856.0
211.00	1611.0
211.80	303.0
212.90	141.0
213.70	43.0
214.90	604.0
215.90	933.0
217.00	11542.0
218.00	1255.0
219.00	123.0
219.80	279.0
221.00	6698.0
221.90	1574.0
223.00	2752.0
224.00	24128.0
225.00	6116.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

226.00	981.0
227.00	10365.0
227.90	1361.0
229.00	2135.0
230.00	239.0
231.00	970.0
231.80	64.0
232.90	233.0
234.10	471.0
234.90	650.0
235.90	492.0
236.90	1111.0
237.80	107.0
239.00	340.0
239.90	398.0
240.90	569.0
241.90	1462.0
243.10	1532.0
244.00	19640.0
245.00	2634.0
246.00	4228.0
247.00	670.0
247.80	156.0
249.00	815.0
249.90	197.0
251.00	266.0
251.90	184.0
253.00	673.0
254.00	948.0
255.00	106032.0
256.00	14284.0
257.00	1231.0
258.00	6065.0
259.00	919.0
259.80	109.0
260.80	159.0
261.70	18.0
262.80	90.0
264.00	242.0
265.00	2406.0
266.00	454.0
267.00	262.0
267.80	26.0
268.80	46.0
269.90	72.0
270.90	207.0
272.00	245.0
272.90	3270.0
274.00	8310.0
275.00	46568.0
276.00	5719.0
276.90	3896.0
277.90	920.0
278.90	185.0
279.70	12.0
279.90	11.0
281.00	986.0
281.90	341.0
283.00	621.0
283.80	444.0
284.90	849.0
285.90	141.0
287.10	6.0
287.90	12.0
288.90	83.0
290.10	193.0
290.90	121.0
292.00	214.0
292.90	1142.0
293.90	383.0
295.10	469.0
296.00	14704.0
297.00	1856.0
297.80	145.0
299.30	12.0
299.90	8.0
300.80	278.0
301.80	310.0
303.00	1877.0
304.10	412.0
305.10	16.0
305.80	10.0
306.70	20.0
307.80	224.0
308.90	182.0
309.90	188.0
310.80	14.0
311.70	27.0
312.90	148.0
313.90	788.0
314.90	2018.0
316.00	993.0
316.90	210.0
317.70	11.0
317.80	11.0
318.90	14.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

319.90	53.0
321.00	398.0
322.00	203.0
323.00	4299.0
324.00	943.0
325.10	70.0
326.00	170.0
326.90	1061.0
327.80	453.0
328.60	79.0
329.10	62.0
329.90	21.0
332.00	324.0
332.90	669.0
334.00	3116.0
335.00	946.0
336.10	97.0
336.80	6.0
337.80	3.0
339.00	121.0
339.90	62.0
341.00	779.0
342.00	259.0
342.70	89.0
344.40	16.0
345.90	1064.0
346.90	175.0
347.70	54.0
348.80	1.0
349.20	2.0
350.90	78.0
352.00	1370.0
353.00	988.0
354.00	1496.0
354.90	491.0
356.10	139.0
357.10	152.0
357.90	32.0
359.00	172.0
360.10	42.0
360.60	8.0
361.60	12.0
362.30	14.0
362.60	12.0
363.10	19.0
364.90	8255.0
365.90	1205.0
366.80	104.0
367.50	4.0
367.90	6.0
368.50	4.0
369.10	52.0
370.00	281.0
370.90	518.0
372.00	2686.0
373.00	582.0
373.90	80.0
374.50	1.0
376.10	6.0
377.10	88.0
378.00	15.0
379.00	11.0
380.80	6.0
381.60	12.0
383.00	537.0
384.00	238.0
385.00	86.0
385.90	6.0
386.80	15.0
388.10	11.0
388.90	7.0
390.00	390.0
390.90	382.0
392.00	173.0
392.80	23.0
394.40	3.0
394.90	42.0
395.60	13.0
396.60	23.0
397.50	1.0
398.00	6.0
399.10	11.0
399.90	12.0
400.90	261.0
402.00	1393.0
403.00	2002.0
403.90	756.0
405.00	159.0
405.80	23.0
407.10	3.0
408.20	14.0
408.80	15.0
409.60	13.0
410.10	20.0
411.00	12.0
412.10	3.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

413.10	19.0
413.70	9.0
415.10	131.0
415.80	13.0
416.60	24.0
417.20	8.0
418.10	13.0
418.80	21.0
419.90	52.0
421.00	1415.0
422.00	1569.0
423.00	9625.0
424.00	2991.0
425.00	522.0
426.00	31.0
426.70	14.0
427.50	7.0
429.00	22.0
429.70	17.0
430.80	14.0
431.40	11.0
431.90	12.0
432.90	14.0
433.60	12.0
434.70	12.0
435.30	7.0
435.90	26.0
436.70	16.0
437.60	22.0
438.80	90.0
441.00	27128.0
442.00	178880.0
443.00	33064.0
444.00	2857.0
445.10	170.0
445.90	10.0
446.50	10.0
447.40	0.0
448.10	5.0
448.80	3.0
449.50	3.0
450.90	10.0
451.30	4.0
452.60	2.0
453.60	1.0
454.20	3.0
454.50	3.0
455.40	1.0
456.00	4.0
456.60	20.0
457.40	3.0
458.30	11.0
459.00	3.0
460.00	0.0
461.00	20.0
461.80	13.0
463.10	8.0
463.90	9.0
465.30	4.0
466.30	1.0
467.00	2.0
468.50	3.0
469.40	1.0
470.10	3.0
470.50	4.0
471.10	7.0
471.80	3.0
473.30	4.0
474.80	23.0
475.10	16.0
476.00	35.0
476.70	16.0
478.00	21.0
478.50	0.0
479.80	3.0
481.20	3.0
482.30	7.0
482.90	3.0
483.40	1.0
484.00	4.0
485.40	1.0
486.00	1.0
486.40	1.0
487.40	4.0
488.60	10.0
489.20	7.0
490.00	1.0
490.90	15.0
491.50	1.0
492.10	4.0
492.90	8.0
493.60	5.0
494.90	4.0
495.40	2.0
496.90	13.0
498.30	5.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694

499.10	2.0
499.90	10.0
500.60	1.0
501.40	10.0
502.50	2.0
503.30	14.0
504.10	9.0
504.70	4.0
506.10	16.0
507.10	6.0
507.90	5.0
508.90	1.0
509.50	17.0
511.00	2.0
511.70	16.0
512.40	3.0
513.30	1.0
514.10	4.0
514.70	9.0
515.60	4.0
517.40	12.0
518.20	0.0
518.80	3.0
520.40	4.0
520.80	8.0
521.90	2.0
522.50	12.0
523.70	3.0
525.20	7.0
526.40	2.0
526.80	6.0
527.60	2.0
528.10	2.0
528.60	2.0
529.20	1.0
530.00	10.0
530.70	0.0
531.40	3.0
532.10	1.0
533.10	3.0
534.80	16.0
536.30	3.0
537.80	4.0
539.60	6.0
540.90	4.0
542.50	5.0
544.00	2.0
544.80	12.0
545.80	5.0
546.70	13.0
547.40	17.0
548.80	18.0

Instrument :
BNA_P
ClientSampleId :
DFTPP694