
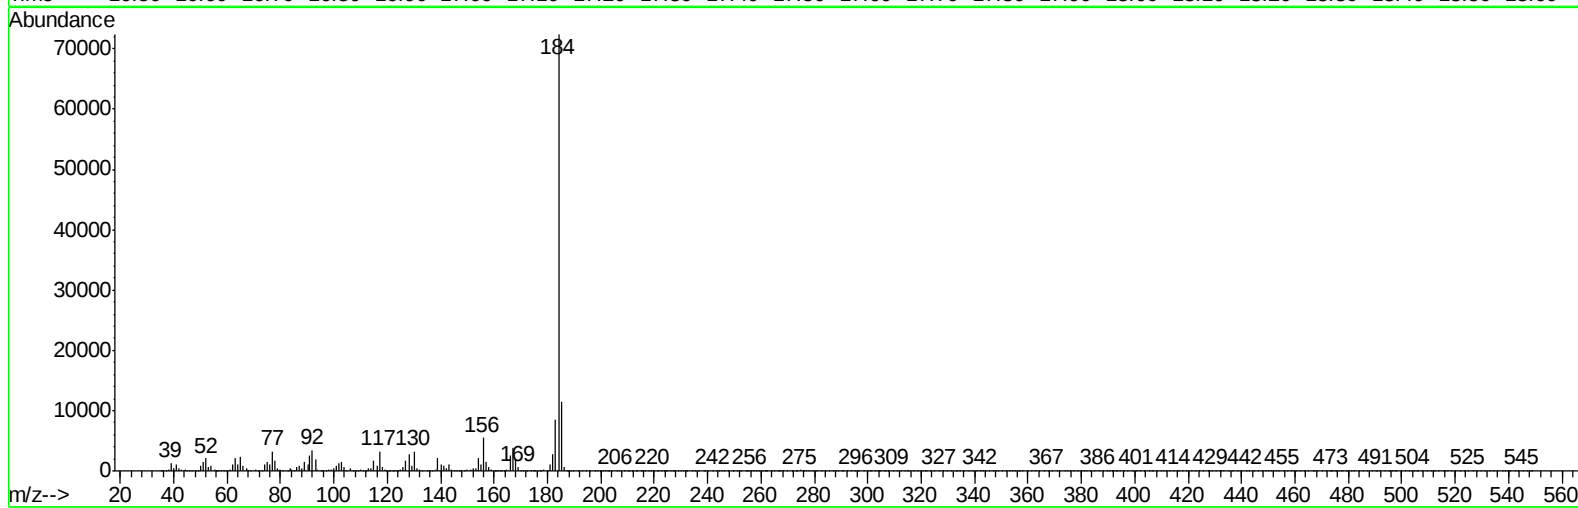


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122719\
Data File : BP001455.D
Acq On : 27 Dec 2019 12:48
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:21:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

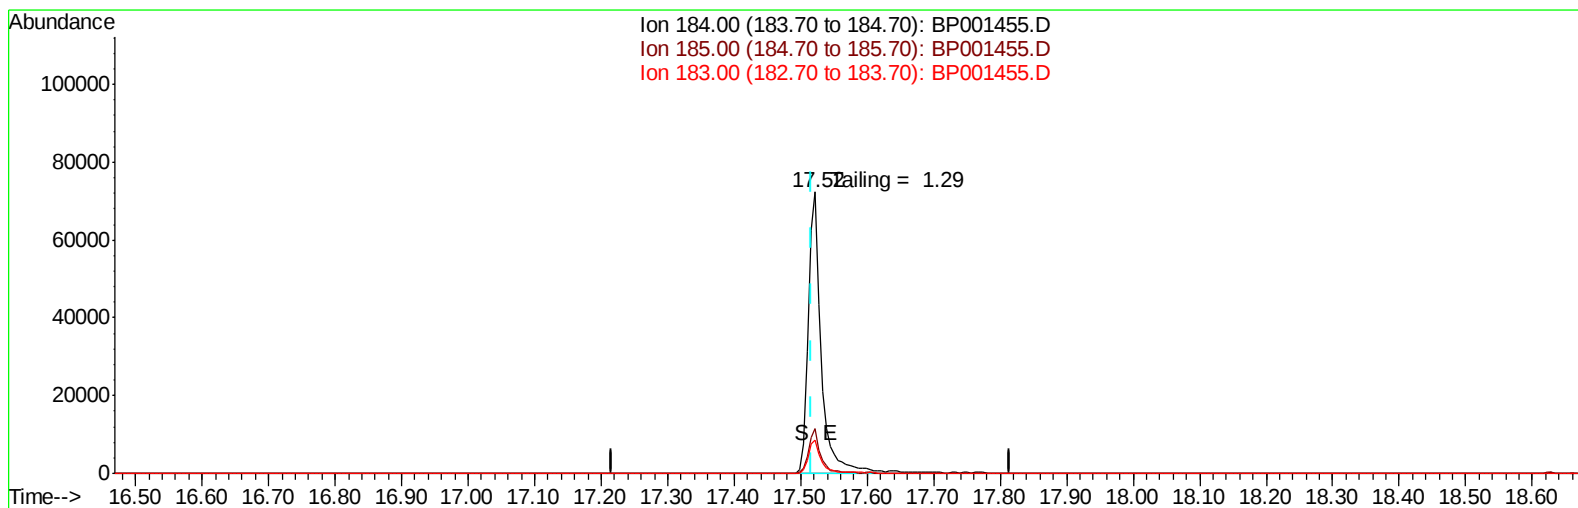

TIC: BP001455.D

(77) Benzidine



17.522min (+0.006) 288506.62ng

response 100799

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.94
183.00	12.00	11.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122719\
Data File : BP001455.D
Acq On : 27 Dec 2019 12:48
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:21:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

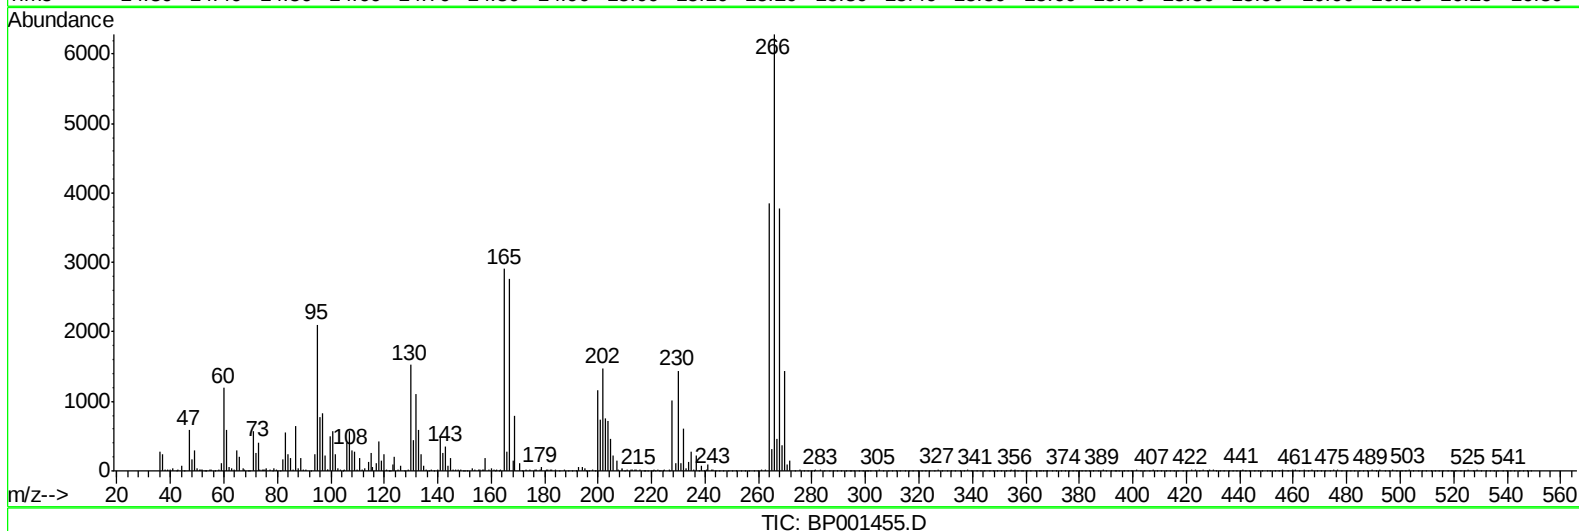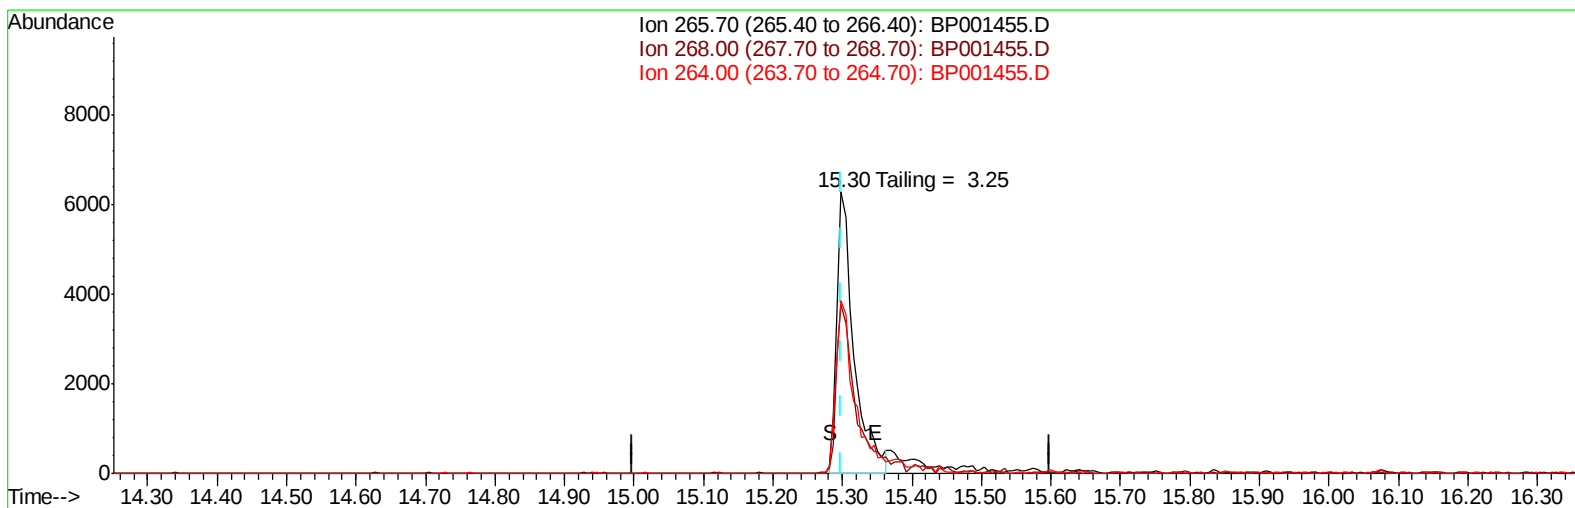

TIC: BP001455.D

(70) Pentachlorophenol (C)

15.298min (-0.000) 309108.72ng

response 10668

Ion	Exp%	Act%
265.70	100	100
268.00	71.20	60.15
264.00	63.50	66.27
0.00	0.00	0.00