

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122719\
 Data File : BP001466.D
 Acq On : 27 Dec 2019 19:14
 Operator : JU
 Sample : K6431-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FIELD-BLANK

Quant Time: Dec 28 05:25:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 16:04:49 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	21398	20.00	ng	0.00
21) Naphthalene-d8	10.32	136	76830	20.00	ng	0.00
39) Acenaphthene-d10	13.18	164	48719	20.00	ng	0.00
64) Phenanthrene-d10	15.57	188	101592	20.00	ng	0.00
76) Chrysene-d12	19.22	240	84626	20.00	ng	0.00
87) Perylene-d12	20.99	264	85520	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.20	112	108350	81.84	ng	0.00
7) Phenol-d6	7.75	99	98116	56.79	ng	0.00
23) Nitrobenzene-d5	9.17	82	160345	80.14	ng	0.00
42) 2,4,6-Tribromophenol	14.47	330	92206	151.38	ng	0.00
45) 2-Fluorobiphenyl	12.10	172	322332	83.66	ng	0.00
79) Terphenyl-d14	17.86	244	517588	104.76	ng	0.00
Target Compounds						
50) Dimethylphthalate	12.77	163	21796	5.453	ng	Qvalue # 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122719\
Data File : BP001466.D
Acq On : 27 Dec 2019 19:14
Operator : JU
Sample : K6431-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FIELD-BLANK

Quant Time: Dec 28 05:25:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

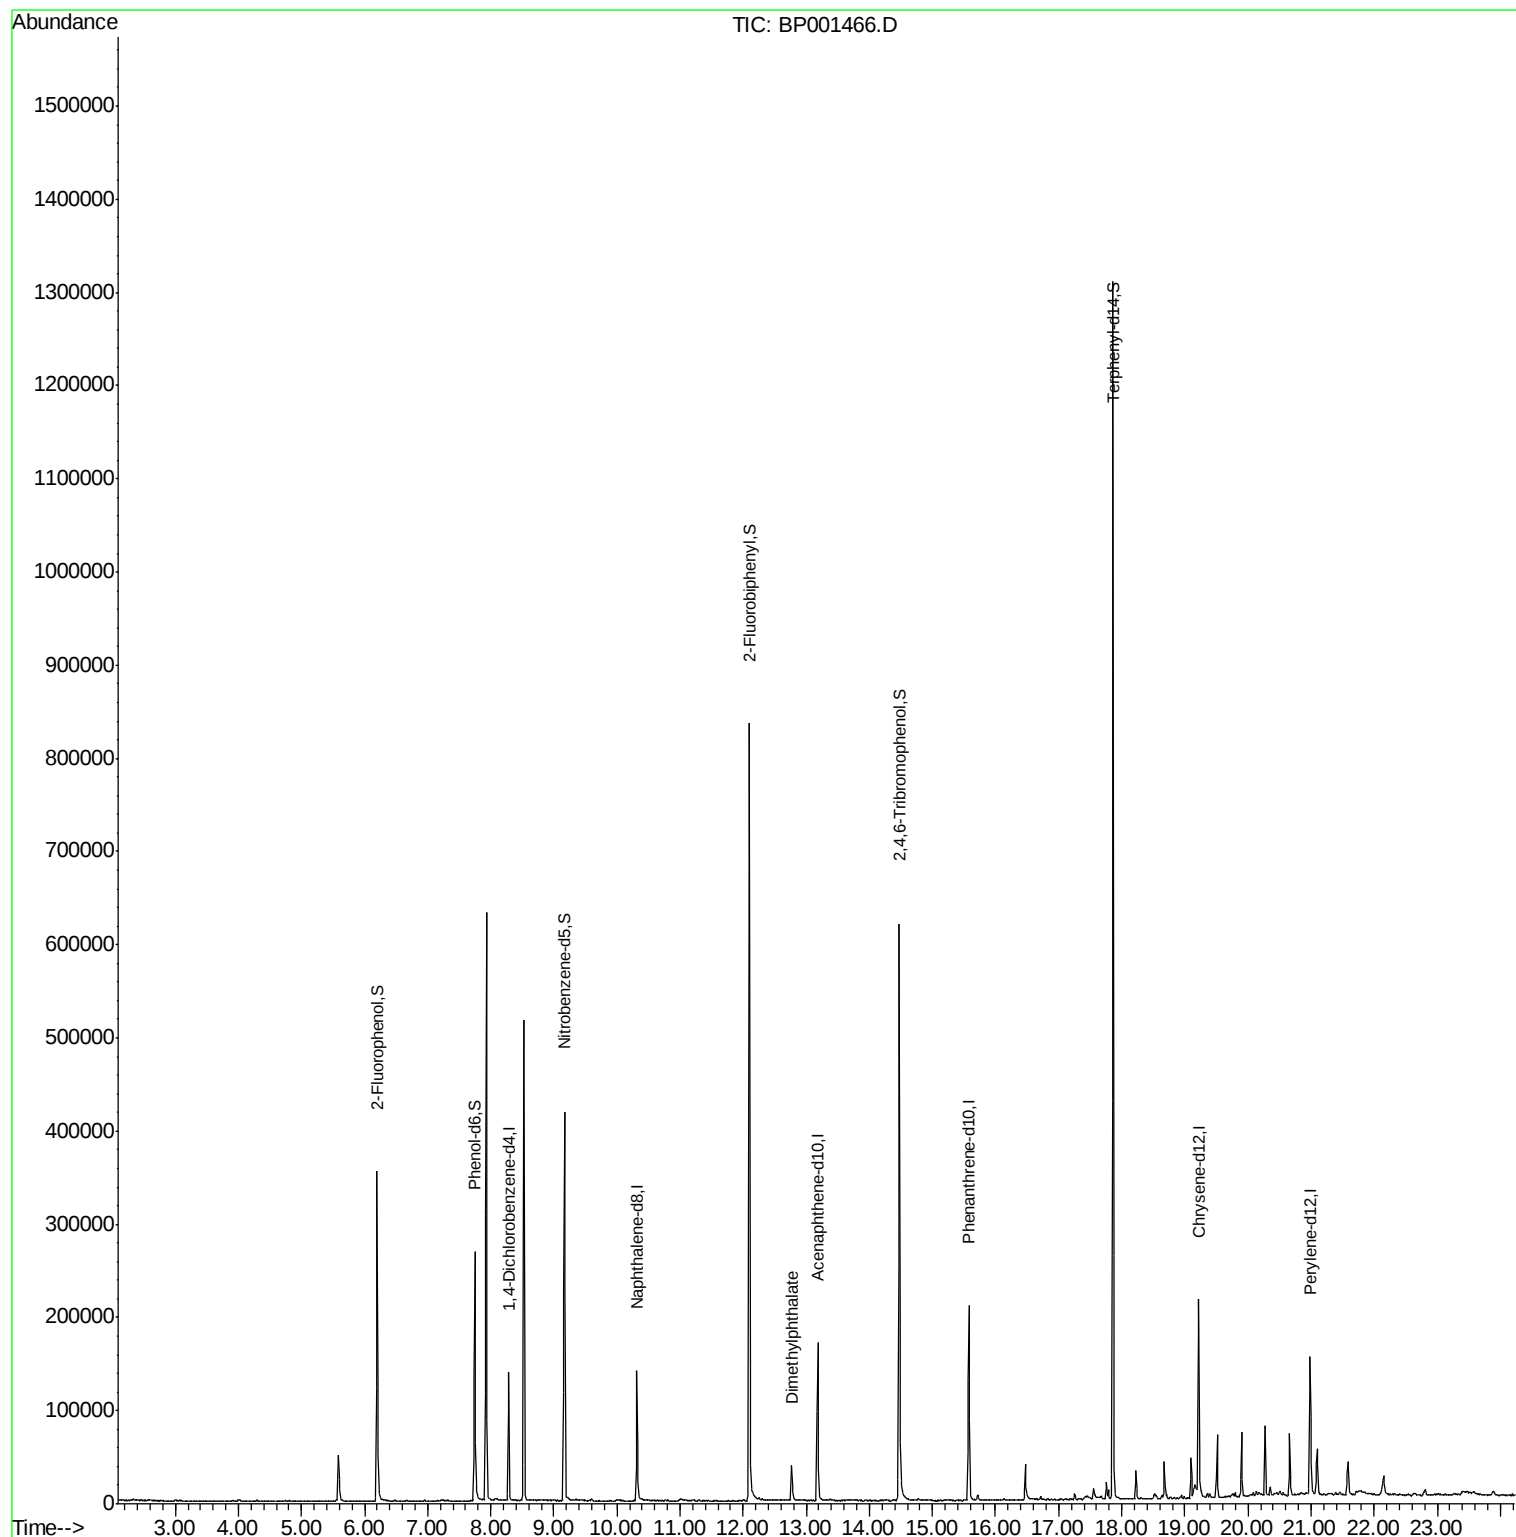

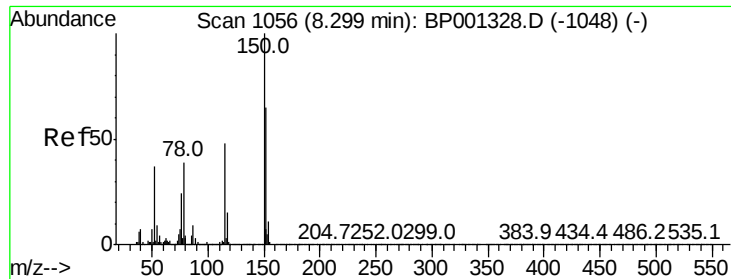

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.28 min Scan# 1053

Delta R.T. -0.01 min

Lab File: BP001466.D

Acq: 27 Dec 2019 19:14

Instrument :

BNA_P

ClientSampleId :

FIELD-BLANK


Tot Ion:152 Resp: 21398

Ion Ratio Lower Upper

152 100

150 167.8 127.0 190.6




115 74.3 56.1 84.1

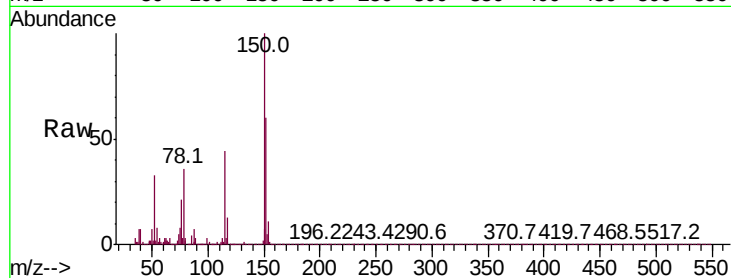

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

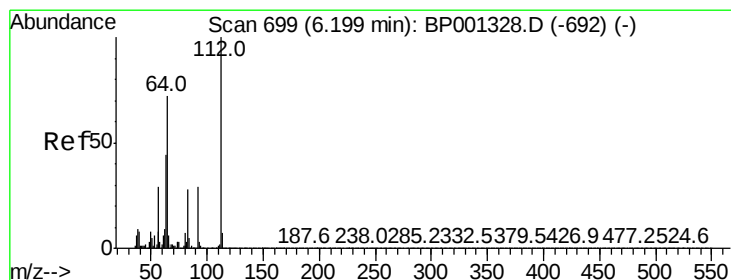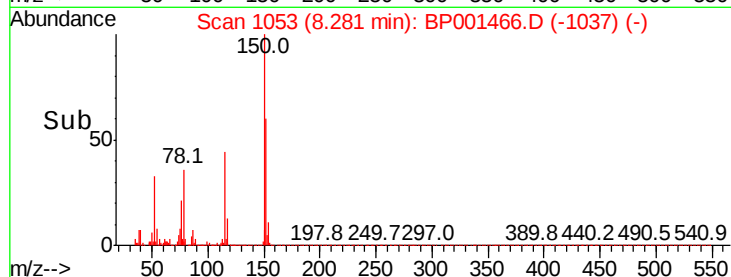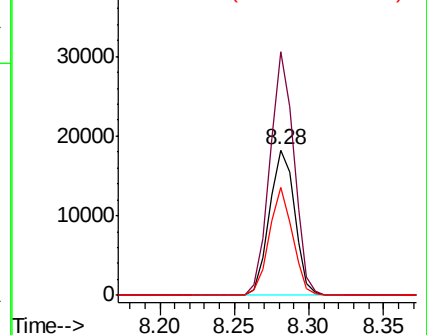

#5

2-Fluorophenol

Concen: 81.837 ng

RT: 6.20 min Scan# 699

Delta R.T. -0.00 min

Lab File: BP001466.D

Acq: 27 Dec 2019 19:14


Tgt Ion:112 Resp: 108350

Ion Ratio Lower Upper

112 100

64 64.7 53.9 80.9



63 41.3 33.4 50.0

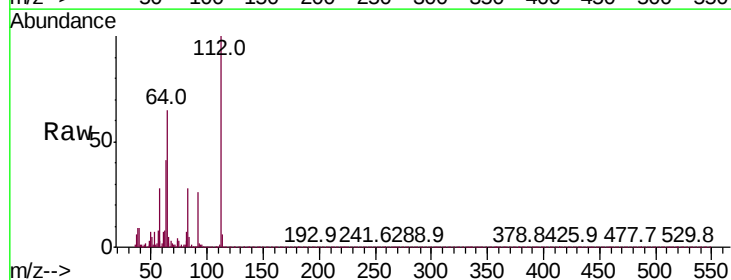


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

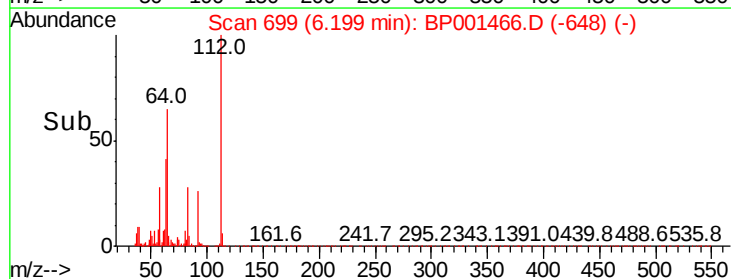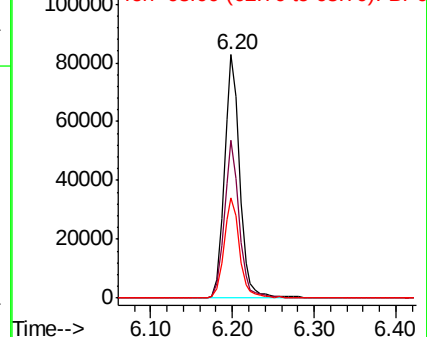

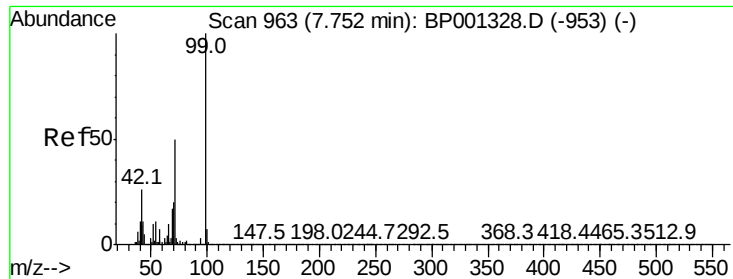

#7

Phenol-d6

Concen: 56.793 ng

RT: 7.75 min Scan# 962

Delta R.T. -0.01 min

Lab File: BP001466.D

Acq: 27 Dec 2019 19:14

Instrument :

BNA_P

ClientSampled :

FIELD-BLANK


Tot Ion: 99 Resp: 98116

Ion Ratio Lower Upper

99 100

42 24.9 20.8 31.2




71 47.7 38.2 57.4

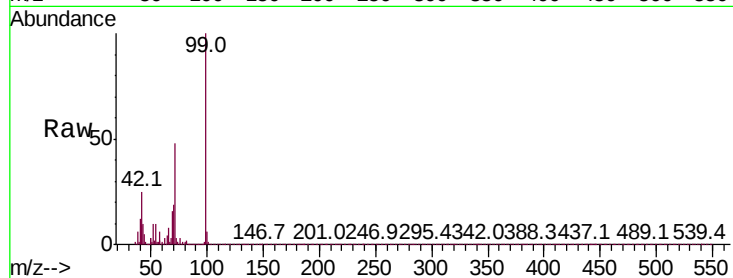

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

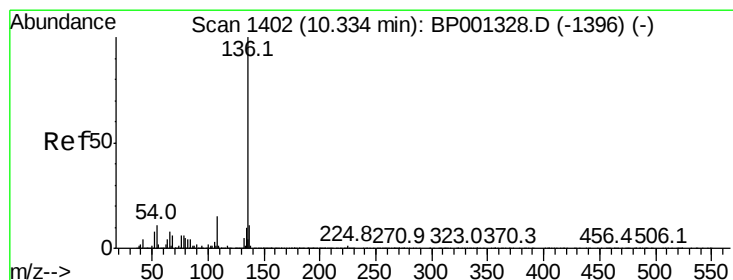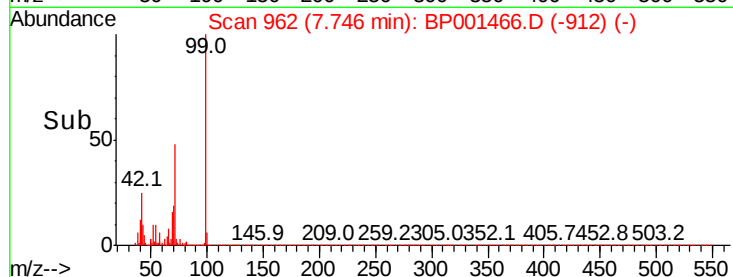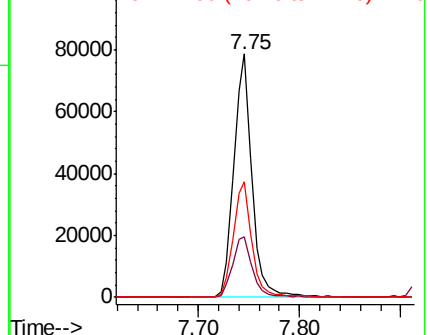

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.32 min Scan# 1399

Delta R.T. -0.01 min

Lab File: BP001466.D

Acq: 27 Dec 2019 19:14

Tgt Ion: 136 Resp: 76830


Ion Ratio Lower Upper

136 100

137 11.3 9.0 13.4

54 9.9 7.3 10.9

68 5.1 3.8 5.6


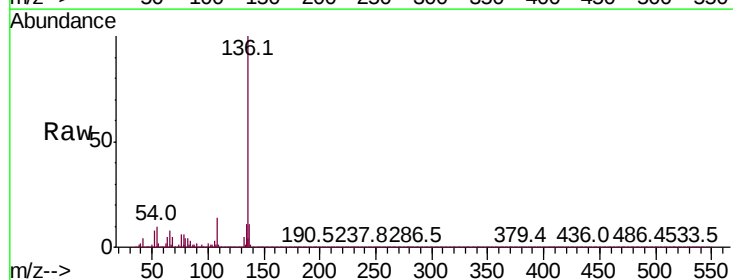



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



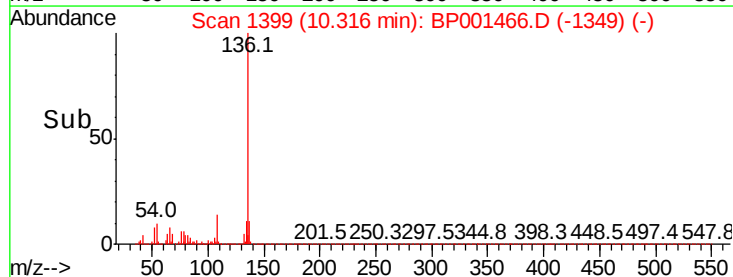
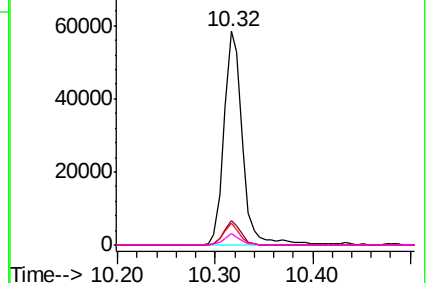


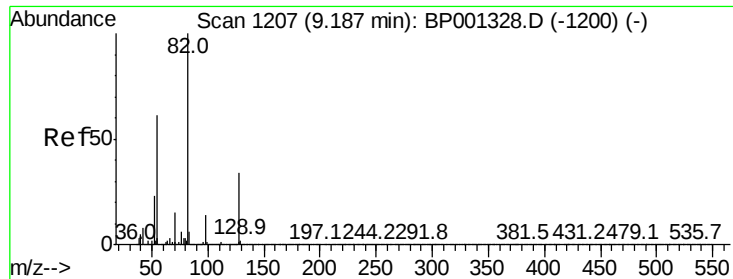

#23
Nitrobenzene-d5
Concen: 80.144 ng
RT: 9.17 min Scan# 1204
Delta R.T. -0.01 min
Lab File: BP001466.D
Acq: 27 Dec 2019 19:14




Instrument :
BNA_P
ClientSampleId :
FIELD-BLANK


Tot Ion	82	Resp	160345
Ion Ratio	100	Lower	Upper
128	36.9	27.4	41.0
54	60.7	47.5	71.3

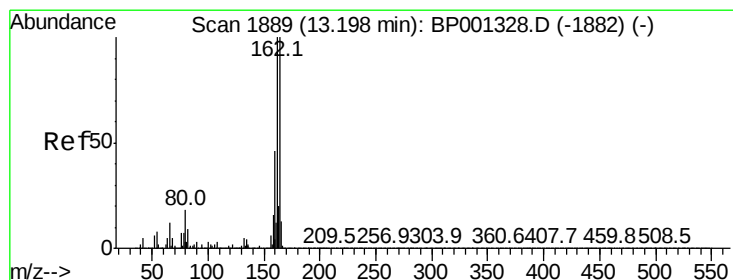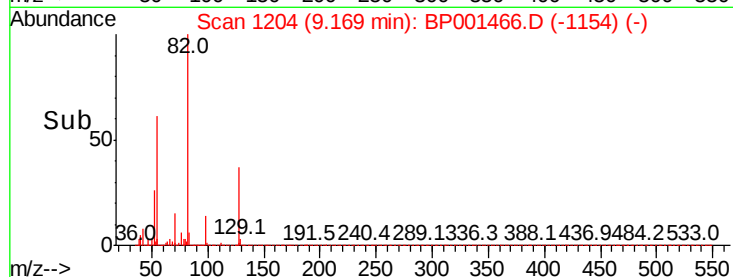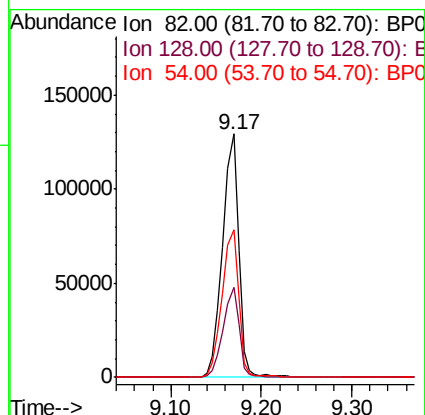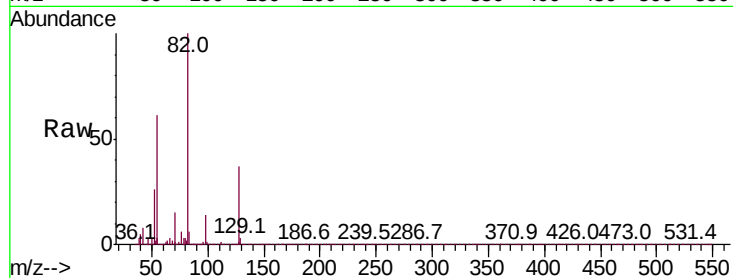

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 13.18 min Scan# 1886
Delta R.T. -0.00 min
Lab File: BP001466.D
Acq: 27 Dec 2019 19:14

Tgt Ion	164	Resp	48719
Ion Ratio	100	Lower	Upper
162	99.1	78.2	117.4
160	44.1	35.1	52.7

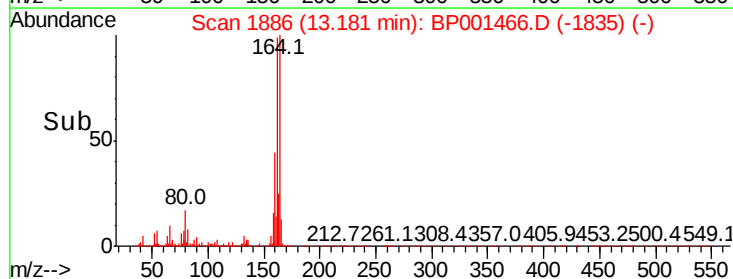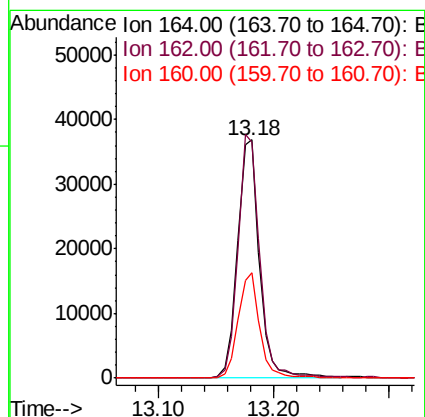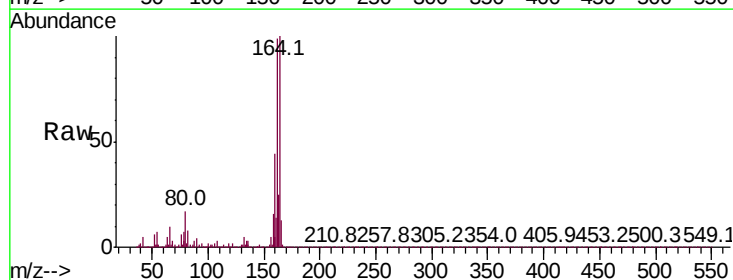


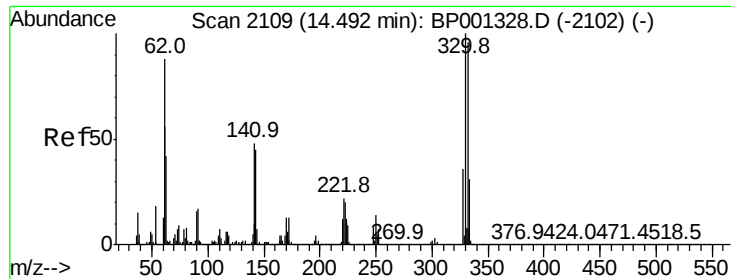




#42
 2,4,6-Tribromophenol
 Concen: 151.381 ng
 RT: 14.47 min Scan# 2106
 Delta R.T. -0.01 min
 Lab File: BP001466.D
 Acq: 27 Dec 2019 19:14

Instrument :
 BNA_P
 ClientSampleId :
 FIELD-BLANK

Tot Ion:330 Resp: 92206
 Ion Ratio Lower Upper
 330 100
 332 96.9 78.3 117.5
 141 38.5 26.8 40.2

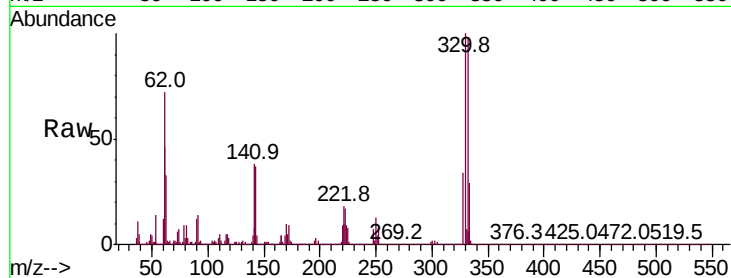


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

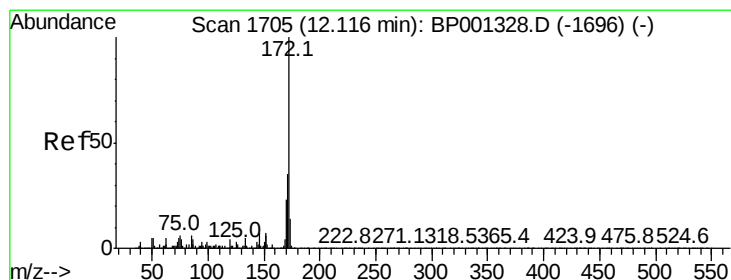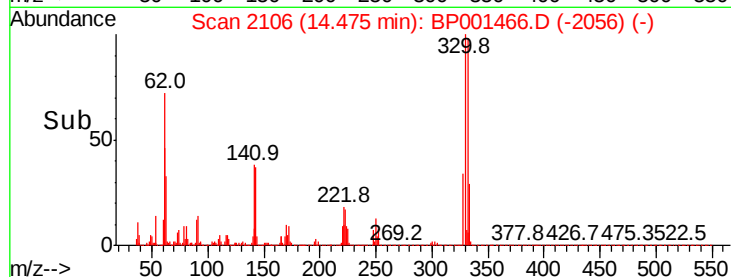
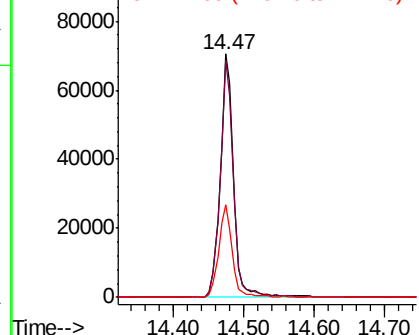



#45
 2-Fluorobiphenyl
 Concen: 83.660 ng
 RT: 12.10 min Scan# 1702
 Delta R.T. -0.00 min
 Lab File: BP001466.D
 Acq: 27 Dec 2019 19:14

Tgt Ion:172 Resp: 322332
 Ion Ratio Lower Upper
 172 100
 171 33.8 27.4 41.0
 170 22.3 18.2 27.4

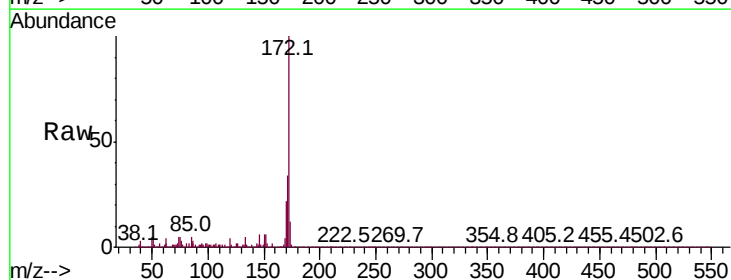

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

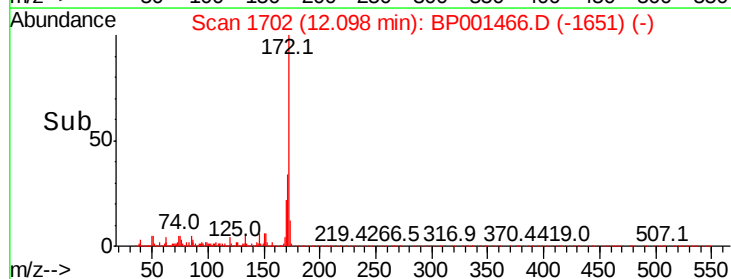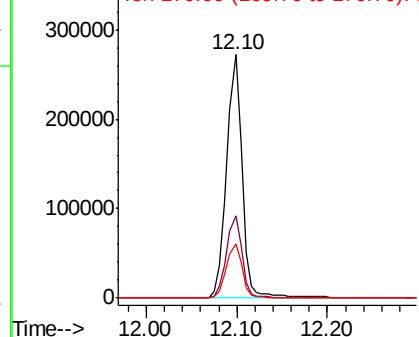

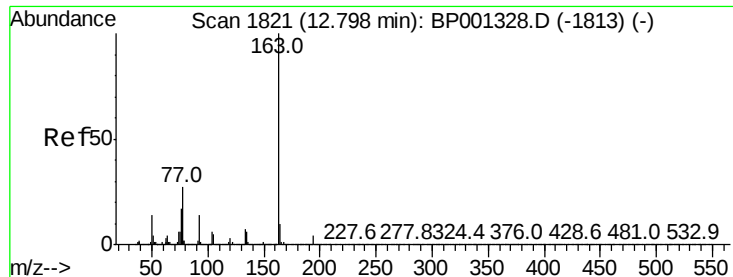

#50

Dimethylphthalate

Concen: 5.453 ng

RT: 12.77 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BP001466.D

Acq: 27 Dec 2019 19:14

Instrument :

BNA_P

ClientSampleId :

FIELD-BLANK


Tot Ion:163 Resp: 21796

Ion Ratio Lower Upper

163 100

194 4.9 3.2 4.8#




164 10.5 7.7 11.5

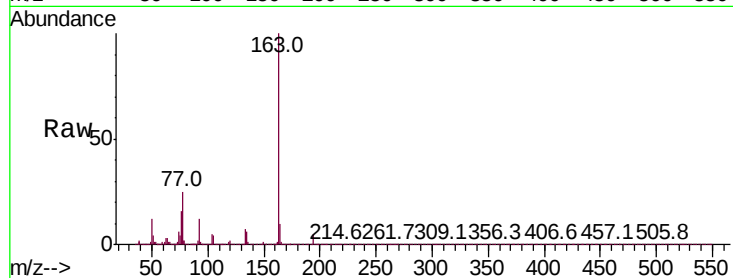

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

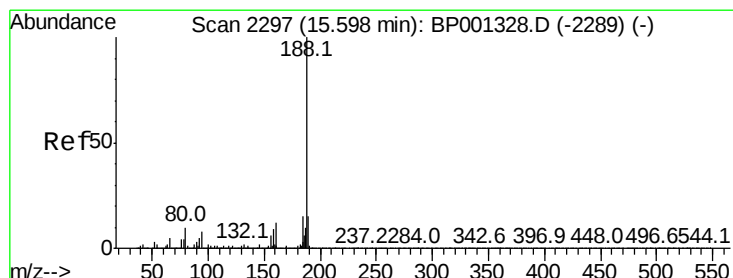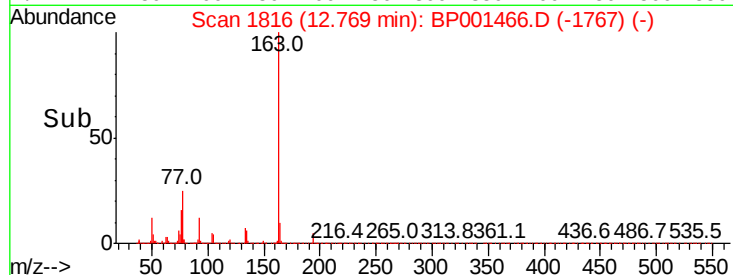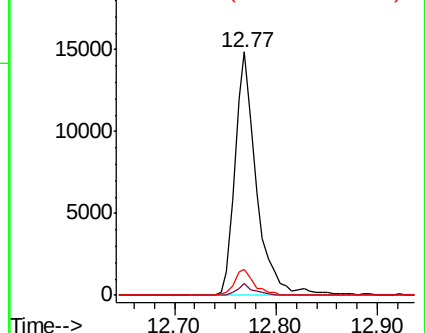

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.57 min Scan# 2293

Delta R.T. -0.01 min

Lab File: BP001466.D

Acq: 27 Dec 2019 19:14


Tgt Ion:188 Resp: 101592

Ion Ratio Lower Upper

188 100

94 6.8 5.8 8.8



80 7.3 5.7 8.5

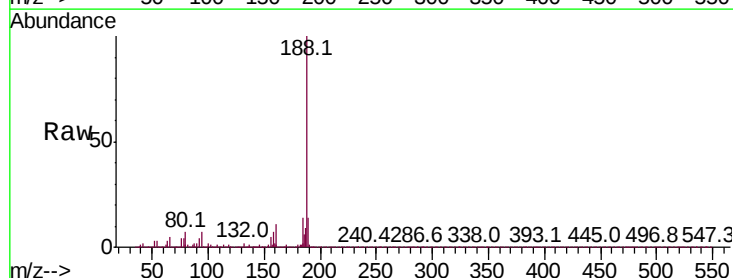


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0



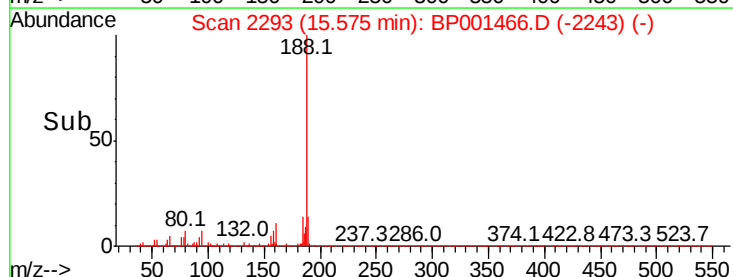
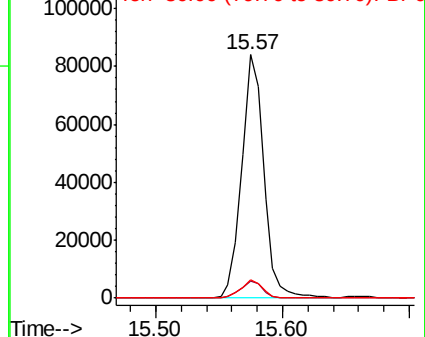


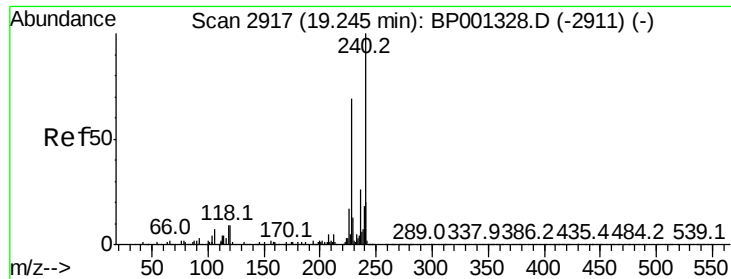

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 19.22 min Scan# 2913
 Delta R.T. -0.01 min
 Lab File: BP001466.D
 Acq: 27 Dec 2019 19:14




Instrument :
 BNA_P
 ClientSampleId :
 FIELD-BLANK


Tot Ion:240 Resp: 84626
 Ion Ratio Lower Upper
 240 100
 120 7.1 6.2 9.2
 236 25.9 20.2 30.2

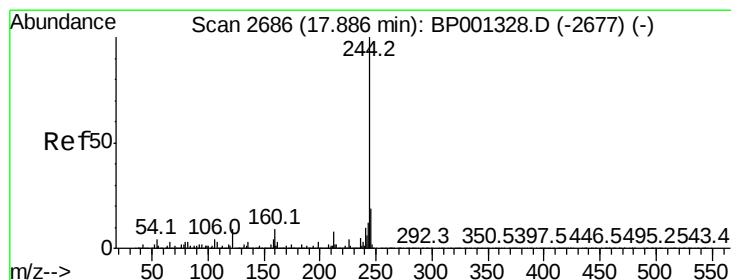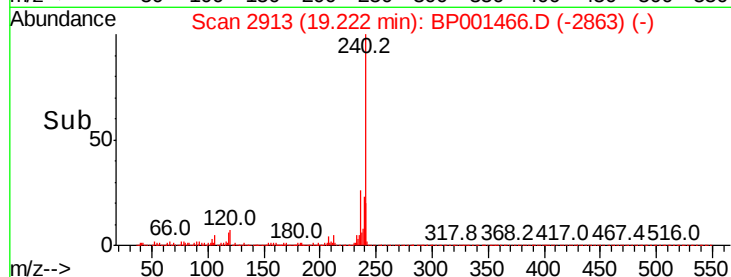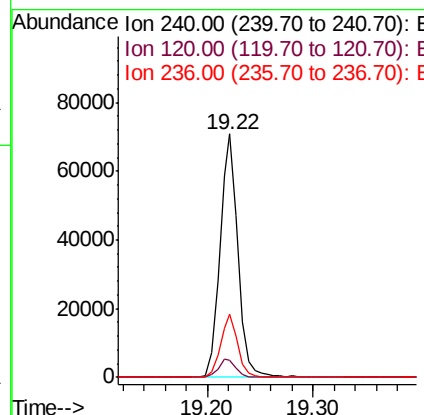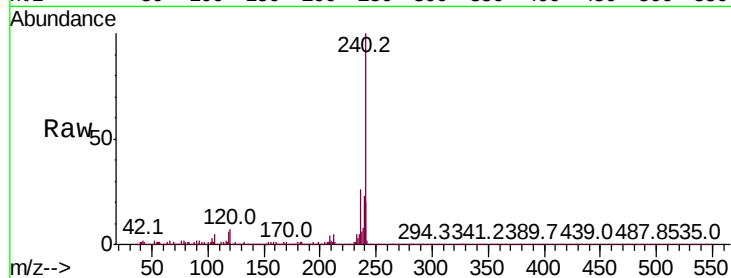

#79
 Terphenyl-d14
 Concen: 104.756 ng
 RT: 17.86 min Scan# 2682
 Delta R.T. -0.01 min
 Lab File: BP001466.D
 Acq: 27 Dec 2019 19:14

Tgt Ion:244 Resp: 517588
 Ion Ratio Lower Upper
 244 100
 212 7.6 5.8 8.8
 122 8.8 6.4 9.6

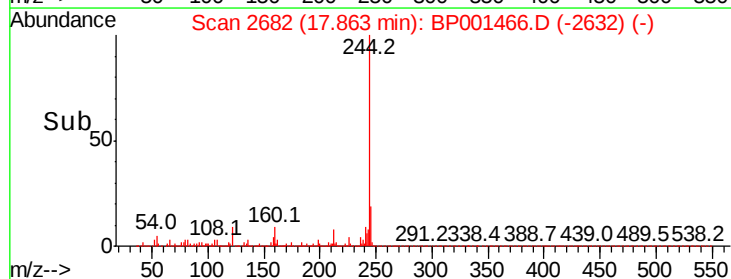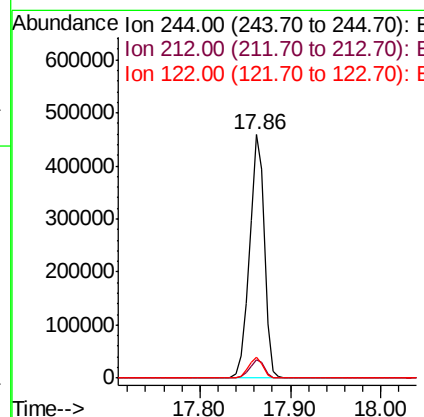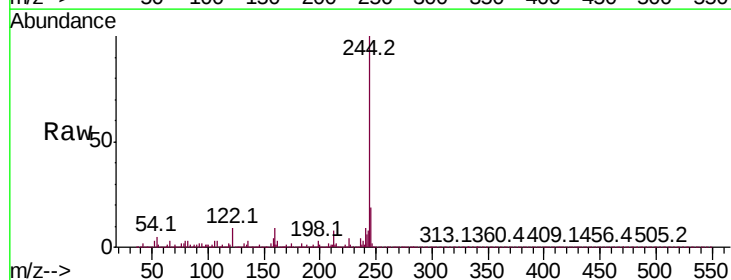


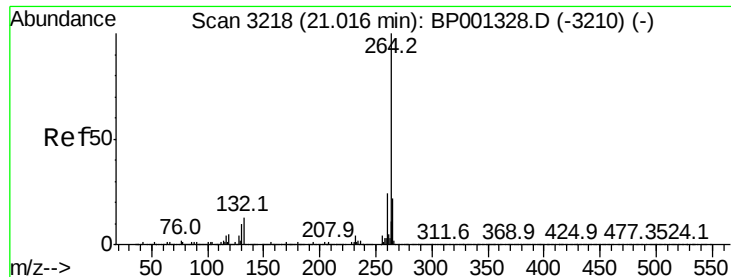

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 20.99 min Scan# 3213
 Delta R.T. -0.01 min
 Lab File: BP001466.D
 Acq: 27 Dec 2019 19:14

Instrument :
 BNA_P
 ClientSampleId :
 FIELD-BLANK

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.0	28.4
265	21.8	17.0	25.4

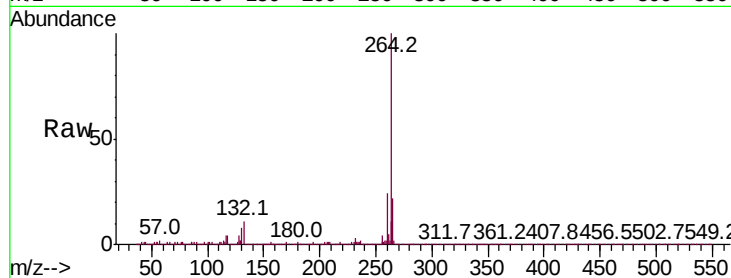

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

