


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122719\
 Data File : BP001455.D
 Acq On : 27 Dec 2019 12:48
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 16:04:49 2019

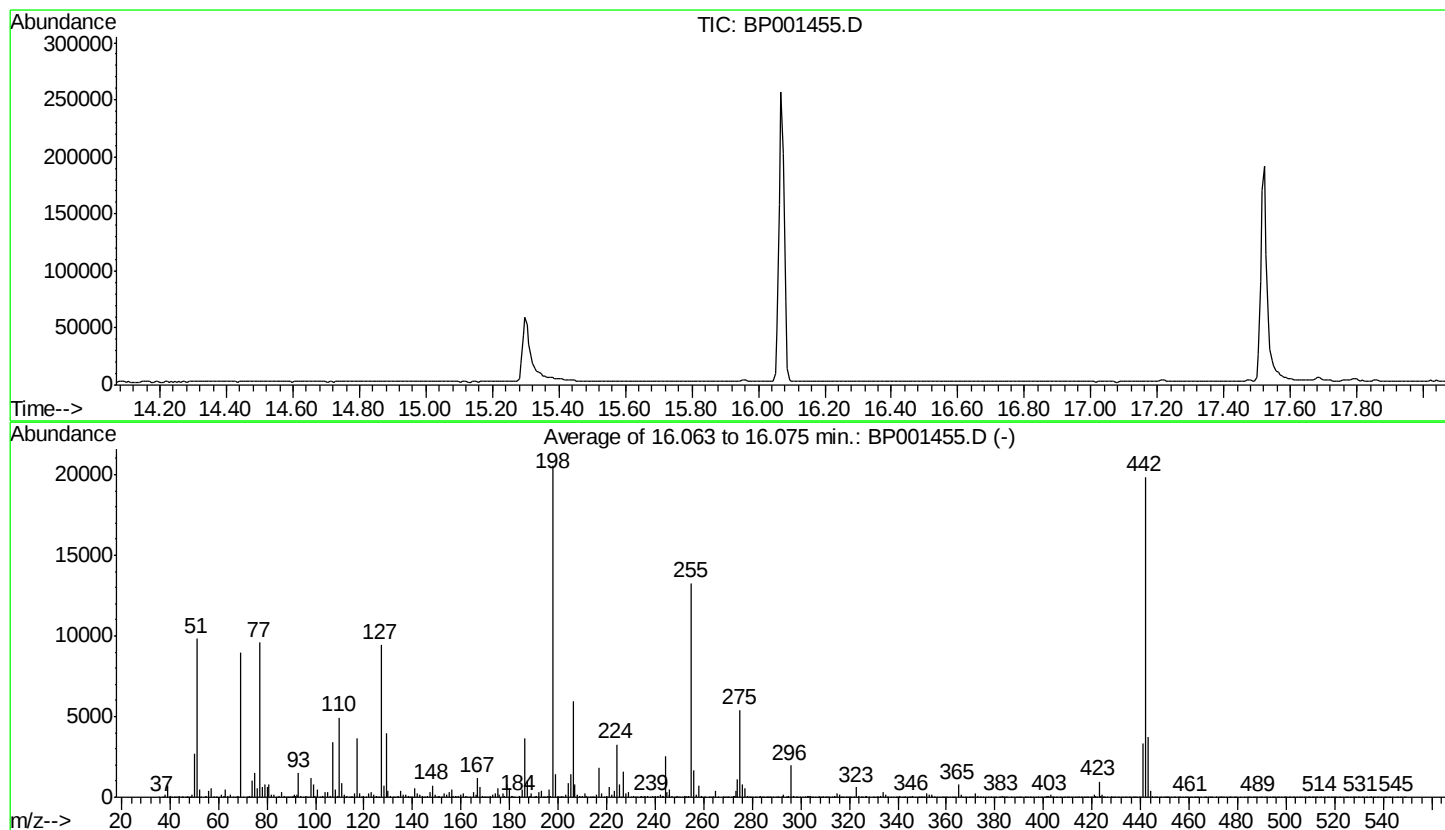

AutoFind: Scans 2376, 2377, 2378; Background Corrected with Scan 2370

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	9803	PASS
68	69	0.00	2	1.3	114	PASS
69	198	0.00	100	43.8	9004	PASS
70	69	0.00	2	0.3	29	PASS
127	198	10	80	46.0	9451	PASS
197	198	0.00	2	0.5	103	PASS
198	198	100	100	100.0	20549	PASS
199	198	5	9	6.9	1409	PASS
275	198	10	60	26.4	5435	PASS
365	198	1	100	3.8	785	PASS
441	198	0.01	100	16.3	3346	PASS
442	198	50	100	96.5	19840	PASS
443	442	15	24	18.7	3712	PASS