

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
 Data File : BP019118.D
 Acq On : 27 Dec 2023 17:15
 Operator : MA/JU
 Sample : PB158030BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK030

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	32	rBV	47293	56455	1.40%	0.162%
2	3.652	92	96	109	rBV	556505	792433	19.69%	2.268%
3	3.976	148	151	156	rVB	8152	10236	0.25%	0.029%
4	4.440	227	230	233	rBV5	2603	4058	0.10%	0.012%
5	6.981	651	662	675	rBV	586066	932369	23.17%	2.668%
6	7.146	684	690	702	rVB	498782	763588	18.98%	2.185%
7	7.340	715	723	731	rBV	595379	937054	23.29%	2.682%
8	7.805	795	802	811	rBV	434897	688302	17.11%	1.970%
9	8.522	917	924	937	rBV	681231	1123779	27.93%	3.216%
10	8.969	993	1000	1010	rBV	545485	874547	21.73%	2.503%
11	9.369	1067	1068	1075	rVB6	2959	5207	0.13%	0.015%
12	9.693	1115	1123	1140	rBV	425988	704272	17.50%	2.015%
13	10.228	1205	1214	1230	rBV	678245	1168936	29.05%	3.345%
14	10.605	1270	1278	1290	rBV	565657	933761	23.21%	2.672%
15	10.752	1292	1303	1319	rBV	657479	1170403	29.09%	3.349%
16	11.805	1475	1482	1487	rBV9	4544	10417	0.26%	0.030%
17	12.210	1546	1551	1556	rBV3	9385	18073	0.45%	0.052%
18	12.816	1649	1654	1659	rBV7	4805	9874	0.25%	0.028%
19	13.352	1740	1745	1752	rBV5	6628	10314	0.26%	0.030%
20	13.734	1805	1810	1815	rBV7	3922	6047	0.15%	0.017%
21	13.869	1826	1833	1841	rBV	1205326	1638637	40.72%	4.689%
22	14.146	1873	1880	1890	rBV	1366873	1948265	48.42%	5.575%
23	14.451	1925	1932	1941	rBV	823307	1217890	30.27%	3.485%
24	14.669	1962	1969	1984	rBV	425177	724959	18.02%	2.075%
25	14.769	1984	1986	1993	rVB7	4767	7333	0.18%	0.021%
26	14.869	2001	2003	2009	rVB7	2792	4575	0.11%	0.013%
27	15.246	2062	2067	2069	rBV6	3389	4470	0.11%	0.013%
28	15.451	2094	2102	2110	rBV	1721134	2499473	62.12%	7.153%
29	15.575	2117	2123	2138	rBV	483252	679737	16.89%	1.945%
30	15.693	2139	2143	2153	rVB3	8409	15032	0.37%	0.043%
31	16.240	2232	2236	2241	rVB3	7963	10731	0.27%	0.031%
32	16.510	2278	2282	2286	rBV7	2865	5678	0.14%	0.016%
33	16.887	2342	2346	2350	rBV7	3815	5337	0.13%	0.015%
34	17.210	2394	2401	2410	rBV	1107271	1507403	37.46%	4.314%
35	17.310	2412	2418	2430	rVV	1877408	2690227	66.86%	7.699%
36	18.104	2548	2553	2559	rBV6	20757	39301	0.98%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019118.D
Acq On : 27 Dec 2023 17:15
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	19.134	2724	2728	2733	rBV	26528	35830	0.89%	0.103%
38	19.204	2736	2740	2743	rBV	23111	34061	0.85%	0.097%
39	19.345	2761	2764	2768	rBV4	18515	25430	0.63%	0.073%
40	19.557	2794	2800	2809	rBV	2658884	3488948	86.71%	9.985%
41	21.316	3094	3099	3110	rBV	1517804	1979109	49.19%	5.664%
42	23.527	3469	3475	3482	rBV2	2110902	4023804	100.00%	11.515%
43	23.680	3495	3501	3511	rVB	1101078	2137171	53.11%	6.116%




Sum of corrected areas: 34943526

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019118.D
Acq On : 27 Dec 2023 17:15
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

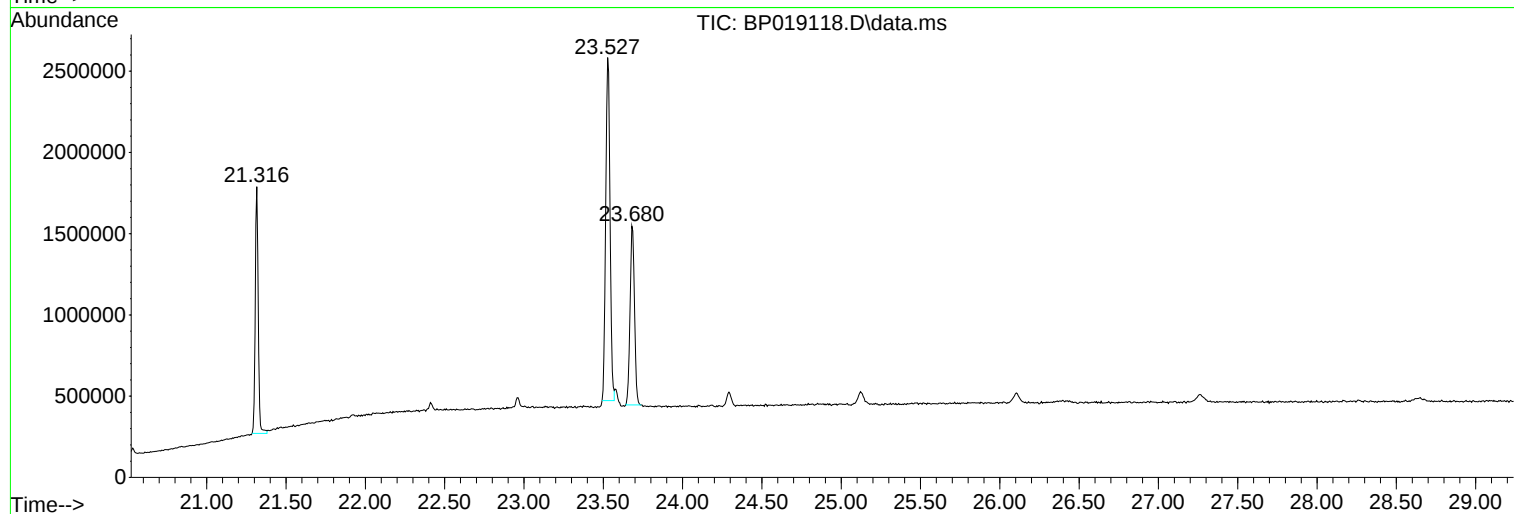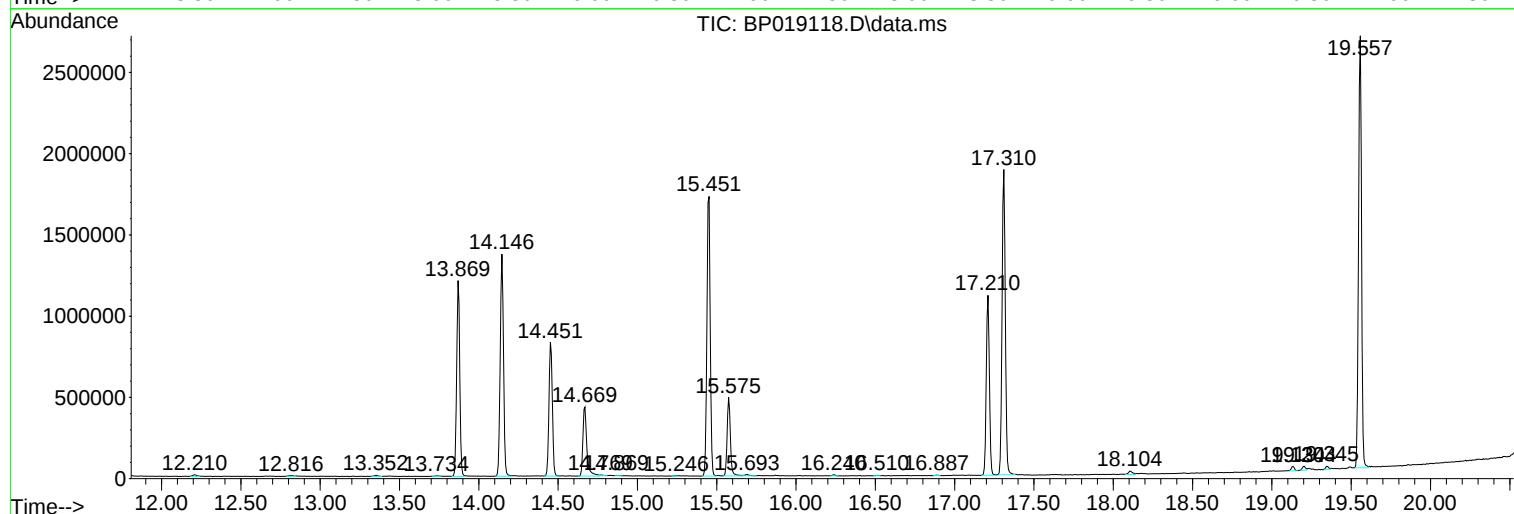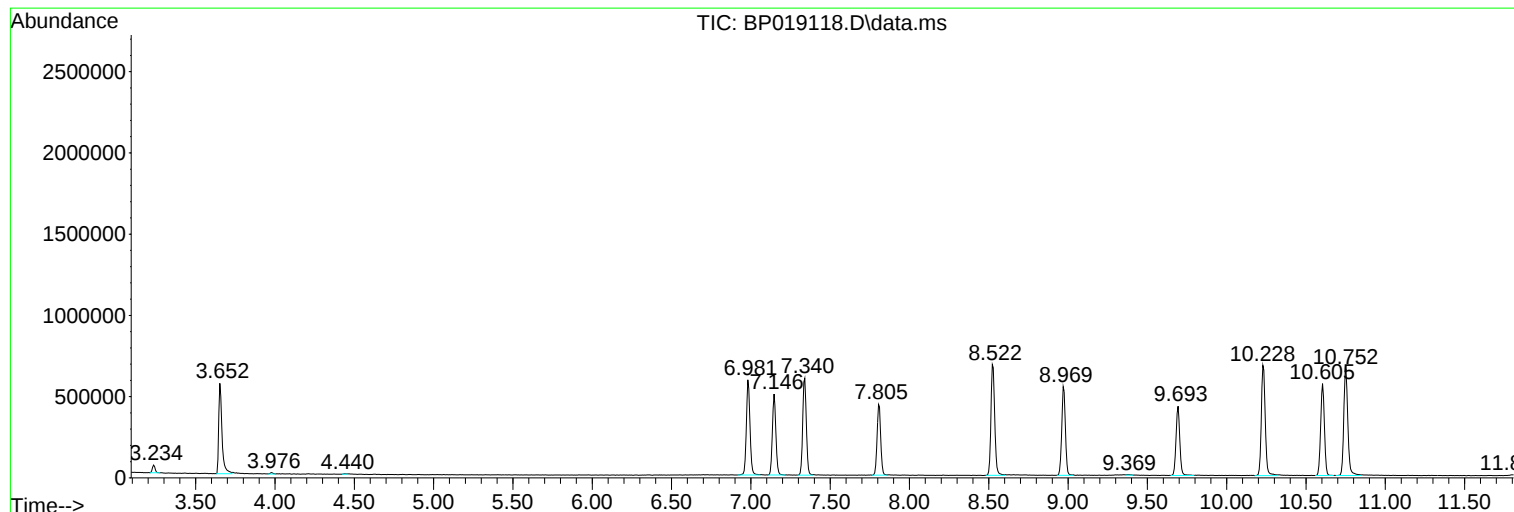

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019118.D
Acq On : 27 Dec 2023 17:15
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019118.D
Acq On : 27 Dec 2023 17:15
Operator : MA/JU
Sample : PB158030BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK030

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------