

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
 Data File : BP019120.D
 Acq On : 27 Dec 2023 18:23
 Operator : MA/JU
 Sample : 05976-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	30	rVB	28362	34346	1.40%	0.159%
2	3.658	94	97	113	rBV	160807	240558	9.77%	1.111%
3	3.981	148	152	155	rBV	6920	9524	0.39%	0.044%
4	4.211	187	191	199	rVB6	7273	11779	0.48%	0.054%
5	4.458	227	233	236	rBV4	5211	8606	0.35%	0.040%
6	4.623	259	261	265	rVB5	4658	4183	0.17%	0.019%
7	5.664	436	438	443	rVB6	1653	2699	0.11%	0.012%
8	6.370	555	558	563	rBV6	1687	2689	0.11%	0.012%
9	6.981	651	662	673	rBV	238769	399455	16.23%	1.845%
10	7.146	683	690	700	rVB	232925	359086	14.59%	1.658%
11	7.340	715	723	733	rBV	262359	419071	17.03%	1.935%
12	7.805	796	802	810	rBV	482631	772032	31.37%	3.565%
13	8.411	901	905	911	rBV7	1227	2511	0.10%	0.012%
14	8.528	917	925	937	rBV	283643	486782	19.78%	2.248%
15	8.969	993	1000	1012	rBV	232817	398705	16.20%	1.841%
16	9.293	1049	1055	1058	rBV6	1565	2945	0.12%	0.014%
17	9.358	1064	1066	1069	rVV3	2501	3902	0.16%	0.018%
18	9.381	1069	1070	1077	rVB7	3180	4715	0.19%	0.022%
19	9.693	1115	1123	1131	rBV	183177	297886	12.10%	1.376%
20	9.916	1160	1161	1169	rVB8	1818	3711	0.15%	0.017%
21	10.234	1204	1215	1231	rBV	289614	520150	21.13%	2.402%
22	10.605	1271	1278	1288	rBV	633491	1032006	41.93%	4.766%
23	10.752	1296	1303	1317	rBV	290619	529075	21.50%	2.443%
24	11.805	1474	1482	1487	rBV	3691	8971	0.36%	0.041%
25	12.216	1548	1552	1554	rVB5	2745	3704	0.15%	0.017%
26	12.669	1625	1629	1635	rBV9	1705	3702	0.15%	0.017%
27	12.816	1647	1654	1658	rBV9	4431	8609	0.35%	0.040%
28	13.357	1738	1746	1751	rBV6	10532	17752	0.72%	0.082%
29	13.434	1754	1759	1764	rVB8	1961	4043	0.16%	0.019%
30	13.734	1803	1810	1814	rBV8	4745	8561	0.35%	0.040%
31	13.869	1826	1833	1843	rBV	560408	766278	31.13%	3.539%
32	14.146	1873	1880	1890	rBV	608544	880404	35.77%	4.066%
33	14.357	1912	1916	1919	rVB6	2242	3182	0.13%	0.015%
34	14.451	1925	1932	1944	rBV	941968	1360167	55.26%	6.281%
35	14.669	1964	1969	1989	rBV	124472	259946	10.56%	1.200%
36	14.822	1993	1995	2000	rVB6	2627	3619	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
 Data File : BP019120.D
 Acq On : 27 Dec 2023 18:23
 Operator : MA/JU
 Sample : 05976-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	15.251	2064	2068	2074	rBV8	4480	7132	0.29%	0.033%
38	15.446	2094	2101	2113	rBV	842357	1191333	48.40%	5.502%
39	15.575	2117	2123	2133	rBV	167123	250553	10.18%	1.157%
40	15.687	2138	2142	2147	rVB6	3430	5827	0.24%	0.027%
41	16.010	2193	2197	2198	rBV3	2451	2475	0.10%	0.011%
42	16.240	2232	2236	2239	rVB6	3891	4659	0.19%	0.022%
43	17.022	2361	2369	2384	rBV	151631	241236	9.80%	1.114%
44	17.210	2394	2401	2411	rBV	1172554	1654197	67.21%	7.639%
45	17.310	2411	2418	2431	rVV	860100	1251762	50.86%	5.781%
46	18.104	2549	2553	2560	rBV3	32107	47042	1.91%	0.217%
47	19.128	2725	2727	2732	rVB4	12570	15215	0.62%	0.070%
48	19.345	2760	2764	2770	rBV5	34614	49528	2.01%	0.229%
49	19.551	2794	2799	2808	rBV	1170329	1596658	64.87%	7.373%
50	20.533	2963	2966	2970	rVB	70358	78277	3.18%	0.361%
51	21.316	3094	3099	3106	rBV	1615952	2120129	86.14%	9.791%
52	23.527	3469	3475	3481	rBV2	938005	1801357	73.19%	8.319%
53	23.680	3495	3501	3515	rVB	1217964	2461310	100.00%	11.367%




Sum of corrected areas: 21654044

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019120.D
Acq On : 27 Dec 2023 18:23
Operator : MA/JU
Sample : 05976-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

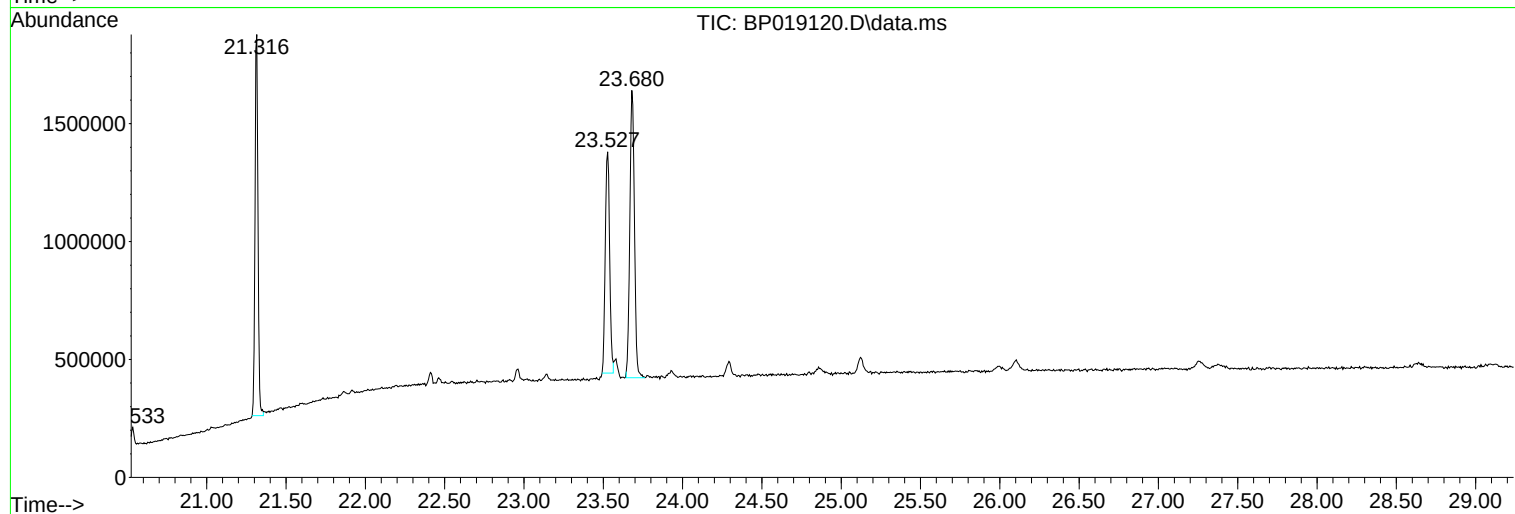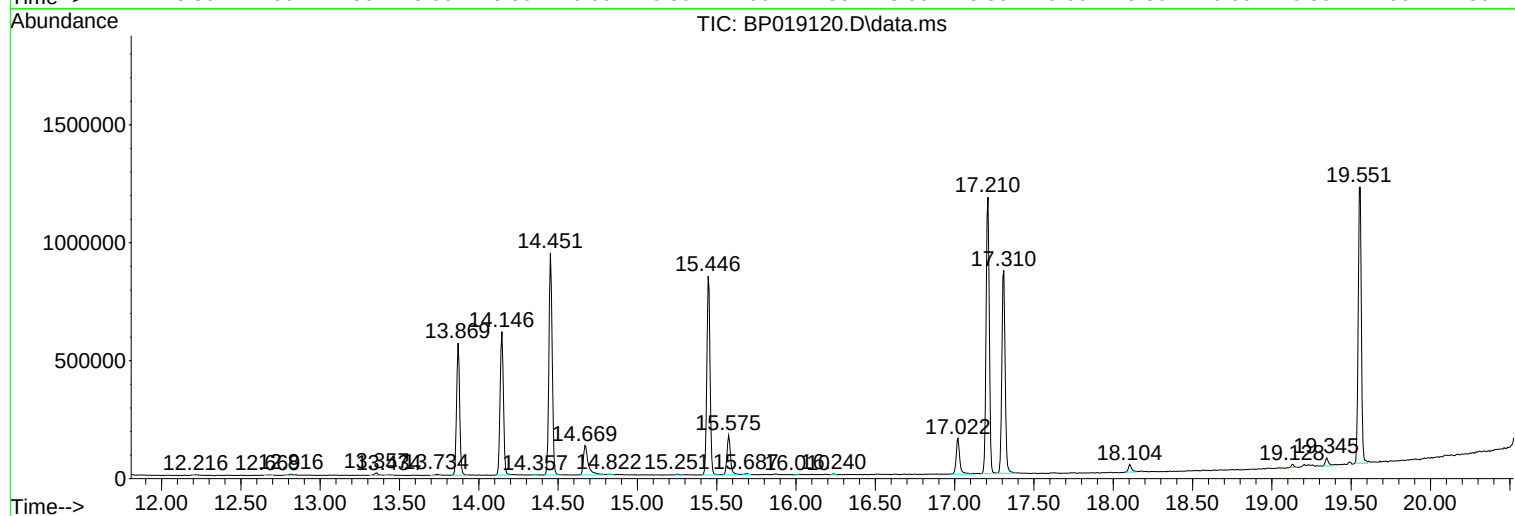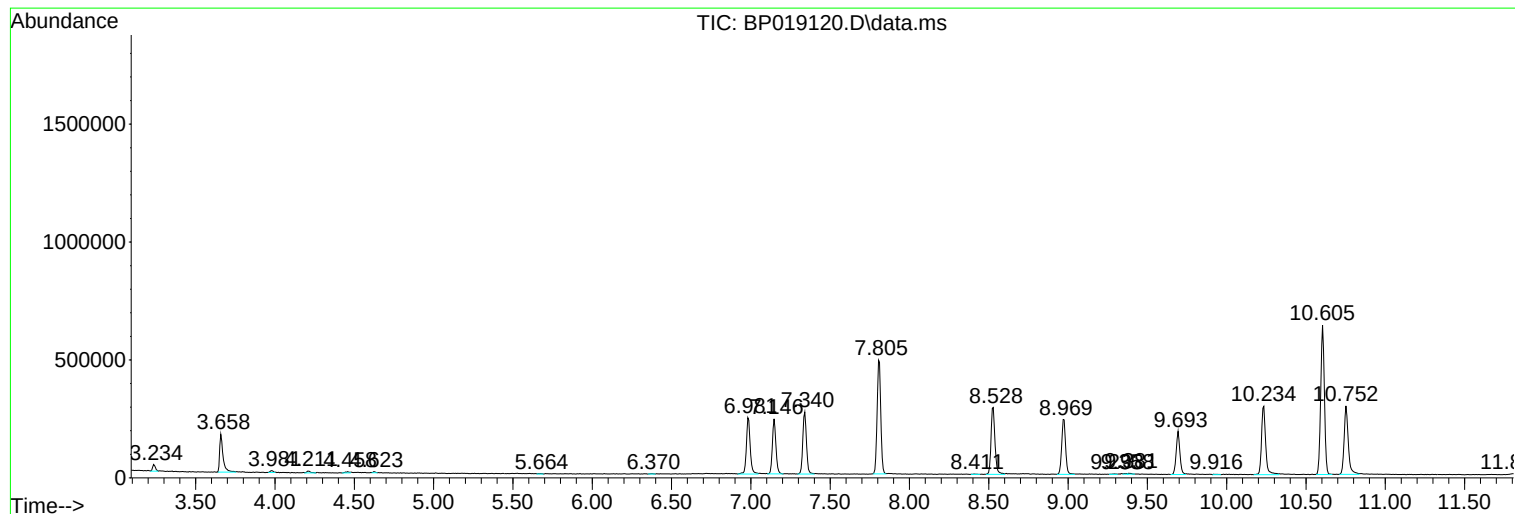

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019120.D
Acq On : 27 Dec 2023 18:23
Operator : MA/JU
Sample : 05976-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.022	2.92 ng/ul	241236	Phenanthrene-d10	17.210

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	90
2			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	70
3			2-propenoic acid, 2-methyl-, 2-[...]	269	C12H15NO4S	1000401-71-8	64
4			N-(2-Cyano-ethyl)-benzenesulfona...	210	C9H10N2O2S	002619-21-8	59
5			N-Benzenesulfonyloxy-2,2-bis(tri...	335	C10H7F6NO3S	055734-41-3	50

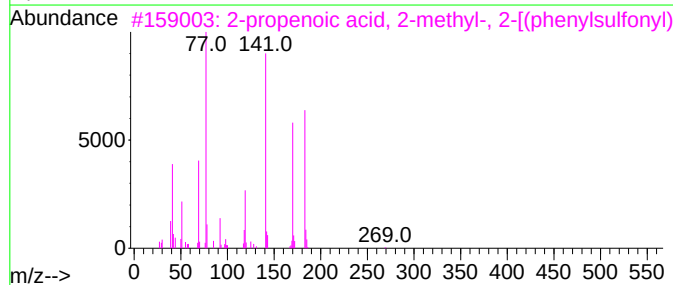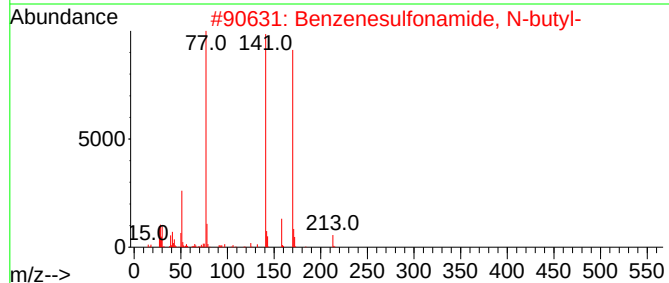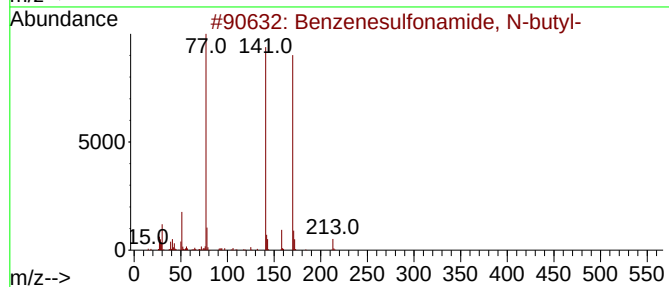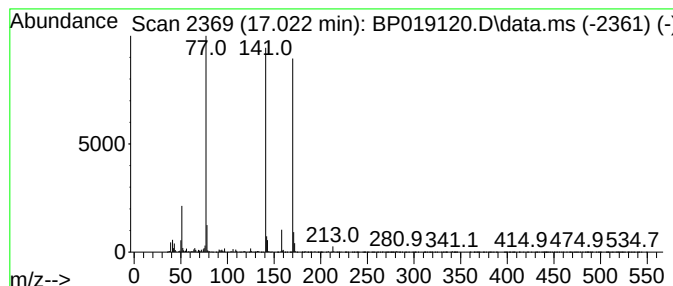

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122723\
Data File : BP019120.D
Acq On : 27 Dec 2023 18:23
Operator : MA/JU
Sample : 05976-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.022	2.9	ng/u1	241236	4	17.210	1654200	20.0