

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
 Data File : BP013347.D
 Acq On : 28 Dec 2022 11:32
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 29 00:16:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	501645	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	2227514	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	1561060	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	3597110	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	3079103	20.000	ng/u1	0.00
88) Perylene-d12	23.898	264	2514321	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	92439	7.879	ng/uL	0.00
4) Pyridine-d5	3.752	84	675150	20.257	ng/u1	0.00
7) Phenol-d5	7.093	99	812545	19.886	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	533134	21.630	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	640254	19.905	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	684470	20.444	ng/u1	0.00
21) Nitrobenzene-d5	9.105	128	328425	20.067	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	374688	20.336	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	733237	20.488	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	1044588	20.675	ng/u1	0.00
46) Dimethylphthalate-d6	13.987	166	2335863	19.470	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	2590588	19.651	ng/u1	0.00
54) 4-Nitrophenol-d4	14.787	143	413247	19.149	ng/u1	0.00
60) Fluorene-d10	15.575	176	1996551	19.671	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	419689	18.131	ng/u1	0.00
73) Anthracene-d10	17.439	188	3198716	19.711	ng/u1	0.00
81) Pyrene-d10	19.669	212	3759799	21.273	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.733	264	2458153	19.614	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.358	88	97943	7.997	ng/uL#	89
5) Pyridine	3.770	79	678901	20.496	ng/u1	93
6) Benzaldehyde	7.069	77	326838	20.428	ng/u1	97
8) Phenol	7.122	94	843481	20.417	ng/u1	94
10) Bis(2-Chloroethyl)ether	7.352	93	696031	20.527	ng/u1	95
12) 2-Chlorophenol	7.493	128	665549	20.177	ng/u1	96
13) 2-Methylphenol	8.381	108	643039	19.965	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.469	45	1076888	23.144	ng/u1	99
16) Acetophenone	8.763	105	1116178	21.743	ng/u1#	94
17) N-Nitroso-di-n-propyla...	8.746	70	585091	22.665	ng/u1	92
18) 4-Methylphenol	8.710	108	736386	20.641	ng/u1	98
19) Hexachloroethane	9.016	117	260093	19.732	ng/u1	97
22) Nitrobenzene	9.146	77	830958	21.637	ng/u1	96
23) Isophorone	9.675	82	1632490	21.022	ng/u1	98
25) 2-Nitrophenol	9.857	139	407909	20.432	ng/u1	91
26) 2,4-Dimethylphenol	9.916	107	814302	20.905	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.157	93	1019409	20.530	ng/u1	100
29) 2,4-Dichlorophenol	10.399	162	727646	20.756	ng/u1	99
30) Naphthalene	10.799	128	2302776	19.767	ng/u1	100
32) 4-Chloroaniline	10.910	127	1043281	20.867	ng/u1	99
33) Hexachlorobutadiene	11.081	225	483934	20.105	ng/u1	98
34) Caprolactam	11.699	113	143105	11.972	ng/u1	91
35) 4-Chloro-3-methylphenol	12.034	107	778746	21.767	ng/u1	100
36) 2-Methylnaphthalene	12.404	142	1623170	20.310	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
 Data File : BP013347.D
 Acq On : 28 Dec 2022 11:32
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 29 00:16:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.622	142	1665819	20.268	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.769	216	987826	19.652	ng/ul	98
40) Hexachlorocyclopentadiene	12.746	237	544196	16.637	ng/ul	98
41) 2,4,6-Trichlorophenol	13.016	196	651072	20.154	ng/ul	100
42) 2,4,5-Trichlorophenol	13.087	196	713280	20.556	ng/ul	100
43) 1,1'-Biphenyl	13.410	154	2288047	19.516	ng/ul	99
44) 2-Chloronaphthalene	13.457	162	1799774	19.505	ng/ul	100
45) 2-Nitroaniline	13.663	65	501120	22.399	ng/ul	94
47) Dimethylphthalate	14.034	163	2339627	19.675	ng/ul	100
48) 2,6-Dinitrotoluene	14.157	165	456116	20.640	ng/ul	97
50) Acenaphthylene	14.304	152	2787404	19.667	ng/ul	100
51) 3-Nitroaniline	14.493	138	386603	18.527	ng/ul	98
52) Acenaphthene	14.645	153	1910045	19.447	ng/ul	99
53) 2,4-Dinitrophenol	14.698	184	236008	15.624	ng/ul	97
55) 4-Nitrophenol	14.798	109	311808	21.175	ng/ul	92
56) Dibenzofuran	14.981	168	2740234	19.623	ng/ul	100
57) 2,4-Dinitrotoluene	14.945	165	666353	20.759	ng/ul	90
58) 2,3,4,6-Tetrachlorophenol	15.210	232	643934	20.335	ng/ul	95
59) Diethylphthalate	15.398	149	2267055	19.612	ng/ul	99
61) Fluorene	15.634	166	2285208	20.405	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.622	204	1209410	20.421	ng/ul	99
63) 4-Nitroaniline	15.657	138	348728	18.992	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.710	198	415422	18.364	ng/ul	95
67) N-Nitrosodiphenylamine	15.840	169	1938369	19.437	ng/ul	99
68) 4-Bromophenyl-phenylether	16.522	248	766208	19.614	ng/ul	99
69) Hexachlorobenzene	16.639	284	887364	19.131	ng/ul	99
70) Atrazine	16.792	200	760293	19.564	ng/ul	100
71) Pentachlorophenol	16.987	266	484578	17.251	ng/ul	99
72) Phenanthrene	17.381	178	3679197	19.637	ng/ul	100
74) Anthracene	17.475	178	3710900	19.836	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.381	216	989063	19.272	ng/ul	100
76) Pentachlorobenzene	14.898	250	1017415	19.444	ng/ul	99
77) Carbazole	17.745	167	3235754	20.538	ng/ul	99
78) Di-n-butylphthalate	18.286	149	3804293	19.832	ng/ul	99
80) Fluoranthene	19.345	202	4383951	21.854	ng/ul	99
82) Pyrene	19.698	202	4541864	21.949	ng/ul	100
83) Butylbenzylphthalate	20.563	149	1587864	19.863	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.339	252	1200145	17.253	ng/ul	99
85) Benzo(a)anthracene	21.410	228	4067743	19.900	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.316	149	2192261	19.441	ng/ul	99
87) Chrysene	21.463	228	3793705	19.626	ng/ul	99
89) Di-n-octyl phthalate	22.263	149	3204277	22.748	ng/ul	100
90) Benzo(b)fluoranthene	23.139	252	3328678	20.761	ng/ul	99
91) Benzo(k)fluoranthene	23.186	252	3266262	20.544	ng/ul	100
93) Benzo(a)pyrene	23.786	252	2768953	19.834	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.480	276	3307947	19.023	ng/ul	100
95) Dibenzo(a,h)anthracene	26.492	278	2750674	19.105	ng/ul	99
96) Benzo(g,h,i)perylene	27.274	276	2682353	19.214	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013347.D
Acq On : 28 Dec 2022 11:32
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 29 00:16:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 28 00:16:35 2022
Response via : Initial Calibration




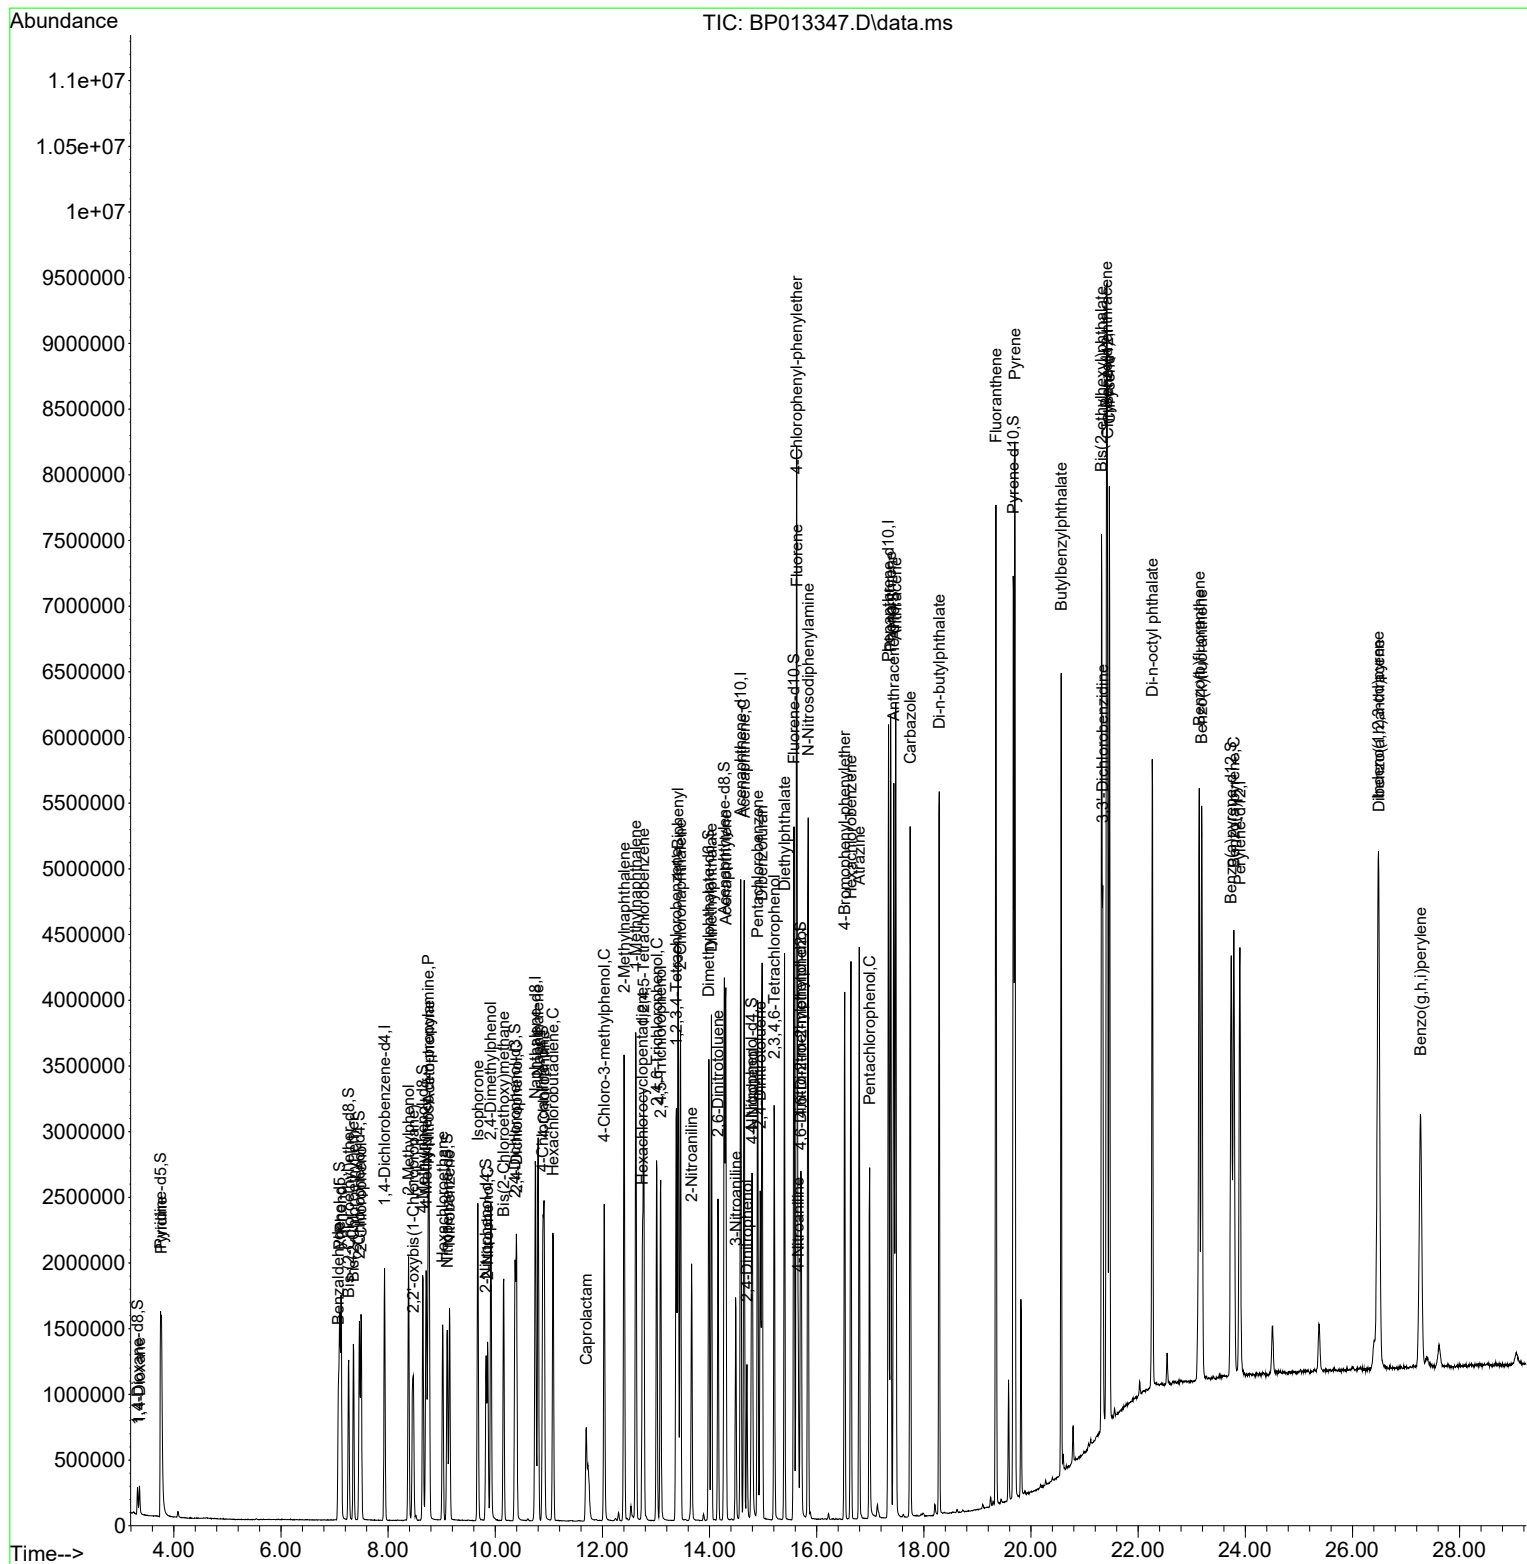


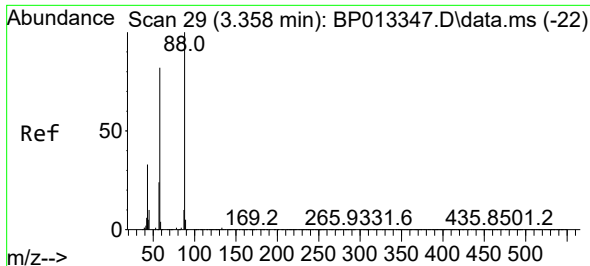

#2
1,4-Dioxane
Concen: 7.997 ng/uL
RT: 3.358 min Scan# 29
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 88 Resp: 97943
Ion Ratio Lower Upper
88 100
43 34.3 22.4 33.6#
58 81.5 58.2 87.4

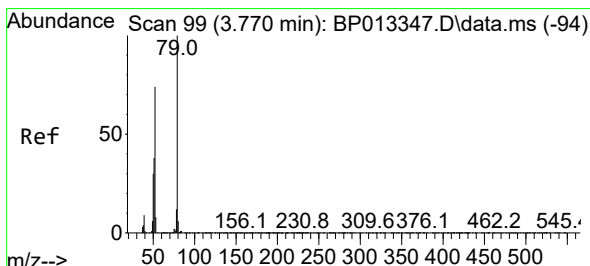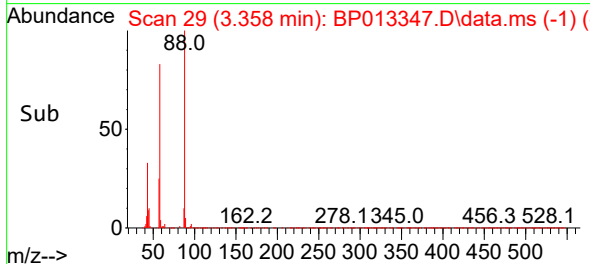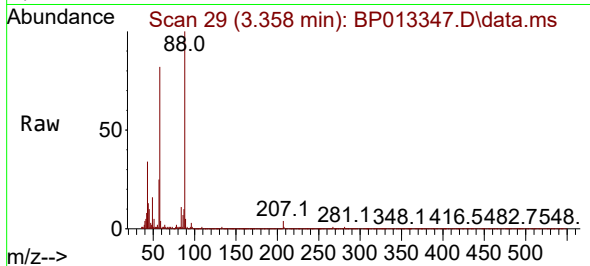

#5
Pyridine
Concen: 20.496 ng/uL
RT: 3.770 min Scan# 99
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion: 79 Resp: 678901
Ion Ratio Lower Upper
79 100
52 82.6 60.7 91.1
51 38.7 28.9 43.3


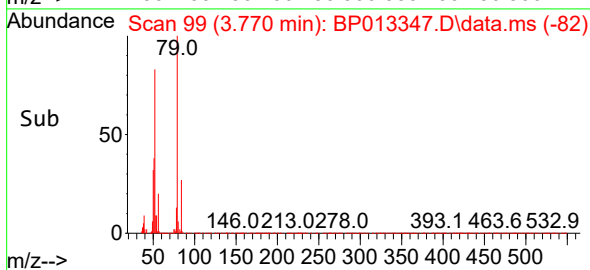

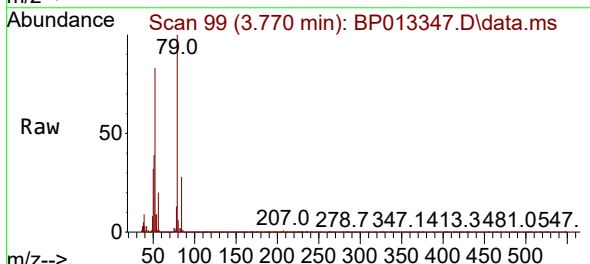


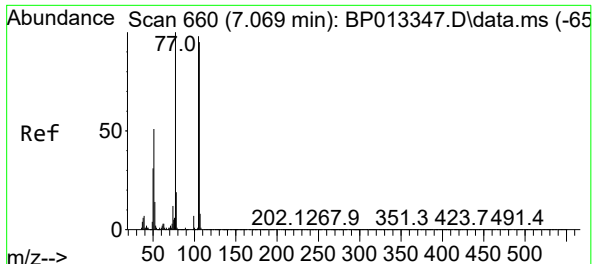

#6
Benzaldehyde
Concen: 20.428 ng/ul
RT: 7.069 min Scan# 660
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 326838
Ion Ratio Lower Upper
77 100
105 97.6 81.5 122.3
106 95.2 76.9 115.3

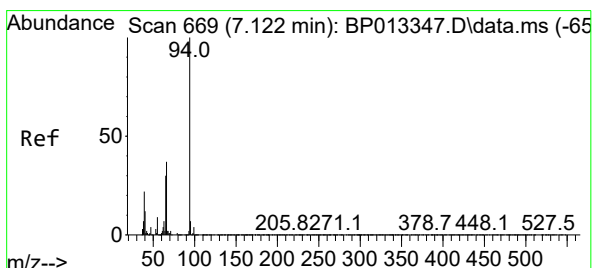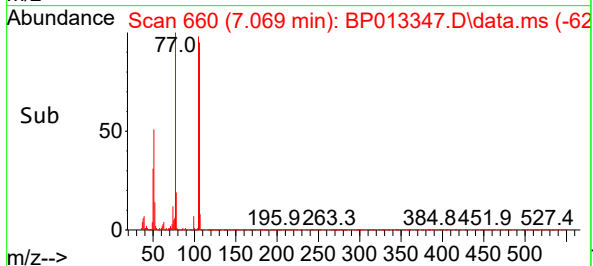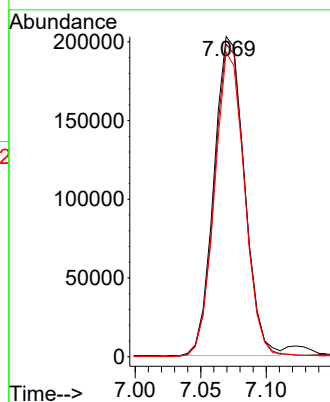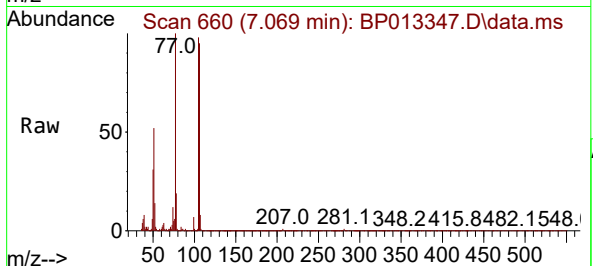

#8
Phenol
Concen: 20.417 ng/ul
RT: 7.122 min Scan# 669
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion: 94 Resp: 843481
Ion Ratio Lower Upper
94 100
65 30.0 21.1 31.7
66 36.6 27.0 40.6


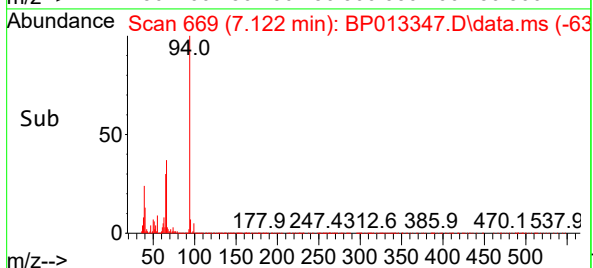

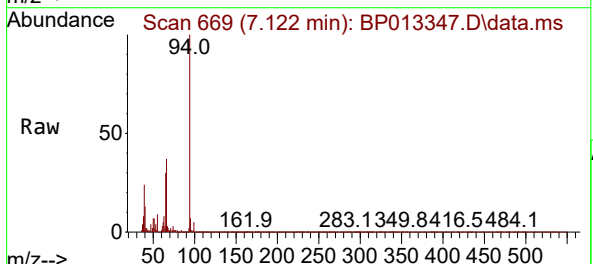




#10
 Bis(2-Chloroethyl)ether
 Concen: 20.527 ng/ul
 RT: 7.352 min Scan# 708
 Delta R.T. 0.000 min
 Lab File: BP013347.D
 Acq: 28 Dec 2022 11:32




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 93 Resp: 696031
 Ion Ratio Lower Upper
 93 100
 63 79.8 59.8 89.8
 95 31.8 26.4 39.6



#12
 2-Chlorophenol
 Concen: 20.177 ng/ul
 RT: 7.493 min Scan# 732
 Delta R.T. 0.000 min
 Lab File: BP013347.D
 Acq: 28 Dec 2022 11:32

Tgt Ion:128 Resp: 665549
 Ion Ratio Lower Upper
 128 100
 64 48.4 34.9 52.3
 130 32.0 25.8 38.6





#13

2-Methylphenol

Concen: 19.965 ng/ul

RT: 8.381 min Scan# 883

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P





ClientSampleId :

Tgt Ion:108 Resp: 643039

Ion Ratio Lower Upper

108 100

107 90.3 69.1 103.7



#14

2,2'-oxybis(1-Chloropropane)

Concen: 23.144 ng/ul

RT: 8.469 min Scan# 898

Delta R.T. 0.012 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion: 45 Resp: 1076888


Ion Ratio Lower Upper

45 100

77 13.9 11.0 16.6


79 10.4 9.3 13.9

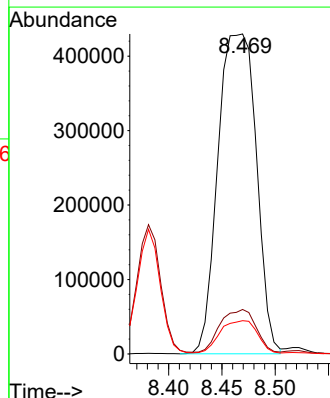






#16
Acetophenone
Concen: 21.743 ng/ul
RT: 8.763 min Scan# 948
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:105 Resp: 1116178
Ion Ratio Lower Upper
105 100
77 77.8 59.3 88.9
51 29.7 19.6 29.4#



#17
N-Nitroso-di-n-propylamine
Concen: 22.665 ng/ul
RT: 8.746 min Scan# 945
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion: 70 Resp: 585091
Ion Ratio Lower Upper
70 100
42 64.6 45.5 68.3
101 9.5 7.9 11.9
130 20.1 17.4 26.2


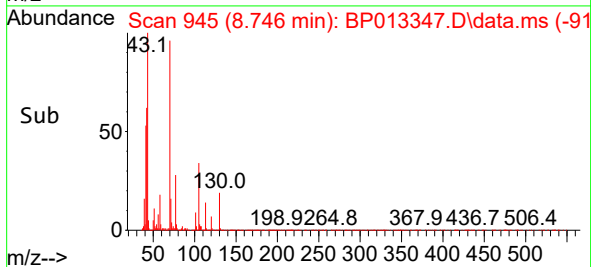

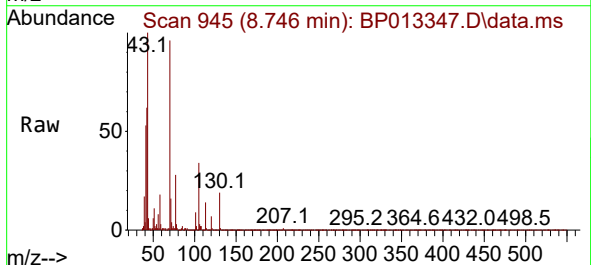




#18
4-Methylphenol
Concen: 20.641 ng/ul
RT: 8.710 min Scan# 911
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:108 Resp: 736386
Ion Ratio Lower Upper
108 100
107 111.0 87.4 131.2



#19
Hexachloroethane
Concen: 19.732 ng/ul
RT: 9.016 min Scan# 991
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:117 Resp: 260093
Ion Ratio Lower Upper
117 100
201 113.7 93.7 140.5
199 70.1 58.6 88.0



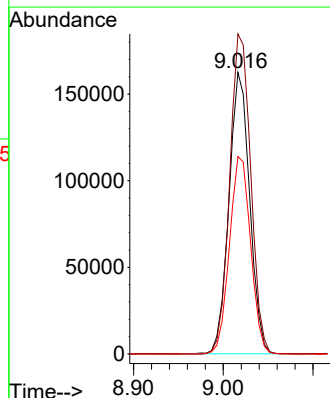





#22
Nitrobenzene
Concen: 21.637 ng/ul
RT: 9.146 min Scan# 1013
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion: 77 Resp: 830958
Ion Ratio Lower Upper
77 100
123 44.5 38.3 57.5
65 13.9 10.3 15.5



#23
Isophorone
Concen: 21.022 ng/ul
RT: 9.675 min Scan# 1103
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion: 82 Resp: 1632490
Ion Ratio Lower Upper
82 100
95 6.6 5.4 8.2
138 18.0 15.3 22.9









#25
2-Nitrophenol
Concen: 20.432 ng/ul
RT: 9.857 min Scan# 1134
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:139 Resp: 407909
Ion Ratio Lower Upper
139 100
65 53.3 36.6 54.8
109 29.2 21.6 32.4



#26
2,4-Dimethylphenol
Concen: 20.905 ng/ul
RT: 9.916 min Scan# 1144
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:107 Resp: 814302
Ion Ratio Lower Upper
107 100
121 50.1 41.8 62.6
122 85.2 72.6 108.8




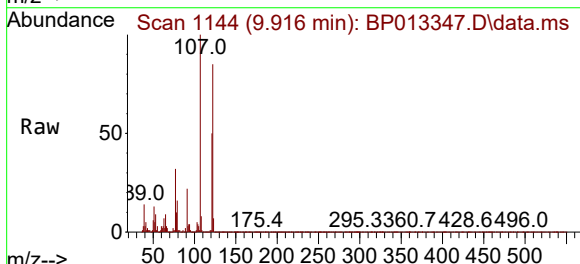




#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.530 ng/ul
 RT: 10.157 min Scan# 1185
 Delta R.T. 0.006 min
 Lab File: BP013347.D
 Acq: 28 Dec 2022 11:32




Instrument :
 BNA_P
 ClientSampleId :


Tgt Ion: 93 Resp: 1019409
 Ion Ratio Lower Upper
 93 100
 95 32.5 26.0 39.0
 123 11.4 9.2 13.8



#29
 2,4-Dichlorophenol
 Concen: 20.756 ng/ul
 RT: 10.399 min Scan# 1226
 Delta R.T. 0.006 min
 Lab File: BP013347.D
 Acq: 28 Dec 2022 11:32

Tgt Ion:162 Resp: 727646
 Ion Ratio Lower Upper
 162 100
 164 64.5 52.5 78.7
 98 33.1 26.6 39.8


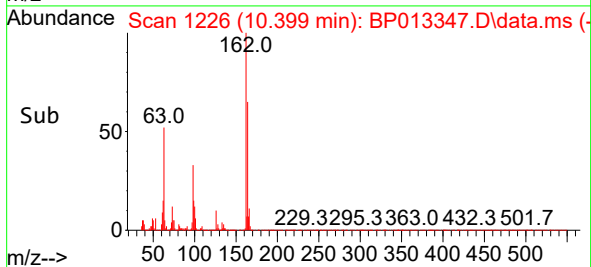

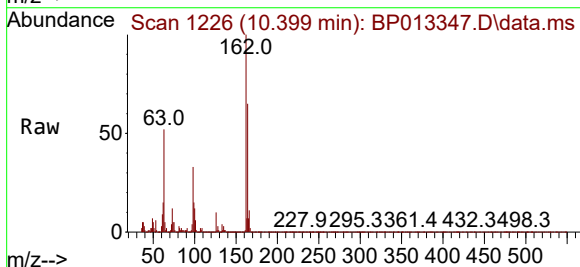




#30
Naphthalene
Concen: 19.767 ng/ul
RT: 10.799 min Scan# 1294
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:128 Resp: 2302776
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 13.0 10.4 15.6



#32
4-Chloroaniline
Concen: 20.867 ng/ul
RT: 10.910 min Scan# 1313
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:127 Resp: 1043281
Ion Ratio Lower Upper
127 100
129 32.6 25.6 38.4

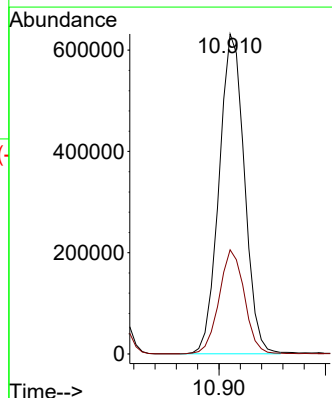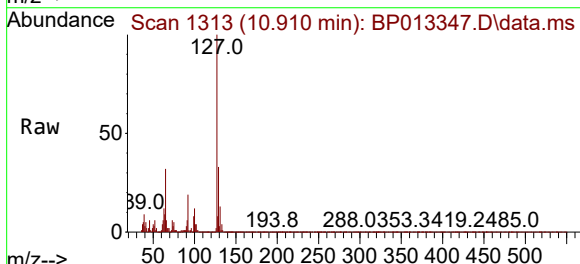



#33

Hexachlorobutadiene

Concen: 20.105 ng/ul

RT: 11.081 min Scan# 11

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:225 Resp: 483934

Ion Ratio Lower Upper

225 100

223 63.5 49.2 73.8

227 64.2 50.2 75.2

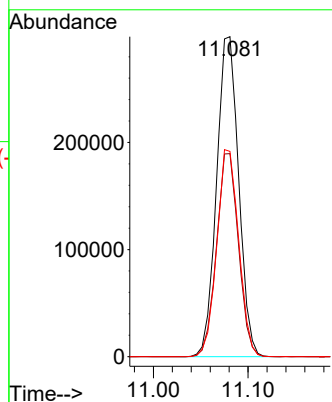

#34

Caprolactam

Concen: 11.972 ng/ul

RT: 11.699 min Scan# 1447

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:113 Resp: 143105


Ion Ratio Lower Upper

113 100

55 186.2 141.9 212.9

56 138.3 99.6 149.4









#35
4-Chloro-3-methylphenol
Concen: 21.767 ng/ul
RT: 12.034 min Scan# 1504
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:107 Resp: 778746
Ion Ratio Lower Upper
107 100
144 26.5 21.4 32.2
142 82.0 65.8 98.6



#36
2-Methylnaphthalene
Concen: 20.310 ng/ul
RT: 12.404 min Scan# 1567
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:142 Resp: 1623170
Ion Ratio Lower Upper
142 100
141 88.0 70.8 106.2





#37

1-Methylnaphthalene

Concen: 20.268 ng/ul

RT: 12.622 min Scan# 1604

Delta R.T. 0.000 min


Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :






Tgt Ion:142 Resp: 1665819

Ion Ratio Lower Upper

142 100

141 91.6 72.7 109.1

116 3.8 2.7 4.1

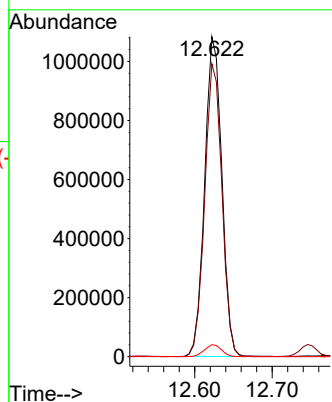

#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.652 ng/ul

RT: 12.769 min Scan# 1629

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Tgt Ion:216 Resp: 987826




Ion Ratio Lower Upper


216 100

214 79.3 61.9 92.9

179 19.8 15.0 22.6

108 15.4 11.0 16.4



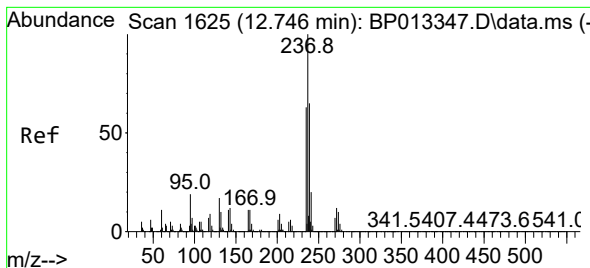

#40

Hexachlorocyclopentadiene

Concen: 16.637 ng/ul

RT: 12.746 min Scan# 1625

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:237 Resp: 544196

Ion Ratio Lower Upper

237 100

235 63.3 49.7 74.5

272 12.4 10.8 16.2

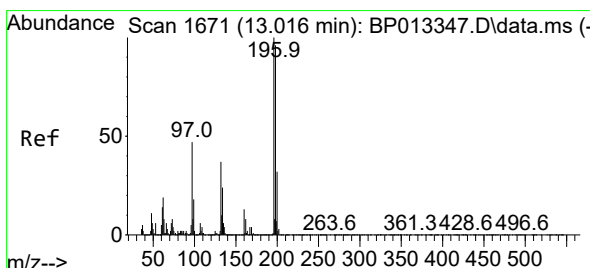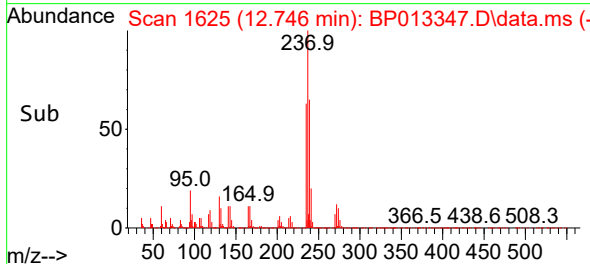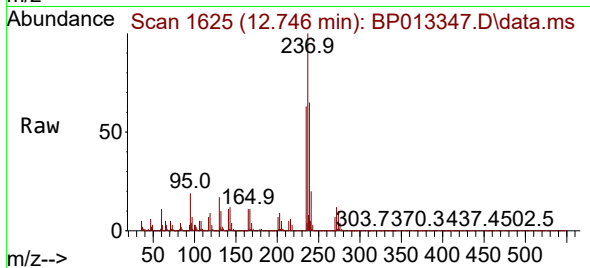

#41

2,4,6-Trichlorophenol

Concen: 20.154 ng/ul

RT: 13.016 min Scan# 1671

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:196 Resp: 651072


Ion Ratio Lower Upper

196 100

198 96.4 77.0 115.6

200 31.9 25.3 37.9

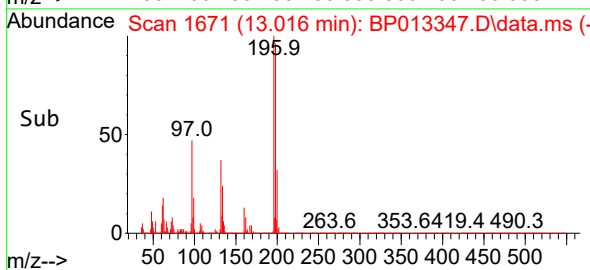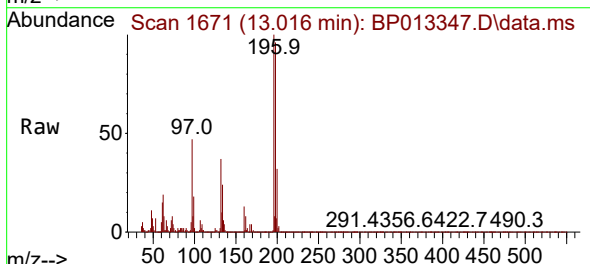



#42

2,4,5-Trichlorophenol

Concen: 20.556 ng/ul

RT: 13.087 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:196 Resp: 713280

Ion Ratio Lower Upper

196 100

198 96.3 77.1 115.7

200 32.0 25.4 38.2



#43

1,1'-Biphenyl

Concen: 19.516 ng/ul

RT: 13.410 min Scan# 1738

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:154 Resp: 2288047


Ion Ratio Lower Upper

154 100

153 39.7 31.5 47.3

76 12.8 9.6 14.4

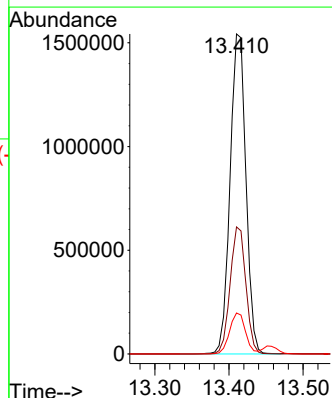



#44

2-Chloronaphthalene

Concen: 19.505 ng/ul

RT: 13.457 min Scan# 1746

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:162 Resp: 1799774

Ion Ratio Lower Upper

162 100

164 33.2 26.3 39.5

127 36.4 29.3 43.9

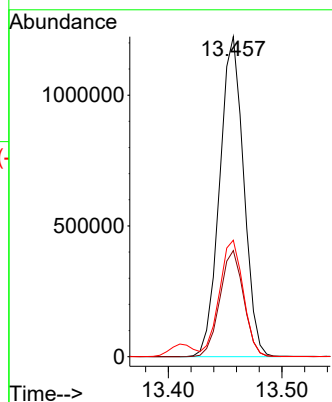

#45

2-Nitroaniline

Concen: 22.399 ng/ul

RT: 13.663 min Scan# 1781

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion: 65 Resp: 501120


Ion Ratio Lower Upper

65 100

92 67.8 56.4 84.6

138 104.0 90.3 135.5









#47
Dimethylphthalate
Concen: 19.675 ng/ul
RT: 14.034 min Scan# 1844
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:163 Resp: 2339627
Ion Ratio Lower Upper
163 100
194 4.3 3.4 5.0
164 10.2 8.3 12.5



#48
2,6-Dinitrotoluene
Concen: 20.640 ng/ul
RT: 14.157 min Scan# 1865
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32


Tgt Ion:165 Resp: 456116
Ion Ratio Lower Upper
165 100
89 56.4 43.0 64.4
121 20.2 16.1 24.1

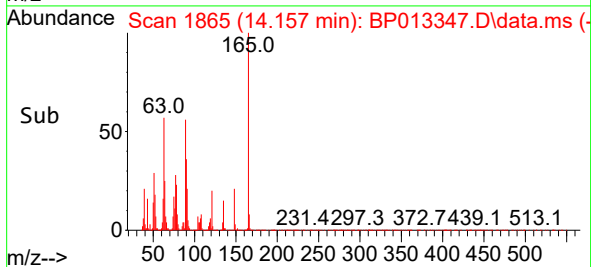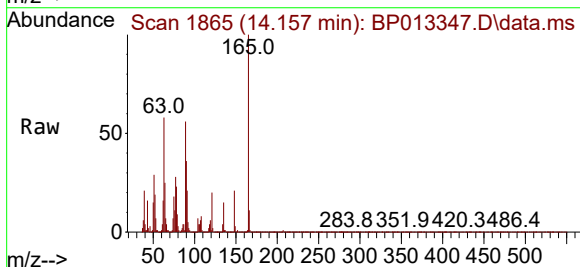






#50
Acenaphthylene
Concen: 19.667 ng/ul
RT: 14.304 min Scan# 1890
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:152 Resp: 2787404
Ion Ratio Lower Upper
152 100
151 20.0 15.8 23.6
153 13.3 10.6 16.0



#51
3-Nitroaniline
Concen: 18.527 ng/ul
RT: 14.493 min Scan# 1922
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:138 Resp: 386603
Ion Ratio Lower Upper
138 100
108 10.3 8.6 13.0
92 112.1 88.4 132.6


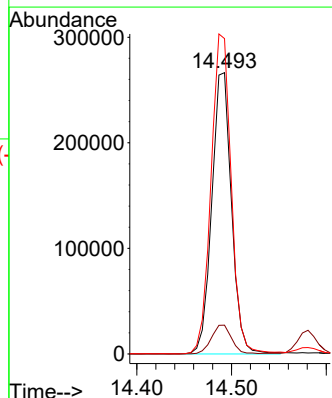






#52
Acenaphthene
Concen: 19.447 ng/ul
RT: 14.645 min Scan# 1948
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:153 Resp: 1910045
Ion Ratio Lower Upper
153 100
152 47.2 38.2 57.4
154 87.9 70.8 106.2



#53
2,4-Dinitrophenol
Concen: 15.624 ng/ul
RT: 14.698 min Scan# 1957
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:184 Resp: 236008
Ion Ratio Lower Upper
184 100
63 64.3 48.4 72.6
154 57.6 45.5 68.3



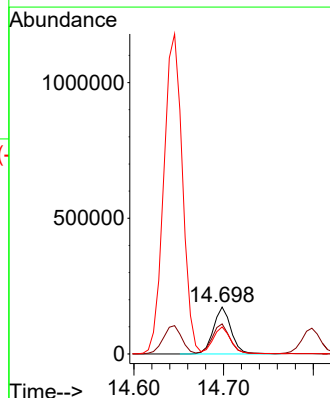





#55
4-Nitrophenol
Concen: 21.175 ng/ul
RT: 14.798 min Scan# 1974
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:109 Resp: 311808
Ion Ratio Lower Upper
109 100
139 137.5 120.8 181.2
65 140.0 107.9 161.9



#56
Dibenzofuran
Concen: 19.623 ng/ul
RT: 14.981 min Scan# 2005
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:168 Resp: 2740234
Ion Ratio Lower Upper
168 100
139 34.9 27.9 41.9


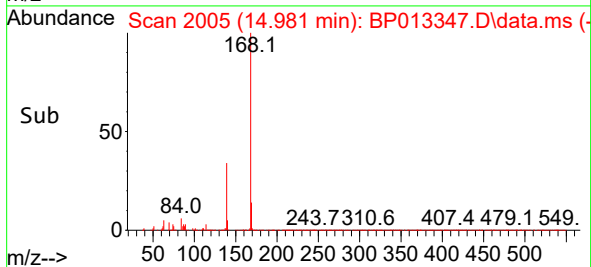

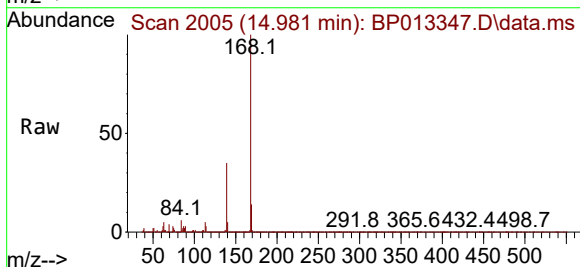




#57
2,4-Dinitrotoluene
Concen: 20.759 ng/ul
RT: 14.945 min Scan# 1999
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:165 Resp: 666353
Ion Ratio Lower Upper
165 100
63 46.0 31.8 47.6
182 2.7 2.1 3.1

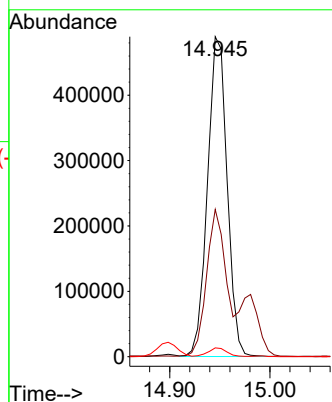

#58
2,3,4,6-Tetrachlorophenol
Concen: 20.335 ng/ul
RT: 15.210 min Scan# 2044
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:232 Resp: 643934
Ion Ratio Lower Upper
232 100
131 36.4 31.8 47.6
130 2.0 1.8 2.6
166 26.1 22.9 34.3

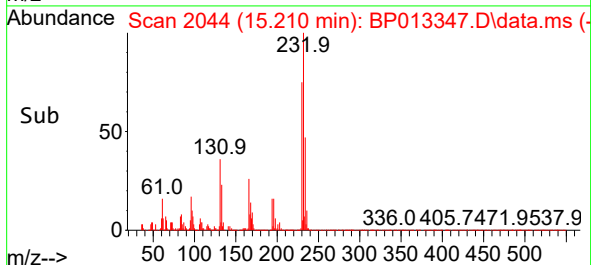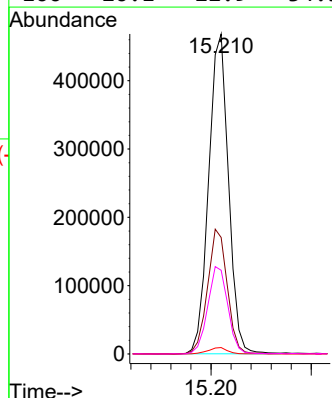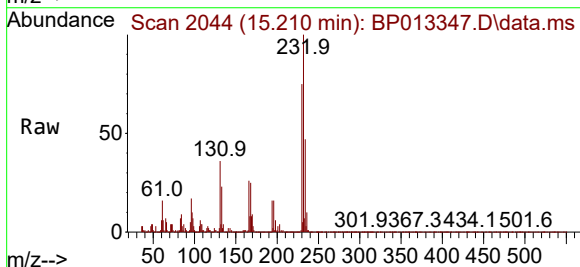



#59

Diethylphthalate

Concen: 19.612 ng/ul

RT: 15.398 min Scan# 2076

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 2267055

Ion Ratio Lower Upper

149 100

177 23.7 18.4 27.6

150 12.6 9.9 14.9



#61

Fluorene

Concen: 20.405 ng/ul

RT: 15.634 min Scan# 2116

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:166 Resp: 2285208


Ion Ratio Lower Upper

166 100

165 99.0 77.4 116.2

167 13.4 10.6 16.0



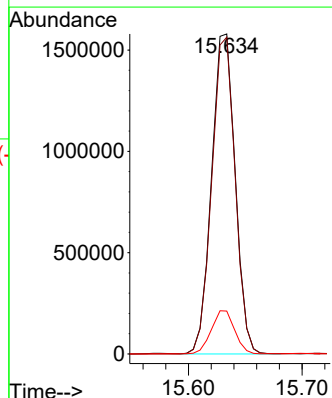





#62
4-Chlorophenyl-phenylether
Concen: 20.421 ng/ul
RT: 15.622 min Scan# 2114
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:204 Resp: 1209410
Ion Ratio Lower Upper
204 100
206 32.9 26.3 39.5
141 51.2 40.4 60.6

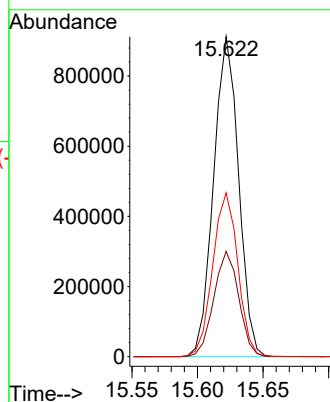

#63
4-Nitroaniline
Concen: 18.992 ng/ul
RT: 15.657 min Scan# 2120
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:138 Resp: 348728
Ion Ratio Lower Upper
138 100
92 51.1 39.0 58.4
108 78.1 55.1 82.7









#66
4,6-Dinitro-2-methylphenol
Concen: 18.364 ng/ul
RT: 15.710 min Scan# 2129
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:198 Resp: 415422
Ion Ratio Lower Upper
198 100
182 4.6 3.3 4.9
77 23.2 16.6 25.0

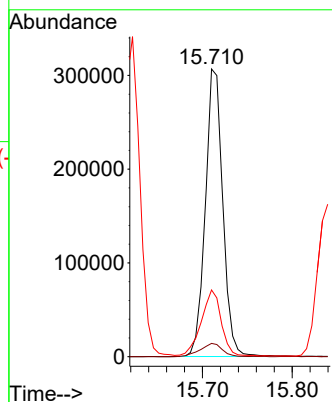

#67
N-Nitrosodiphenylamine
Concen: 19.437 ng/ul
RT: 15.840 min Scan# 2151
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:169 Resp: 1938369
Ion Ratio Lower Upper
169 100
168 65.5 53.0 79.6
167 35.9 29.1 43.7









#68
4-Bromophenyl-phenylether
Concen: 19.614 ng/ul
RT: 16.522 min Scan# 2267
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:248 Resp: 766208
Ion Ratio Lower Upper
248 100
250 96.3 77.4 116.0
141 61.8 48.3 72.5

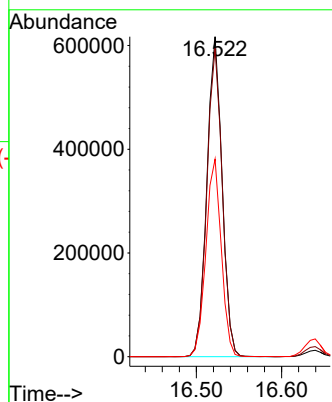

#69
Hexachlorobenzene
Concen: 19.131 ng/ul
RT: 16.639 min Scan# 2287
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:284 Resp: 887364
Ion Ratio Lower Upper
284 100
142 29.5 22.6 34.0
249 30.5 24.6 37.0





#70

Atrazine

Concen: 19.564 ng/ul

RT: 16.792 min Scan# 2313

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:200 Resp: 760293

Ion Ratio Lower Upper

200 100

173 25.4 20.5 30.7

215 49.9 39.9 59.9

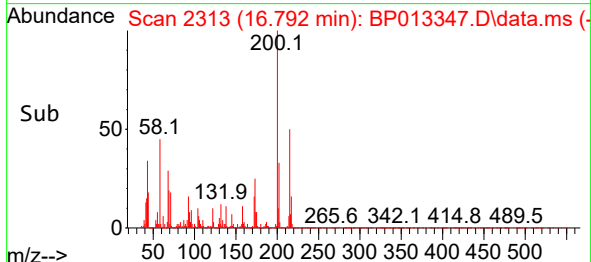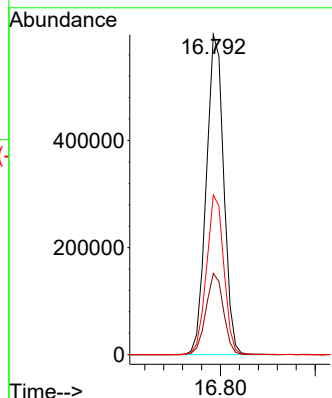

#71

Pentachlorophenol

Concen: 17.251 ng/ul

RT: 16.987 min Scan# 2346

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:266 Resp: 484578


Ion Ratio Lower Upper

266 100

264 64.8 50.9 76.3

268 64.7 51.4 77.2

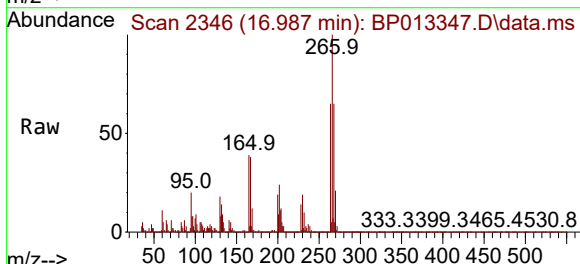



#72

Phenanthrene

Concen: 19.637 ng/ul

RT: 17.381 min Scan# 2413

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:178 Resp: 3679197

Ion Ratio Lower Upper

178 100

179 15.4 12.5 18.7

176 19.2 15.4 23.0



#74

Anthracene

Concen: 19.836 ng/ul

RT: 17.475 min Scan# 2429

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:178 Resp: 3710900


Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7

176 18.4 14.8 22.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.272 ng/uL
RT: 13.381 min Scan# 1733
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:216 Resp: 989063
Ion Ratio Lower Upper
216 100
214 78.3 62.2 93.2
218 48.6 38.9 58.3

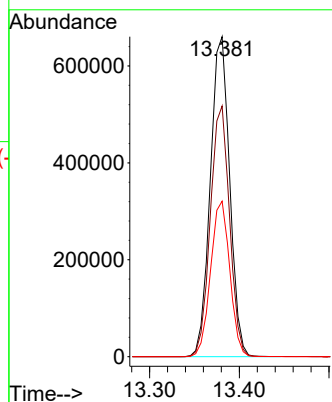

#76
Pentachlorobenzene
Concen: 19.444 ng/uL
RT: 14.898 min Scan# 1991
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32


Tgt Ion:250 Resp: 1017415
Ion Ratio Lower Upper
250 100
248 64.2 50.6 76.0
252 65.2 51.1 76.7








#77
 Carbazole
 Concen: 20.538 ng/ul
 RT: 17.745 min Scan# 2475
 Delta R.T. 0.006 min
 Lab File: BP013347.D
 Acq: 28 Dec 2022 11:32

Instrument :
 BNA_P
 ClientSampleId :







Tgt Ion:167 Resp: 3235754
 Ion Ratio Lower Upper
 167 100
 166 21.2 17.2 25.8
 139 12.1 9.4 14.2



#78
 Di-n-butylphthalate
 Concen: 19.832 ng/ul
 RT: 18.286 min Scan# 2567
 Delta R.T. 0.006 min
 Lab File: BP013347.D
 Acq: 28 Dec 2022 11:32

Tgt Ion:149 Resp: 3804293
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.5 11.3
 104 4.8 3.8 5.6

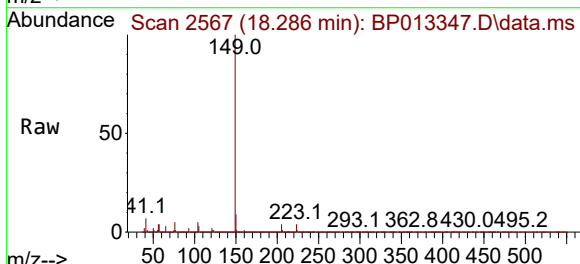



#80

Fluoranthene

Concen: 21.854 ng/ul

RT: 19.345 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:202 Resp: 4383951

Ion Ratio Lower Upper

202 100

101 9.8 8.2 12.2

100 7.7 6.1 9.1



#82

Pyrene

Concen: 21.949 ng/ul

RT: 19.698 min Scan# 2807

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:202 Resp: 4541864


Ion Ratio Lower Upper

202 100

101 12.0 9.4 14.2

100 9.9 7.8 11.8

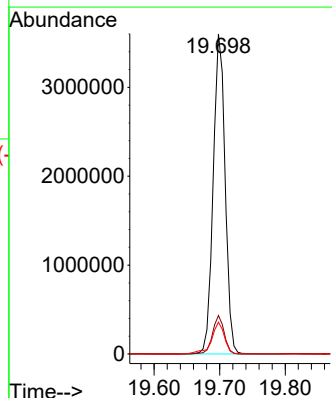



#83

Butylbenzylphthalate

Concen: 19.863 ng/ul

RT: 20.563 min Scan# 2954

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 1587864

Ion Ratio Lower Upper

149 100

91 68.9 53.4 80.0

206 23.4 17.9 26.9

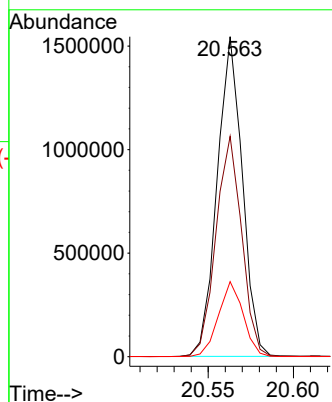

#84

3,3'-Dichlorobenzidine

Concen: 17.253 ng/ul

RT: 21.339 min Scan# 3086

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:252 Resp: 1200145


Ion Ratio Lower Upper

252 100

254 64.1 51.8 77.8

126 9.0 7.4 11.2









#85
Benzo(a)anthracene
Concen: 19.900 ng/ul
RT: 21.410 min Scan# 3098
Delta R.T. 0.006 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:228 Resp: 4067743
Ion Ratio Lower Upper
228 100
229 19.9 16.1 24.1
226 27.2 22.0 33.0

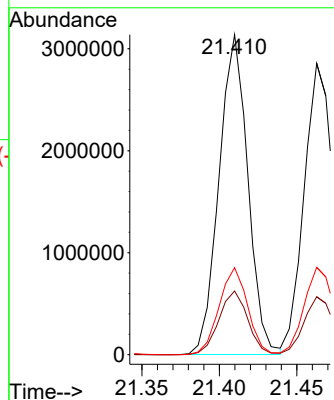

#86
Bis(2-ethylhexyl)phthalate
Concen: 19.441 ng/ul
RT: 21.316 min Scan# 3082
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:149 Resp: 2192261
Ion Ratio Lower Upper
149 100
167 27.8 22.5 33.7
279 4.3 3.8 5.8



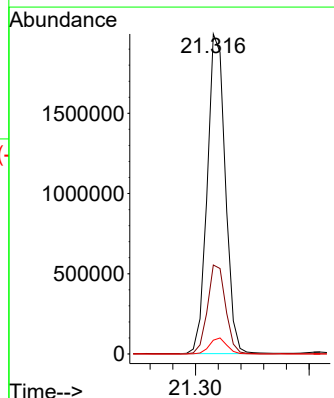





#87
Chrysene
Concen: 19.626 ng/ul
RT: 21.463 min Scan# 3107
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:228 Resp: 3793705
Ion Ratio Lower Upper
228 100
226 30.0 24.5 36.7
229 19.9 16.0 24.0



#89
Di-n-octyl phthalate
Concen: 22.748 ng/ul
RT: 22.263 min Scan# 3243
Delta R.T. 0.000 min
Lab File: BP013347.D
Acq: 28 Dec 2022 11:32

Tgt Ion:149 Resp: 3204277





#90

Benzo(b)fluoranthene

Concen: 20.761 ng/ul

RT: 23.139 min Scan# 31

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 3328678

Ion Ratio Lower Upper

252 100

253 22.5 17.7 26.5

125 8.4 6.8 10.2

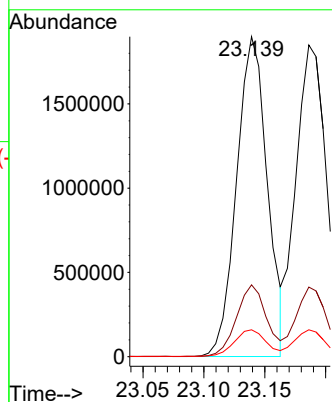

#91

Benzo(k)fluoranthene

Concen: 20.544 ng/ul

RT: 23.186 min Scan# 3400

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:252 Resp: 3266262


Ion Ratio Lower Upper

252 100

253 22.3 17.7 26.5

125 8.6 6.8 10.2





#93

Benzo(a)pyrene

Concen: 19.834 ng/ul

RT: 23.786 min Scan# 3502

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:252 Resp: 2768953

Ion Ratio Lower Upper

252 100

253 21.5 17.5 26.3

125 9.1 7.5 11.3



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.023 ng/ul

RT: 26.480 min Scan# 3960

Delta R.T. 0.006 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32




Tgt Ion:276 Resp: 3307947


Ion Ratio Lower Upper

276 100

138 21.1 17.1 25.7

277 25.1 20.0 30.0





#95

Dibenzo(a,h)anthracene

Concen: 19.105 ng/ul

RT: 26.492 min Scan# 3962

Delta R.T. 0.000 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:278 Resp: 2750674

Ion Ratio Lower Upper

278 100

139 13.0 11.1 16.7

279 24.0 19.0 28.6



#96

Benzo(g,h,i)perylene

Concen: 19.214 ng/ul

RT: 27.274 min Scan# 4095

Delta R.T. 0.012 min

Lab File: BP013347.D

Acq: 28 Dec 2022 11:32

Tgt Ion:276 Resp: 2682353

Ion Ratio Lower Upper

276 100

138 18.2 15.4 23.2

277 24.2 19.1 28.7

