

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
 Data File : BP013355.D
 Acq On : 28 Dec 2022 16:54
 Operator : CG/JU
 Sample : N6187-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 29 14:31:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	473960	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	2125850	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	1470204	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	3888149	20.000	ng/ul	0.01
79) Chrysene-d12	21.421	240	2862638	20.000	ng/ul	0.00
88) Perylene-d12	23.886	264	2605205	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	47648	4.298	ng/uL	0.00
4) Pyridine-d5	3.746	84	716521	22.755	ng/ul	0.00
7) Phenol-d5	7.093	99	1043129	27.020	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	722985	31.045	ng/ul	0.00
11) 2-Chlorophenol-d4	7.458	132	860712	28.322	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	927859	29.333	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	482850	30.914	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	559779	31.834	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	1002306	29.346	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	1392732	28.884	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	3551387	31.430	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	3970409	31.978	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	489268	24.072	ng/ul	0.00
60) Fluorene-d10	15.569	176	3142167	32.871	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	490949	19.621	ng/ul	0.00
73) Anthracene-d10	17.445	188	4775643	27.225	ng/ul	0.01
81) Pyrene-d10	19.669	212	5732968	34.890	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	4281047	32.968	ng/ul	0.00
Target Compounds						
52) Acenaphthene	14.692	153	459601	4.969	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013355.D
Acq On : 28 Dec 2022 16:54
Operator : CG/JU
Sample : N6187-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Dec 29 14:31:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 28 00:16:35 2022
Response via : Initial Calibration

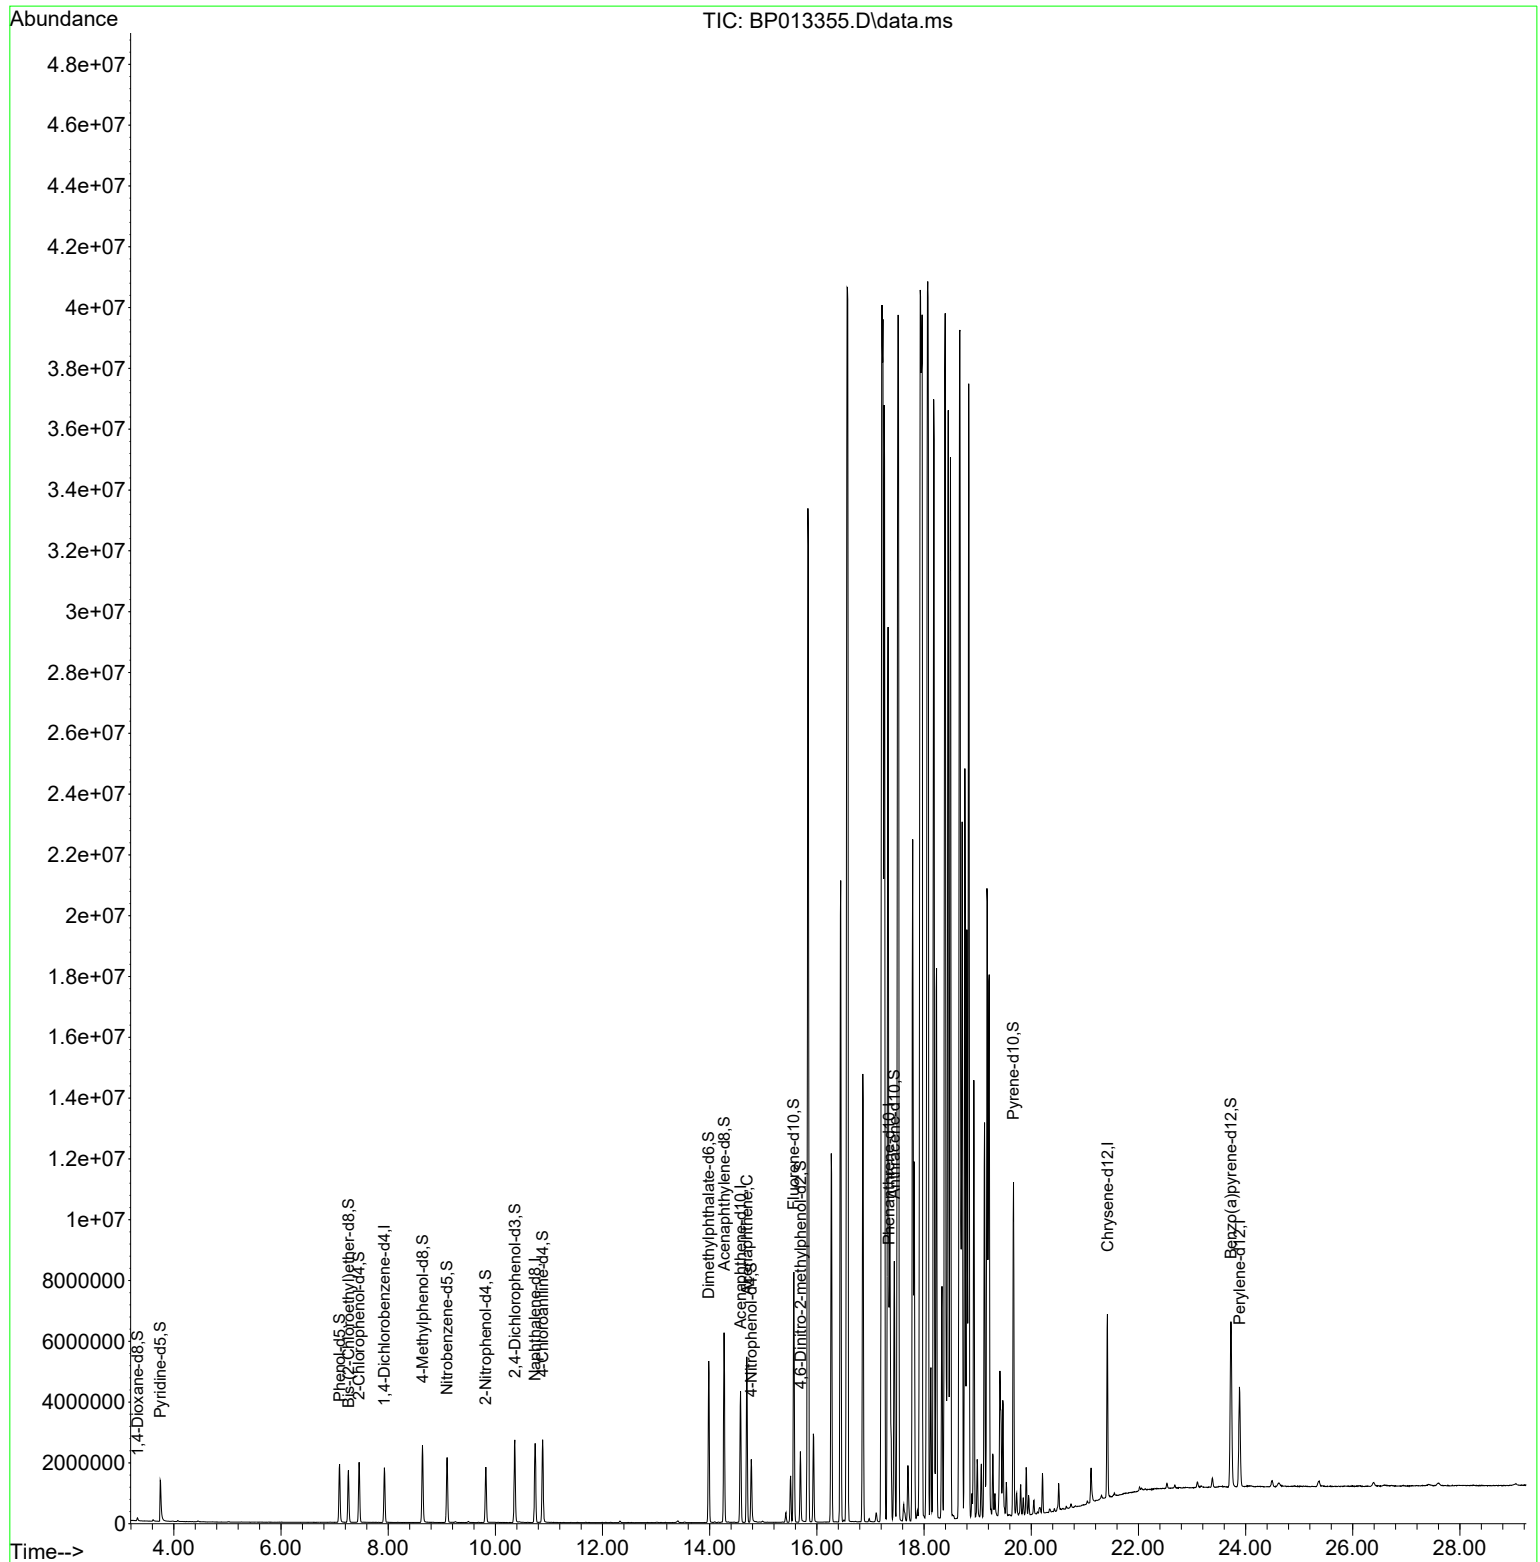

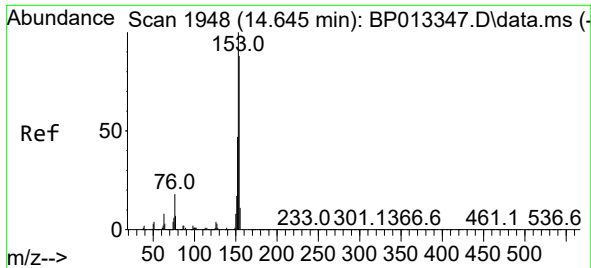

#52
 Acenaphthene
 Concen: 4.969 ng/ul
 RT: 14.692 min Scan# 1956
 Delta R.T. 0.053 min
 Lab File: BP013355.D
 Acq: 28 Dec 2022 16:54

Instrument :
 BNA_P
 ClientSampleId :

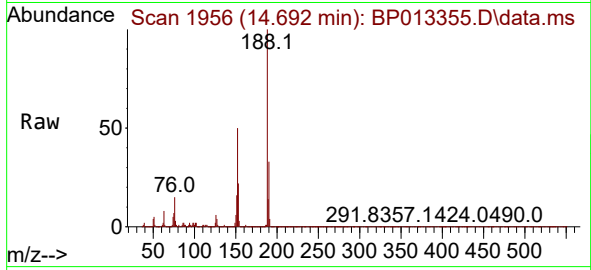

Tgt Ion:153 Resp: 459601
 Ion Ratio Lower Upper
 153 100
 152 228.7 38.2 57.4#
 154 11.8 70.8 106.2#

