

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP122822\  
 Data File : BP013349.D  
 Acq On : 28 Dec 2022 12:44  
 Operator : CG/JU  
 Sample : N6128-06  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A4492

Quant Time: Dec 28 13:09:00 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP120722.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Dec 28 00:16:35 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc Units   | Dev(Min)  |
|-------------------------------|--------|------|----------|--------------|-----------|
| Internal Standards            |        |      |          |              |           |
| 1) 1,4-Dichlorobenzene-d4     | 7.934  | 152  | 397705   | 20.000 ng/u1 | 0.00      |
| 20) Naphthalene-d8            | 10.746 | 136  | 1771747  | 20.000 ng/u1 | 0.00      |
| 38) Acenaphthene-d10          | 14.575 | 164  | 1237686  | 20.000 ng/u1 | 0.00      |
| 64) Phenanthrene-d10          | 17.333 | 188  | 2887125  | 20.000 ng/u1 | 0.00      |
| 79) Chrysene-d12              | 21.421 | 240  | 2666575  | 20.000 ng/u1 | 0.00      |
| 88) Perylene-d12              | 23.892 | 264  | 2315668  | 20.000 ng/u1 | 0.00      |
| System Monitoring Compounds   |        |      |          |              |           |
| 3) 1,4-Dioxane-d8             | 3.322  | 96   | 42108    | 4.527 ng/uL  | 0.00      |
| 4) Pyridine-d5                | 0.000  | 84   | 0d       | 0.000 ng/u1  |           |
| 7) Phenol-d5                  | 7.093  | 99   | 917217   | 28.314 ng/u1 | 0.00      |
| 9) Bis-(2-Chloroethyl)eth...  | 7.258  | 67   | 564383   | 28.882 ng/u1 | 0.00      |
| 11) 2-Chlorophenol-d4         | 7.463  | 132  | 708561   | 27.786 ng/u1 | 0.00      |
| 15) 4-Methylphenol-d8         | 8.646  | 113  | 738972   | 27.841 ng/u1 | 0.00      |
| 21) Nitrobenzene-d5           | 9.104  | 128  | 350489   | 26.924 ng/u1 | 0.00      |
| 24) 2-Nitrophenol-d4          | 9.828  | 143  | 405264   | 27.653 ng/u1 | 0.00      |
| 28) 2,4-Dichlorophenol-d3     | 10.363 | 165  | 778531   | 27.350 ng/u1 | 0.00      |
| 31) 4-Chloroaniline-d4        | 10.887 | 131  | 856501   | 21.313 ng/u1 | 0.00      |
| 46) Dimethylphthalate-d6      | 13.987 | 166  | 2965138  | 31.172 ng/u1 | 0.00      |
| 49) Acenaphthylene-d8         | 14.269 | 160  | 2992022  | 28.626 ng/u1 | 0.00      |
| 54) 4-Nitrophenol-d4          | 14.781 | 143  | 460370   | 26.906 ng/u1 | 0.00      |
| 60) Fluorene-d10              | 15.569 | 176  | 2642118  | 32.832 ng/u1 | 0.00      |
| 65) 4,6-Dinitro-2-methylph... | 15.692 | 200  | 391852   | 21.091 ng/u1 | 0.00      |
| 73) Anthracene-d10            | 17.433 | 188  | 4466923  | 34.295 ng/u1 | 0.00      |
| 81) Pyrene-d10                | 19.669 | 212  | 5420180  | 35.412 ng/u1 | 0.00      |
| 92) Benzo(a)pyrene-d12        | 23.727 | 264  | 4028522  | 34.902 ng/u1 | 0.00      |
| Target Compounds              |        |      |          |              |           |
| 86) Bis(2-ethylhexyl)phtha... | 21.316 | 149  | 5153257  | 52.769 ng/u1 | Qvalue 99 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP122822\  
Data File : BP013349.D  
Acq On : 28 Dec 2022 12:44  
Operator : CG/JU  
Sample : N6128-06  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A4492

Quant Time: Dec 28 13:09:00 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP120722.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Dec 28 00:16:35 2022  
Response via : Initial Calibration

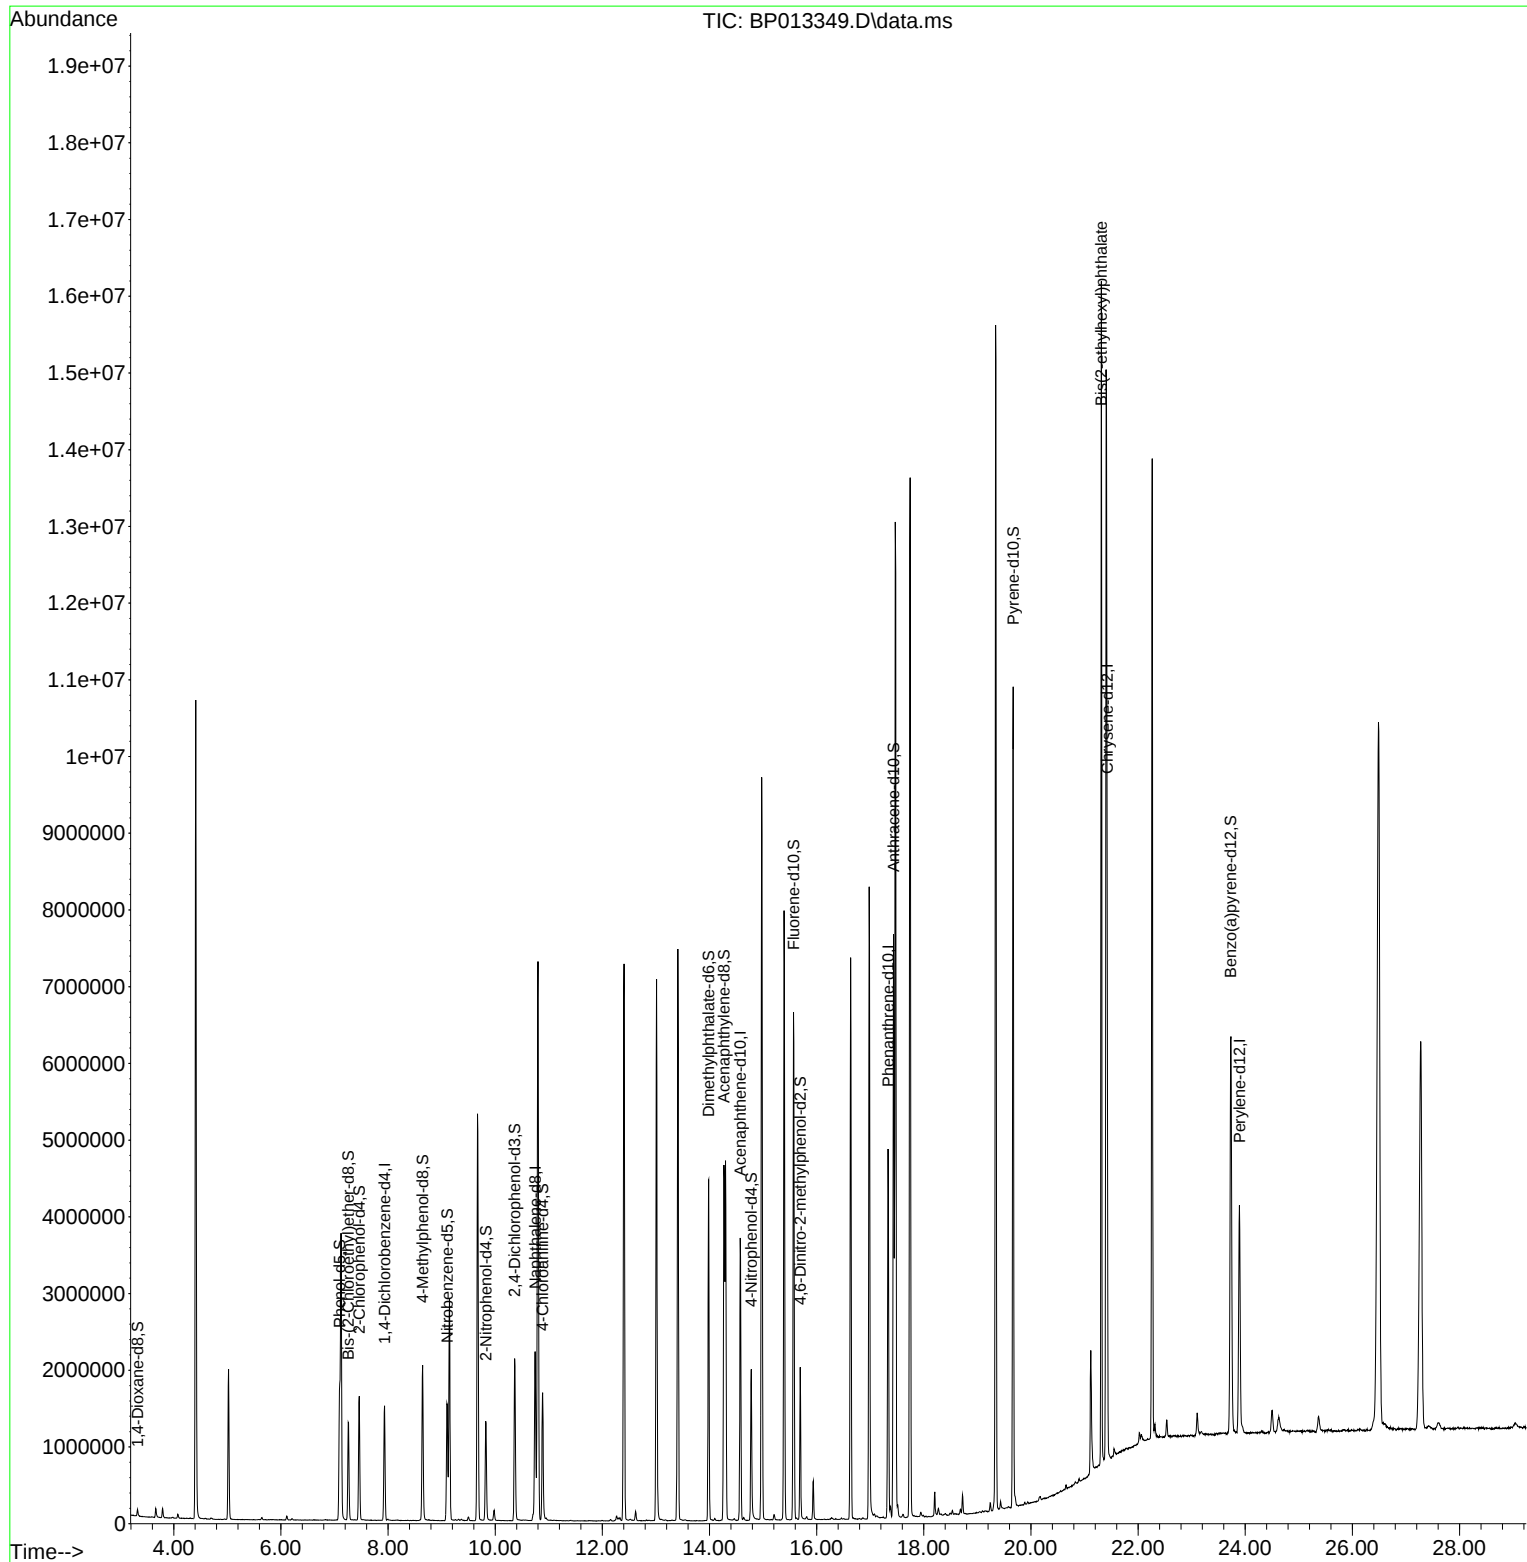

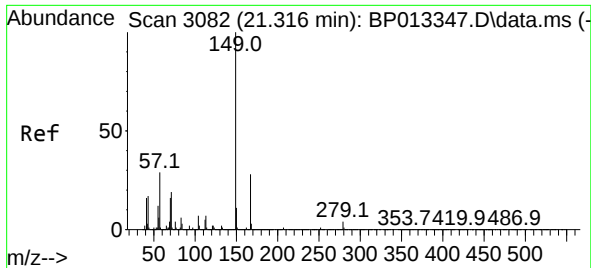

#86

Bis(2-ethylhexyl)phthalate

Concen: 52.769 ng/ul

RT: 21.316 min Scan# 30

Delta R.T. 0.000 min

Lab File: BP013349.D


Acq: 28 Dec 2022 12:44

Instrument :

BNA\_P

ClientSampleId :

A4492

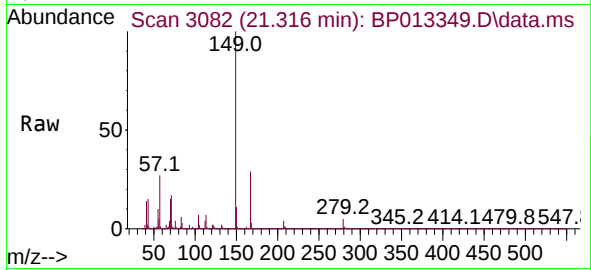

Tgt Ion:149 Resp: 5153257

Ion Ratio Lower Upper

149 100

167 28.8 22.5 33.7

279 5.3 3.8 5.8

