

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
 Data File : BP013351.D
 Acq On : 28 Dec 2022 14:38
 Operator : CG/JU
 Sample : N6187-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T5

Quant Time: Dec 29 00:18:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	581906	20.000	ng/u1	0.00
20) Naphthalene-d8	10.745	136	2597067	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.575	164	1881256	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.333	188	4463728	20.000	ng/u1	0.00
79) Chrysene-d12	21.421	240	4077027	20.000	ng/u1	0.00
88) Perylene-d12	23.886	264	3660457	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	56816	4.175	ng/uL	0.00
4) Pyridine-d5	3.746	84	829918	21.467	ng/u1	0.00
7) Phenol-d5	7.093	99	1120176	23.634	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	718467	25.128	ng/u1	0.00
11) 2-Chlorophenol-d4	7.457	132	890311	23.861	ng/u1	0.00
15) 4-Methylphenol-d8	8.640	113	952931	24.537	ng/u1	0.00
21) Nitrobenzene-d5	9.098	128	465226	24.381	ng/u1	0.00
24) 2-Nitrophenol-d4	9.822	143	542105	25.235	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	993208	23.803	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	1347202	22.871	ng/u1	0.00
46) Dimethylphthalate-d6	13.981	166	3614790	25.001	ng/u1	0.00
49) Acenaphthylene-d8	14.269	160	3851897	24.245	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	522376	20.086	ng/u1	0.00
60) Fluorene-d10	15.569	176	3089870	25.261	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	506683	17.639	ng/u1	0.00
73) Anthracene-d10	17.433	188	5020162	24.929	ng/u1	0.00
81) Pyrene-d10	19.663	212	6103181	26.080	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.727	264	4550684	24.942	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.310	149	197920	1.326	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013351.D
Acq On : 28 Dec 2022 14:38
Operator : CG/JU
Sample : N6187-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43T5

Quant Time: Dec 29 00:18:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 28 00:16:35 2022
Response via : Initial Calibration

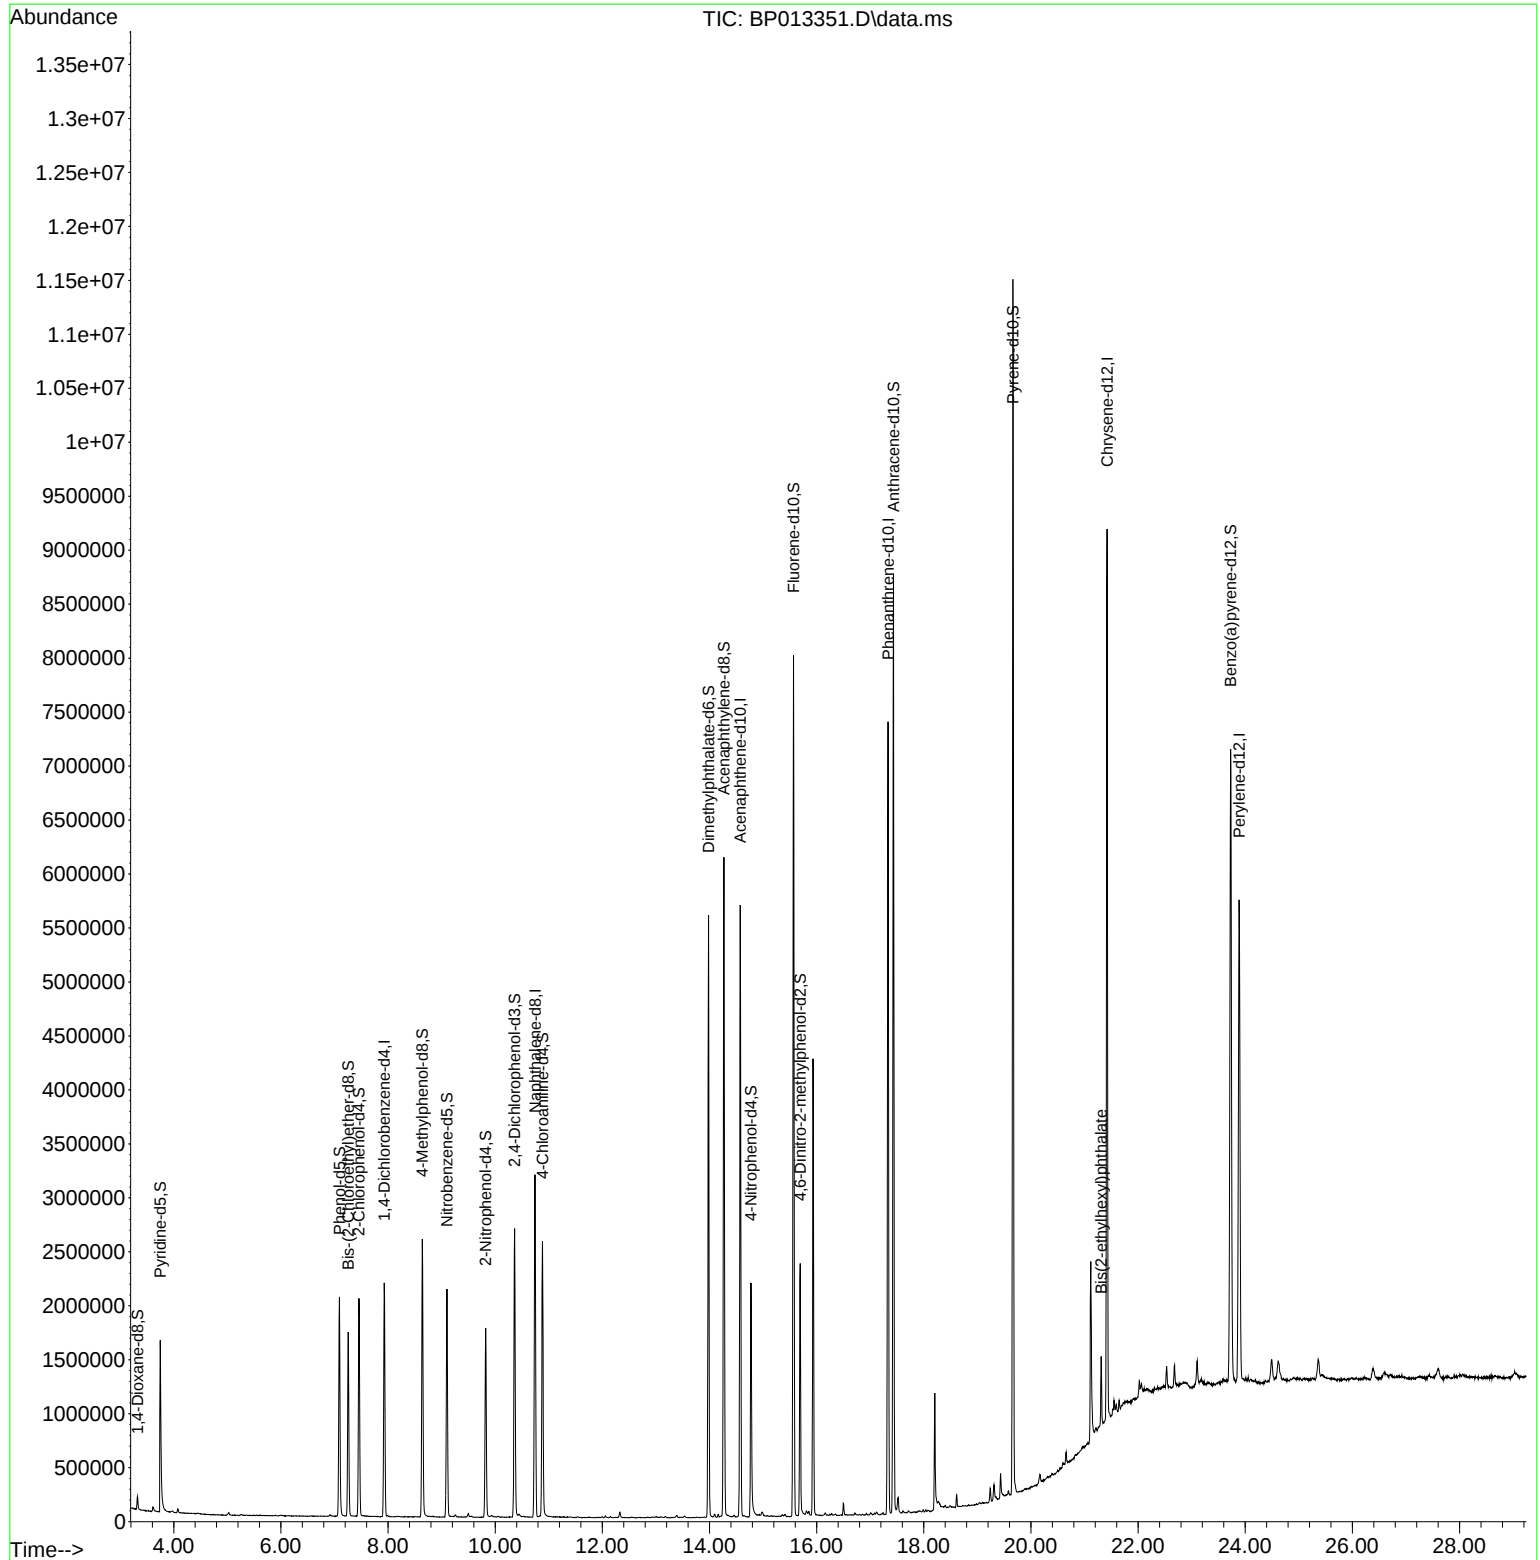

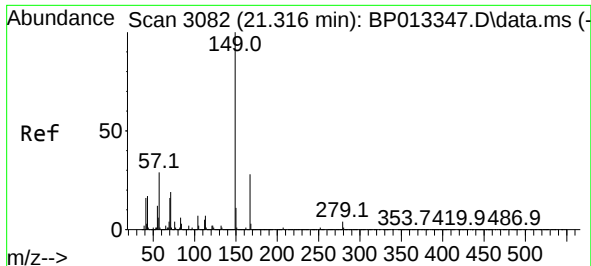

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.326 ng/ul
 RT: 21.310 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP013351.D
 Acq: 28 Dec 2022 14:38

Instrument :
 BNA_P
 ClientSampleId :
 A43T5

Tgt Ion:149 Resp: 197920
 Ion Ratio Lower Upper
 149 100
 167 27.6 22.5 33.7
 279 4.9 3.8 5.8

