

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
 Data File : BP013348.D
 Acq On : 28 Dec 2022 12:06
 Operator : CG/JU
 Sample : PB149897BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	28	rVB	104568	139782	1.03%	0.111%
2	3.746	93	95	114	rBV	1347202	2208752	16.22%	1.758%
3	4.075	147	151	156	rVB	32205	45952	0.34%	0.037%
4	7.093	652	664	675	rBV	1660733	2604560	19.12%	2.073%
5	7.257	686	692	707	rVB	1408839	2160029	15.86%	1.719%
6	7.457	719	726	735	rBV	1726701	2639892	19.38%	2.101%
7	7.928	799	806	815	rBV	1553466	2410643	17.70%	1.918%
8	8.640	919	927	943	rBV	2008192	3287029	24.13%	2.616%
9	9.099	997	1005	1015	rBV	1662387	2662476	19.55%	2.119%
10	9.822	1118	1128	1141	rBV	1362470	2231798	16.38%	1.776%
11	9.922	1141	1145	1153	rVB10	9467	24799	0.18%	0.020%
12	10.363	1212	1220	1230	rBV	2038616	3422906	25.13%	2.724%
13	10.440	1230	1233	1240	rVB5	22542	42938	0.32%	0.034%
14	10.740	1277	1284	1294	rBV	2238678	3711703	27.25%	2.954%
15	10.881	1300	1308	1324	rBV	2127964	3643671	26.75%	2.900%
16	12.328	1547	1554	1560	rBV	37620	62617	0.46%	0.050%
17	13.545	1756	1761	1766	rBV7	8139	13995	0.10%	0.011%
18	13.981	1828	1835	1847	rBV	4399032	5936391	43.58%	4.724%
19	14.269	1877	1884	1901	rBV	4674998	6631024	48.68%	5.277%
20	14.575	1928	1936	1945	rBV	3820426	5546179	40.72%	4.414%
21	14.775	1963	1970	1987	rBV	1752766	2815702	20.67%	2.241%
22	14.986	2002	2006	2010	rVB7	10623	18227	0.13%	0.015%
23	15.569	2098	2105	2118	rBV	6238297	8792682	64.55%	6.997%
24	15.692	2119	2126	2137	rVV	1956194	2663663	19.55%	2.120%
25	15.810	2140	2146	2152	rVB3	29593	59270	0.44%	0.047%
26	16.351	2233	2238	2244	rBV10	7895	17000	0.12%	0.014%
27	17.004	2346	2349	2356	rBV9	11030	16953	0.12%	0.013%
28	17.116	2365	2368	2373	rVB4	12986	16919	0.12%	0.013%
29	17.333	2398	2405	2414	rBV	5304328	7247575	53.21%	5.767%
30	17.433	2415	2422	2437	rBV	7230628	9945856	73.02%	7.915%
31	17.992	2514	2517	2523	rVB7	12659	14871	0.11%	0.012%
32	18.204	2549	2553	2559	rBV5	32272	54860	0.40%	0.044%
33	19.239	2725	2729	2736	rBV3	93829	144114	1.06%	0.115%
34	19.310	2737	2741	2745	rVV	84914	115543	0.85%	0.092%
35	19.663	2796	2801	2807	rBV	9927198	12757703	93.66%	10.152%
36	21.421	3094	3100	3111	rBV	6574093	8928229	65.55%	7.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013348.D
Acq On : 28 Dec 2022 12:06
Operator : CG/JU
Sample : PB149897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	23.727	3485	3492	3505	rVB2	6731330	13621470	100.00%	10.840%
38	23.886	3513	3519	3532	rVB2	4381699	9005457	66.11%	7.166%




Sum of corrected areas: 125663230

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013348.D
Acq On : 28 Dec 2022 12:06
Operator : CG/JU
Sample : PB149897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

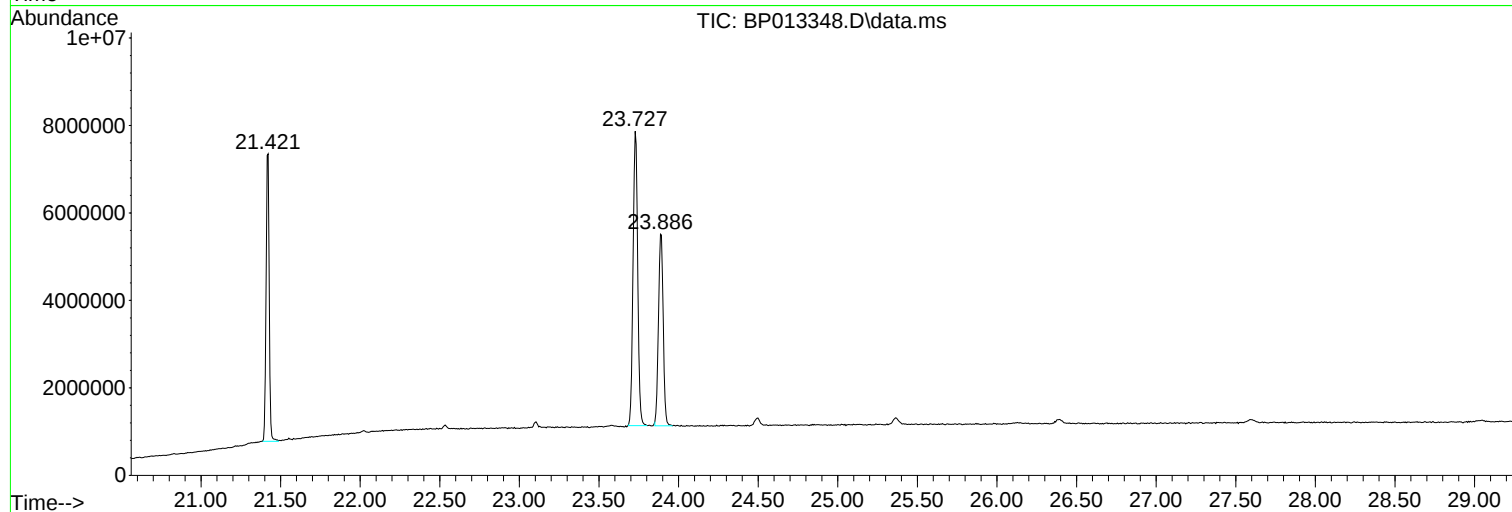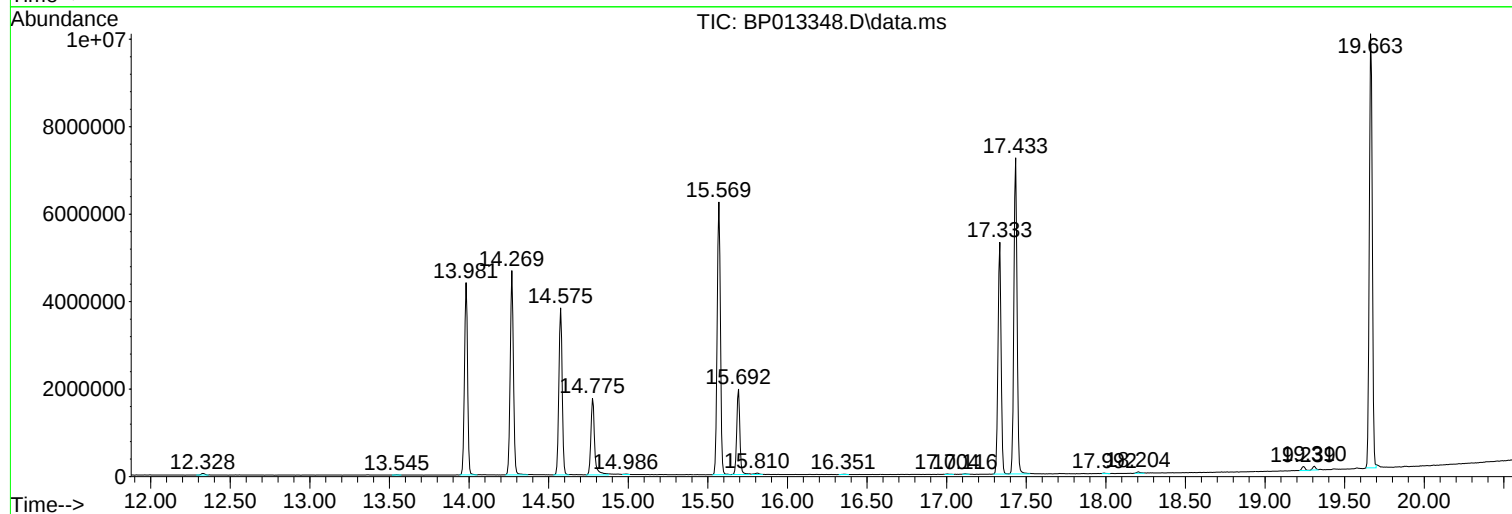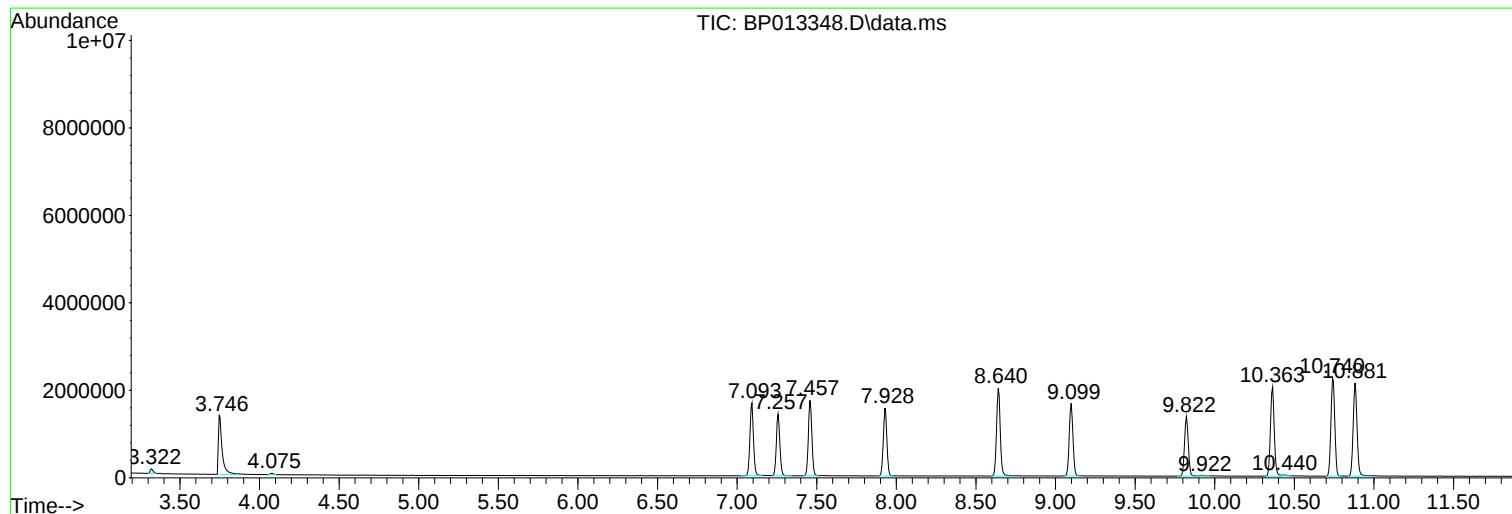

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013348.D
Acq On : 28 Dec 2022 12:06
Operator : CG/JU
Sample : PB149897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122822\
Data File : BP013348.D
Acq On : 28 Dec 2022 12:06
Operator : CG/JU
Sample : PB149897BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc