




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019146.D
 Acq On : 29 Dec 2023 03:53
 Operator : MA/JU
 Sample : 05986-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG2

Manual IntegrationsAPPROVED

Quant Time: Dec 29 04:24:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/29/2023
 Supervised By :mohammad ahmed 01/01/2024

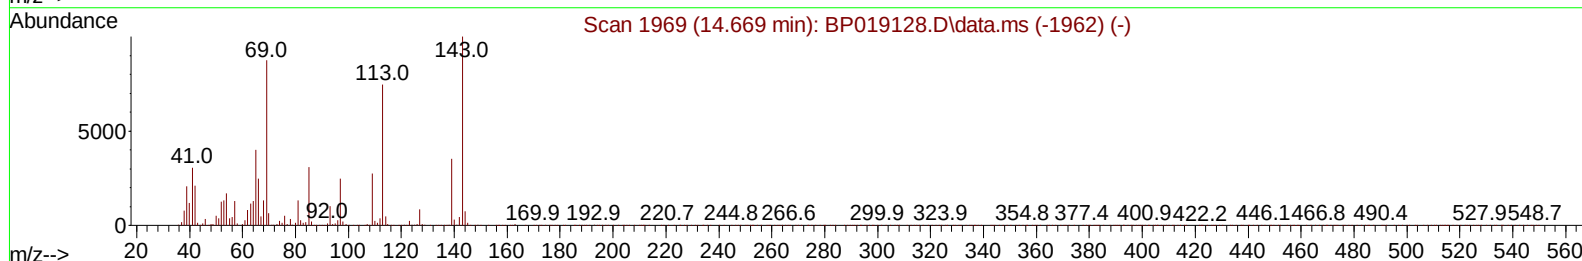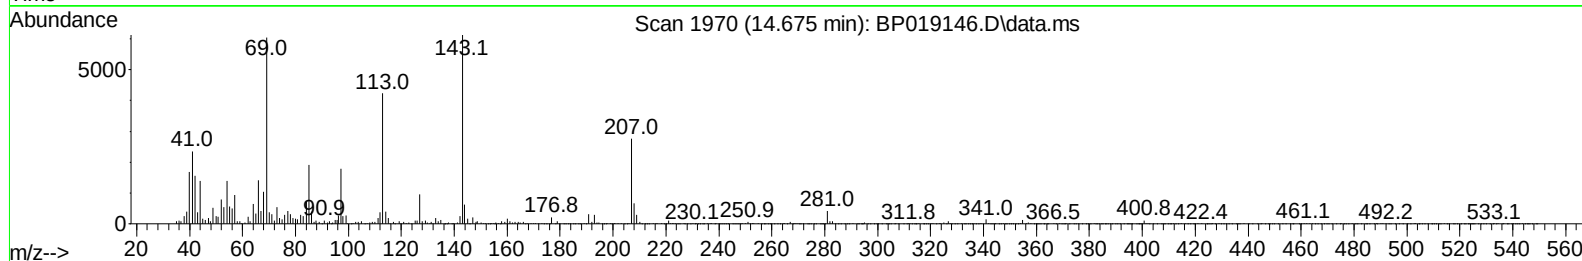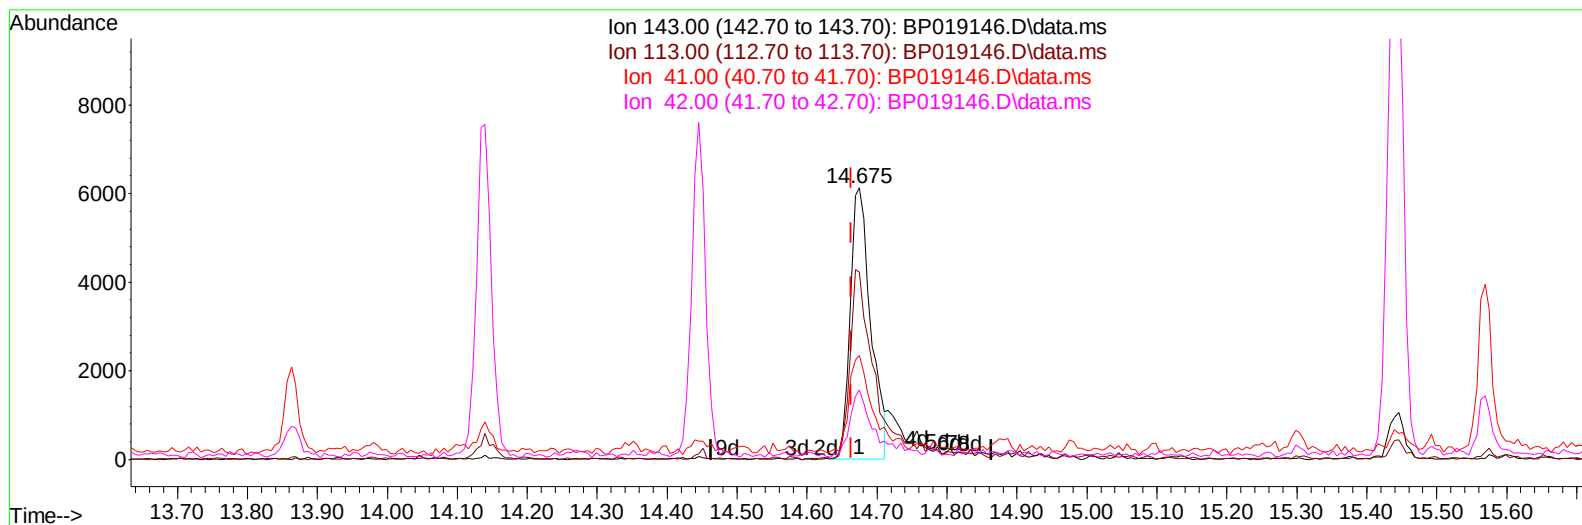

TIC: BP019146.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.012) 2.05 ng/ul

response 12367

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	73.50	69.01
41.00	33.40	38.39
42.00	23.00	25.59




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019146.D
Acq On : 29 Dec 2023 03:53
Operator : MA/JU
Sample : 05986-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Quant Time: Dec 29 04:24:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :mohammad ahmed 01/01/2024

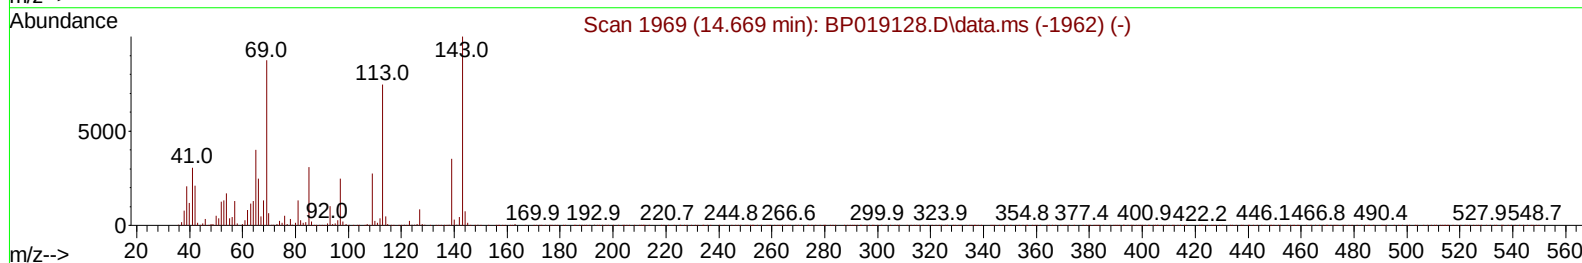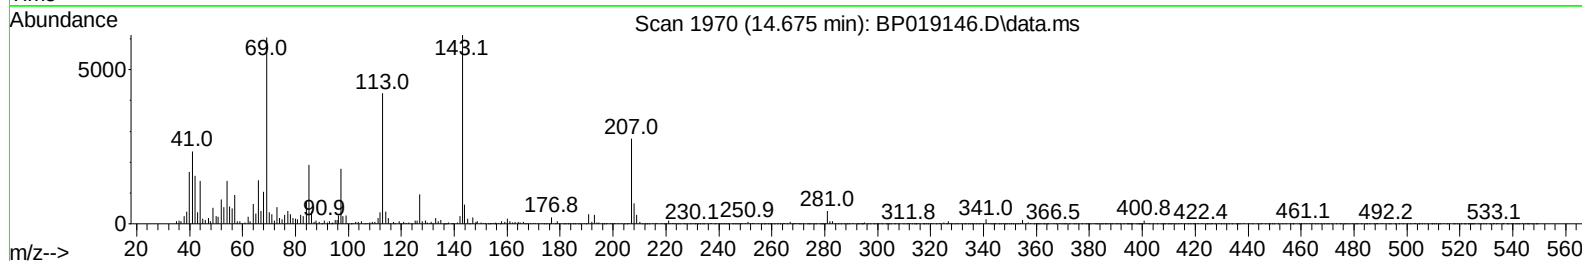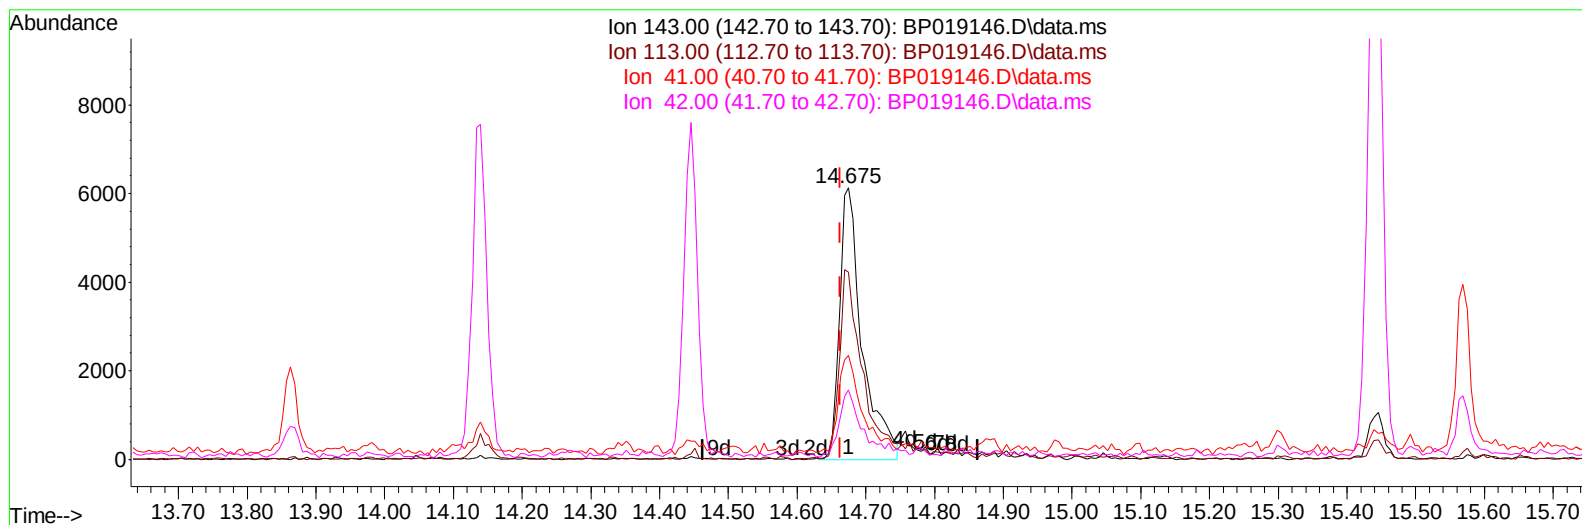

TIC: BP019146.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.012) 2.31 ng/ul m

response 13980

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	73.50	69.01
41.00	33.40	38.39
42.00	23.00	25.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019146.D
 Acq On : 29 Dec 2023 03:53
 Operator : MA/JU
 Sample : 05986-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/29/2023
 Supervised By :mohammad ahmed 01/01/2024

Quant Time: Dec 29 04:25:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	166870	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	638856	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	405405	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	962344	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1100401	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1288023	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	18100	3.704	ng/uL	0.00
4) Pyridine-d5	3.658	84	89373	7.288	ng/ul	0.00
7) Phenol-d5	6.981	99	47157	3.151	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	250823	28.973	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	131849	10.929	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	95815	8.224	ng/ul	0.00
21) Nitrobenzene-d5	8.969	128	152045	27.532	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	81319	13.625	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	154017	12.779	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	324137	21.865	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	1077403	30.088	ng/ul	0.00
49) Acenaphthylene-d8	14.140	160	1102315	28.371	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	13980m	2.312	ng/ul	0.01
60) Fluorene-d10	15.439	176	961365	31.076	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	80678	12.788	ng/ul	0.00
73) Anthracene-d10	17.304	188	1641282	32.658	ng/ul	0.00
81) Pyrene-d10	19.545	212	2252784	33.592	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.521	264	2366612	31.966	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019146.D
Acq On : 29 Dec 2023 03:53
Operator : MA/JU
Sample : 05986-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG2

Manual IntegrationsAPPROVED

Quant Time: Dec 29 04:25:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :mohammad ahmed 01/01/2024

