




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019181.D
Acq On : 30 Dec 2023 00:22
Operator : MA/JU
Sample : PB158060BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK060

Manual IntegrationsAPPROVED

Quant Time: Dec 30 00:53:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

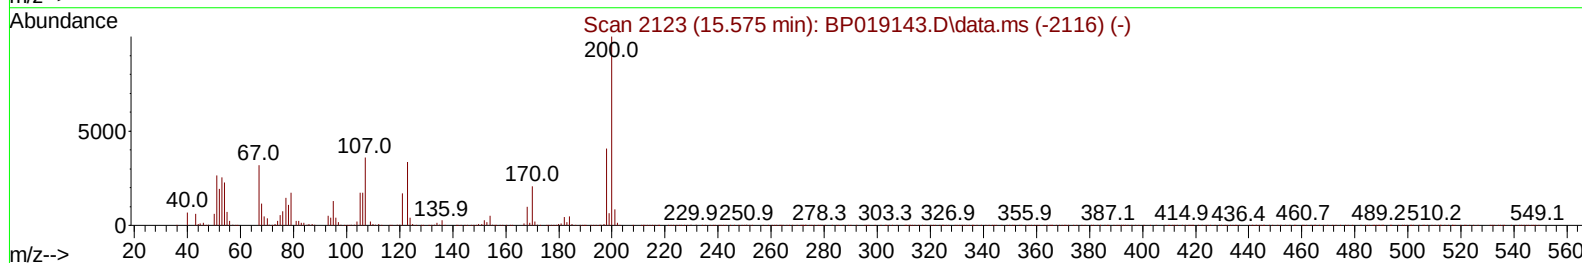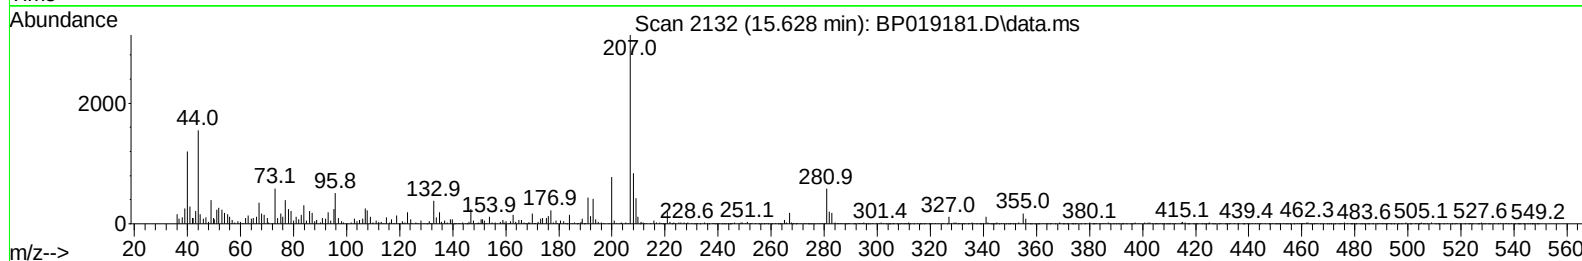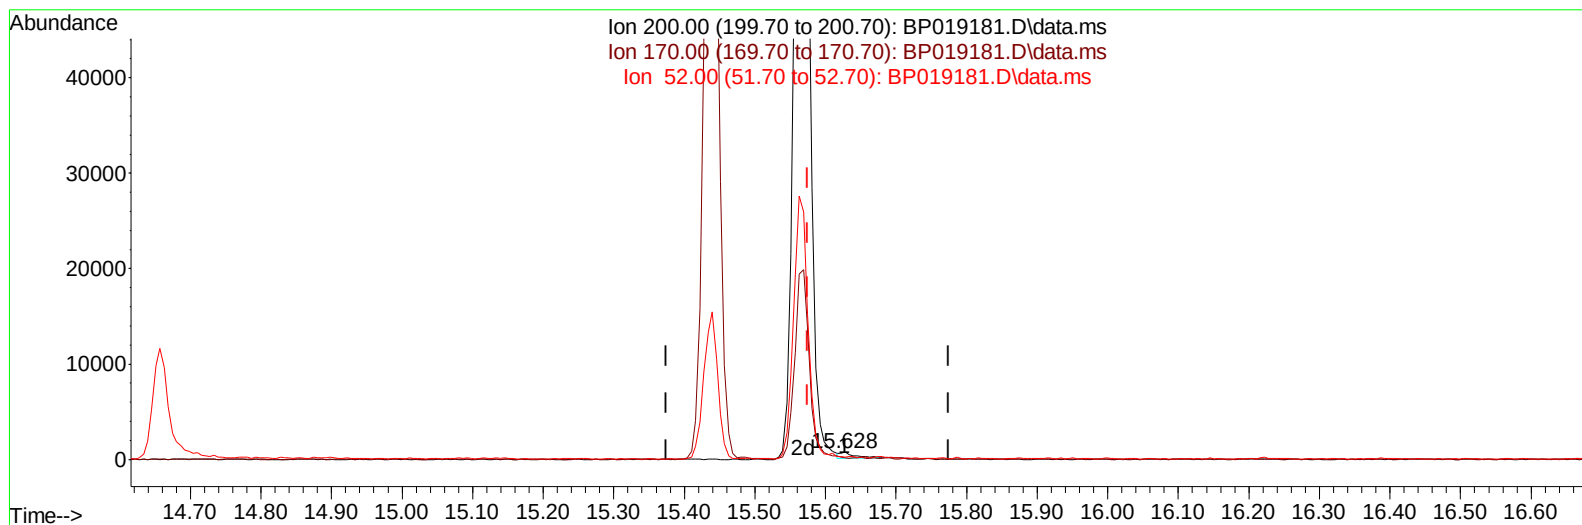

TIC: BP019181.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.628min (+ 0.053) 0.15 ng/ul

response 973

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.60	22.35
52.00	34.00	34.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019181.D
 Acq On : 30 Dec 2023 00:22
 Operator : MA/JU
 Sample : PB158060BL
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK060

Manual IntegrationsAPPROVED

Quant Time: Dec 30 00:53:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

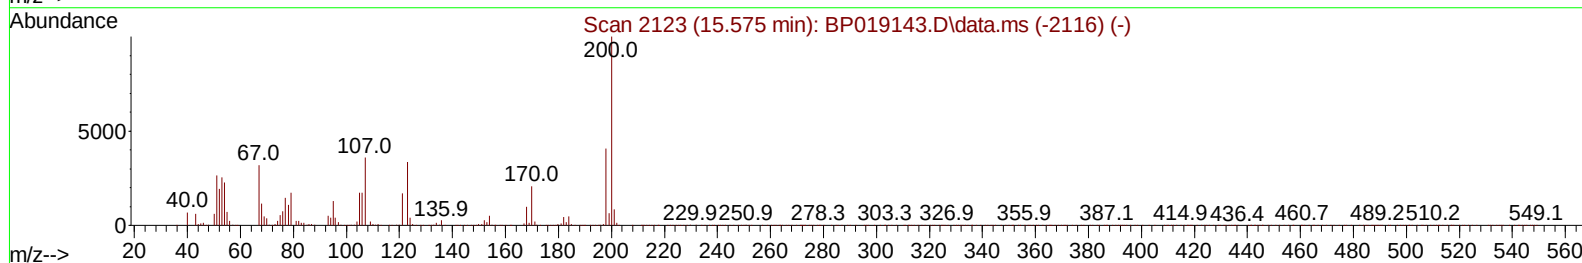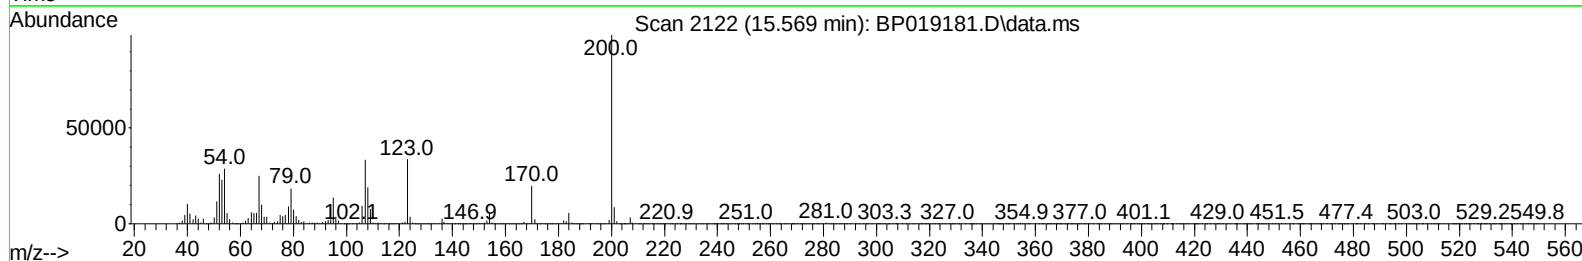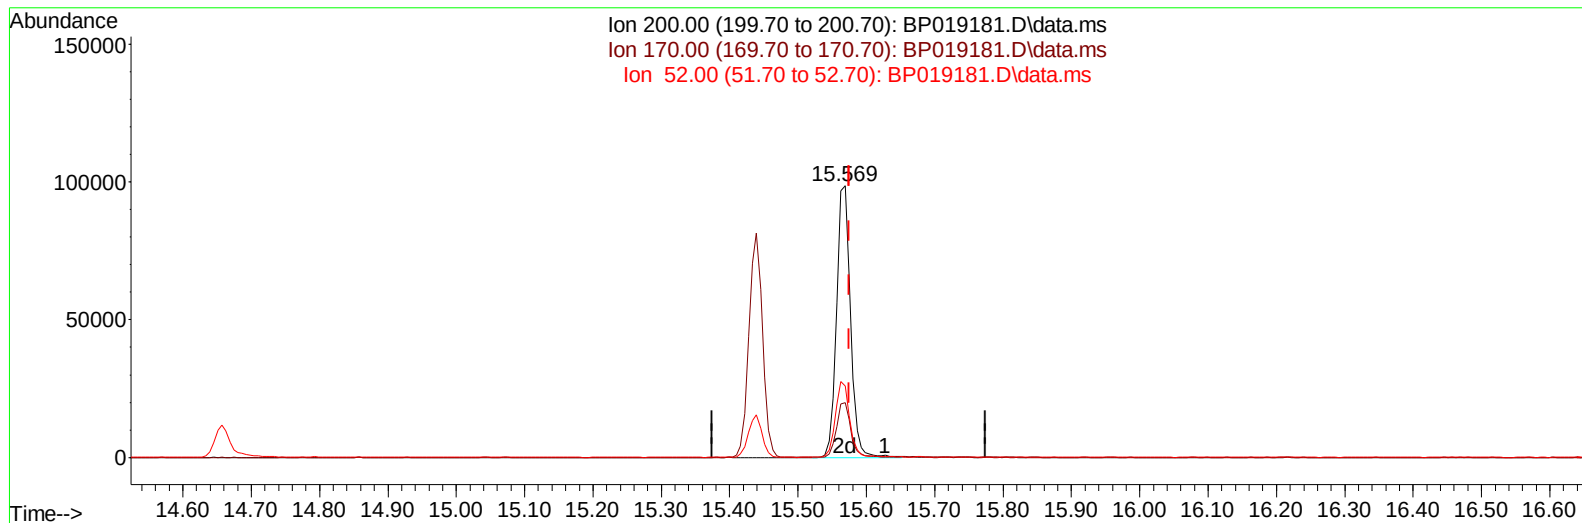

TIC: BP019181.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.569min (-0.006) 21.69 ng/ul m

response 139531

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.60	20.17
52.00	34.00	26.31#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019181.D
 Acq On : 30 Dec 2023 00:22
 Operator : MA/JU
 Sample : PB158060BL
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK060

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

Quant Time: Dec 30 01:01:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	237384	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	866507	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	478949	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	981308	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1018009	20.000	ng/ul	-0.01
88) Perylene-d12	23.662	264	1253253	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	40923	5.888	ng/uL	0.00
4) Pyridine-d5	3.652	84	520542	29.838	ng/ul	0.00
7) Phenol-d5	6.975	99	585890	27.522	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	356101	28.915	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	469737	27.371	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	442514	26.700	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	208647	27.855	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	224273	27.704	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	435893	26.665	ng/ul	0.00
31) 4-Chloroaniline-d4	10.740	131	572420	28.469	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	1120870	26.495	ng/ul	0.00
49) Acenaphthylene-d8	14.134	160	1301991	28.364	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	154783	21.667	ng/ul	0.00
60) Fluorene-d10	15.439	176	956285	26.166	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	139531m	21.689	ng/ul	0.00
73) Anthracene-d10	17.298	188	1459919	28.488	ng/ul	0.00
81) Pyrene-d10	19.539	212	1744641	28.120	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	2054868	28.525	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019181.D
Acq On : 30 Dec 2023 00:22
Operator : MA/JU
Sample : PB158060BL
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK060

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

Quant Time: Dec 30 01:01:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

