




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019186.D
 Acq On : 30 Dec 2023 03:13
 Operator : MA/JU
 Sample : 06020-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:48:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

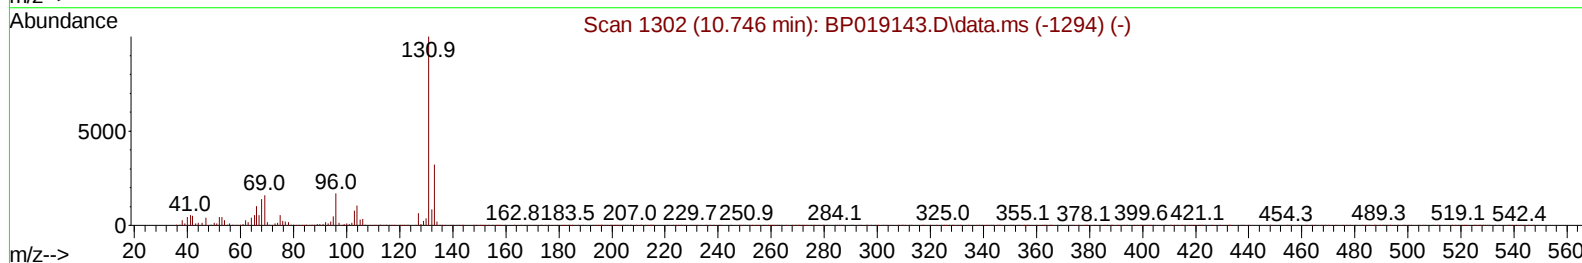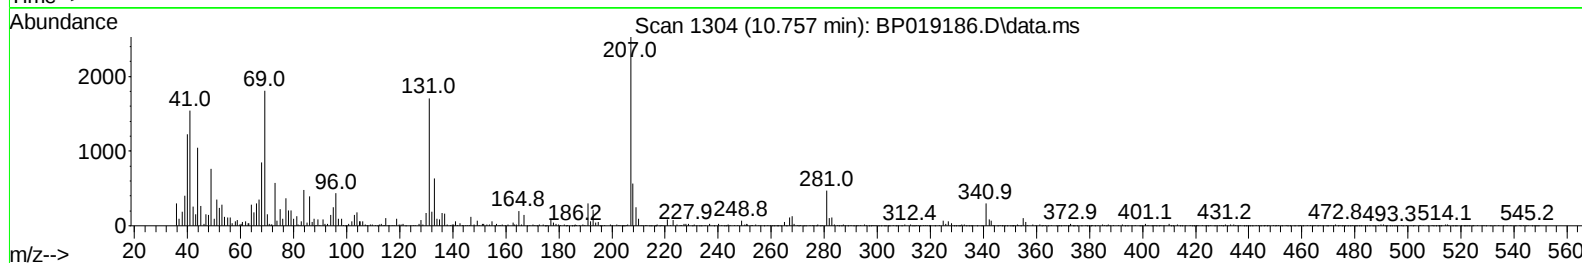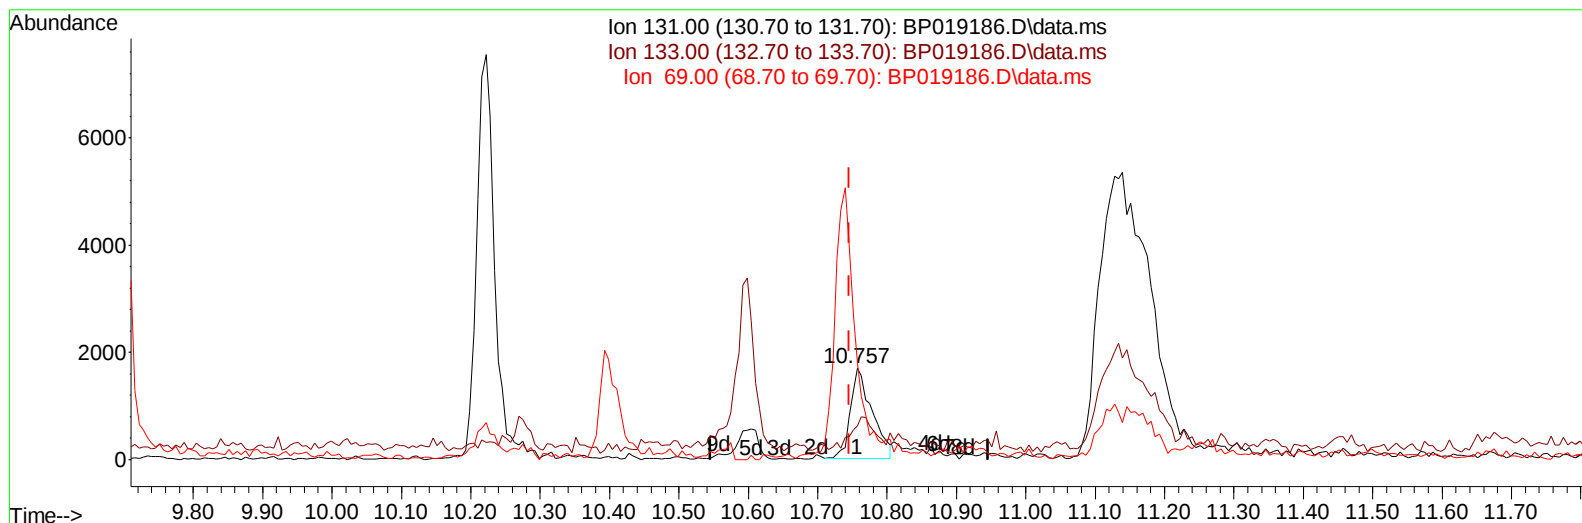

TIC: BP019186.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.757min (+ 0.012) 0.23 ng/u1

response 3663

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	37.02
69.00	16.10	105.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019186.D
 Acq On : 30 Dec 2023 03:13
 Operator : MA/JU
 Sample : 06020-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:48:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

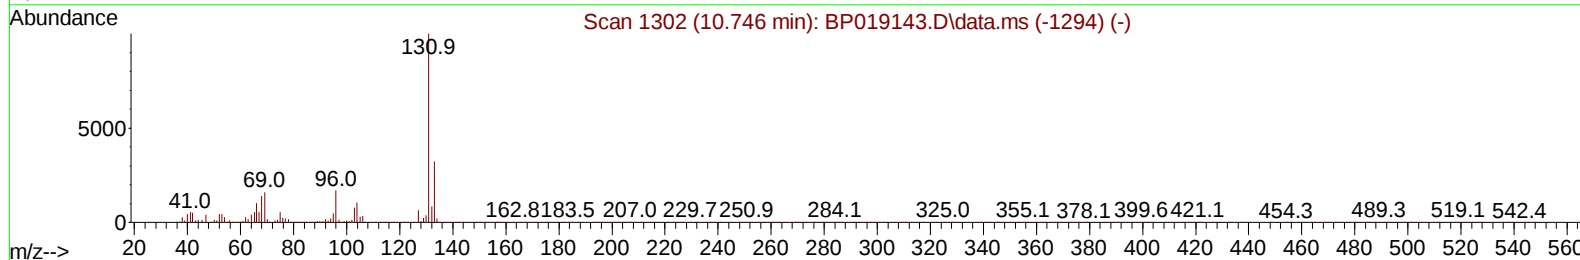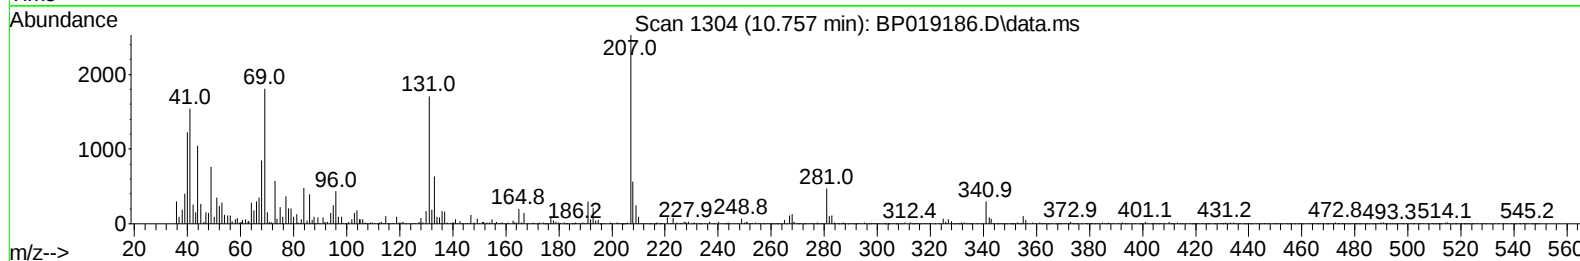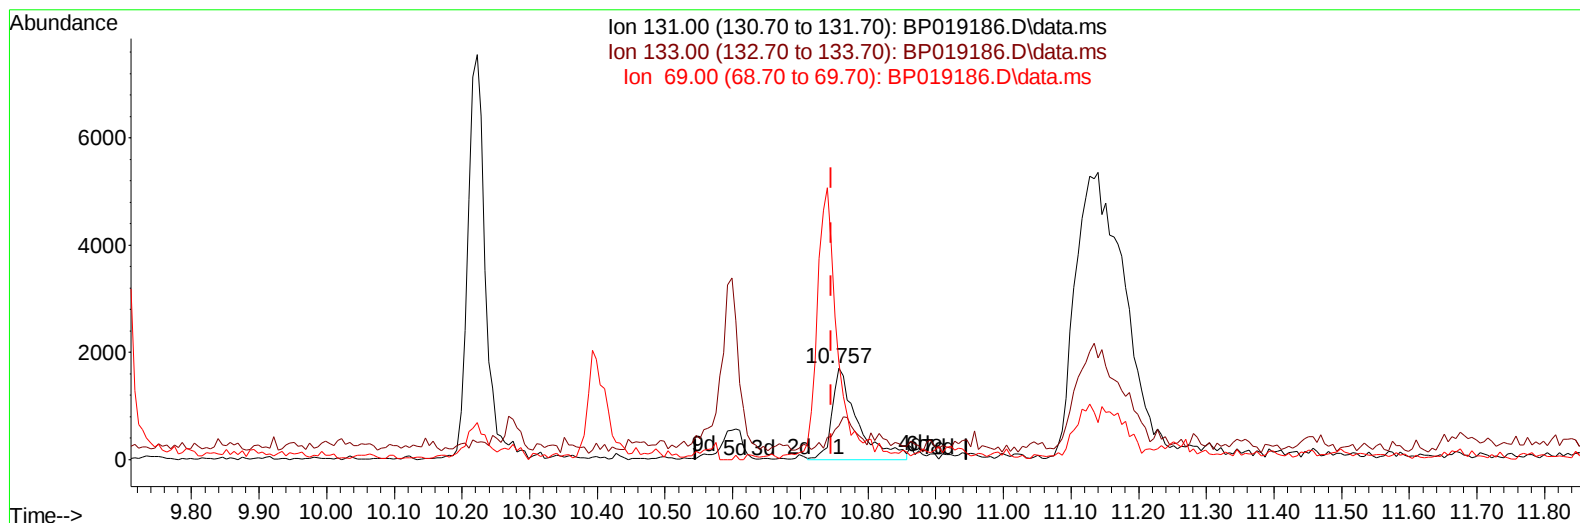

TIC: BP019186.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.757min (+ 0.012) 0.28 ng/ul m

response 4420

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	37.02
69.00	16.10	105.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019186.D
 Acq On : 30 Dec 2023 03:13
 Operator : MA/JU
 Sample : 06020-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:49:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

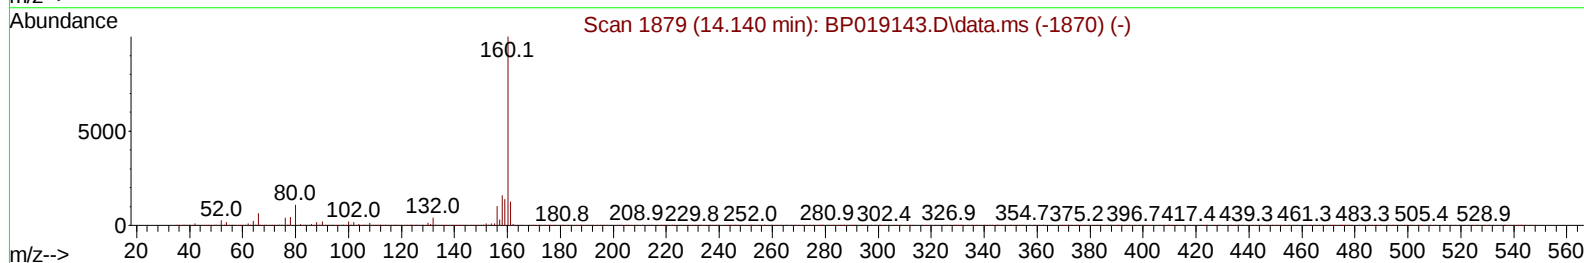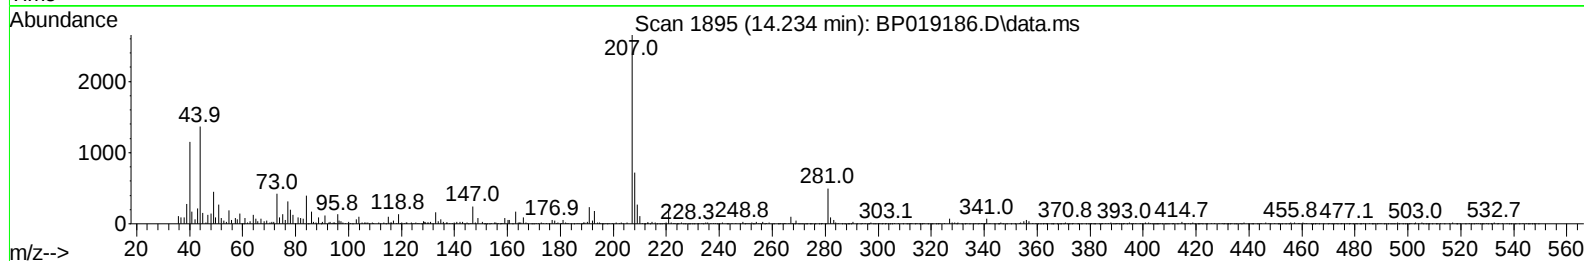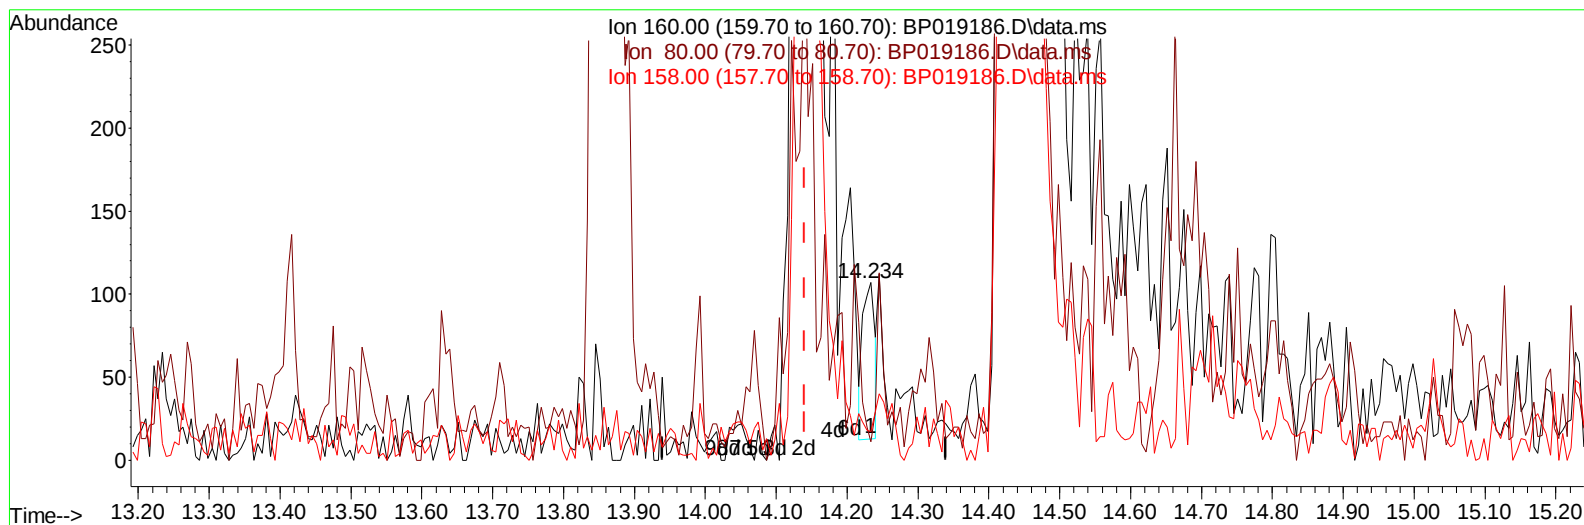

TIC: BP019186.D\data.ms

(49) Acenaphthylene-d8 (S)

14.234min (+ 0.094) 0.00 ng/u1

response	112
Ion	Exp% Act%
160.00	100.00 100.00
80.00	10.90 10.28
158.00	16.10 15.89
0.00	0.00 0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019186.D
 Acq On : 30 Dec 2023 03:13
 Operator : MA/JU
 Sample : 06020-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:49:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

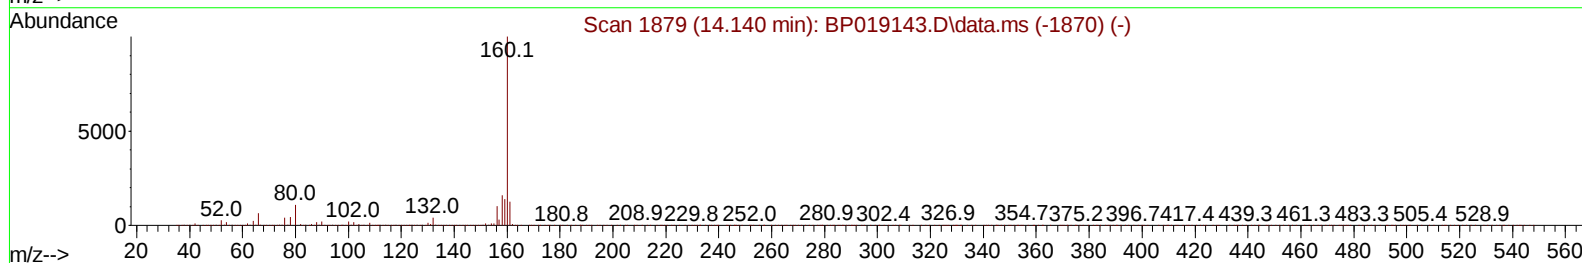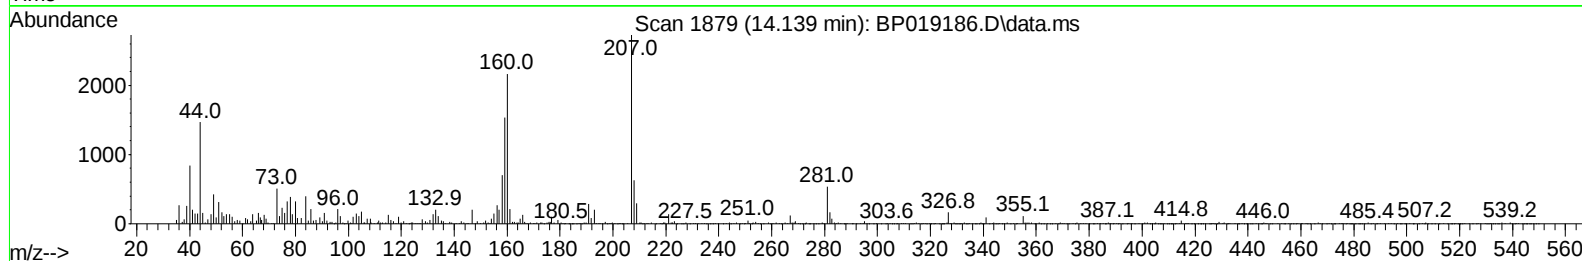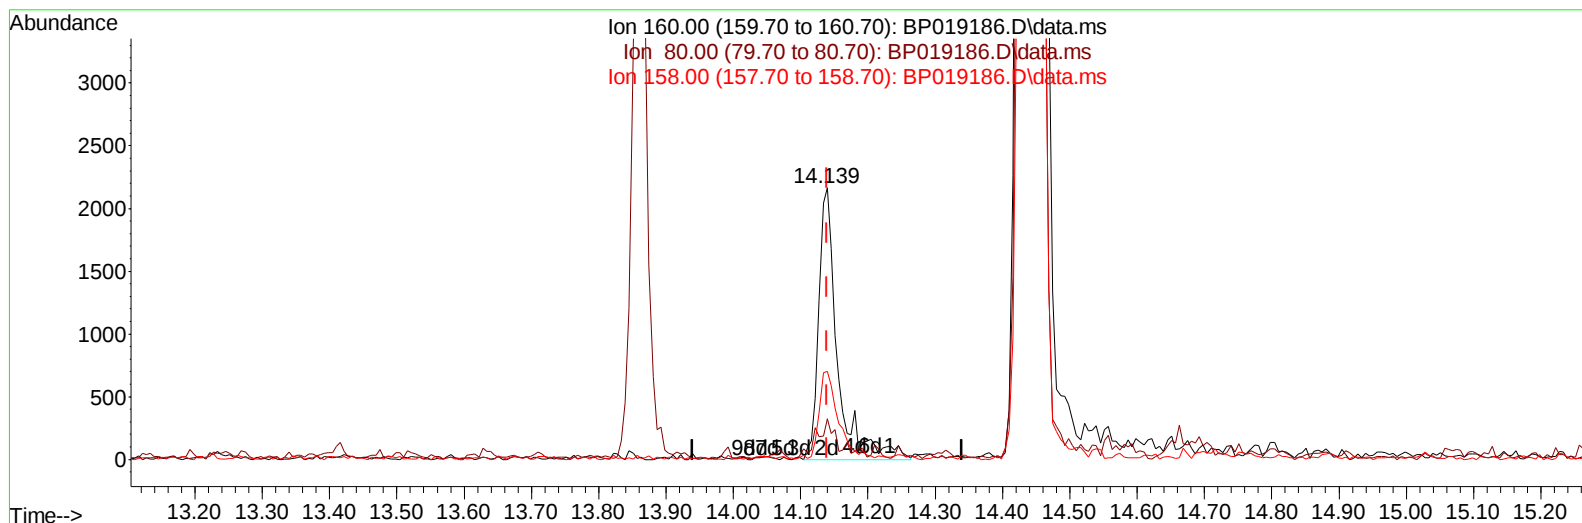

TIC: BP019186.D\data.ms

(49) Acenaphthylene-d8 (S)

14.139min (-0.000) 0.11 ng/ul m

response 4207

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	10.90	14.97#
158.00	16.10	32.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019186.D
 Acq On : 30 Dec 2023 03:13
 Operator : MA/JU
 Sample : 06020-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:48:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

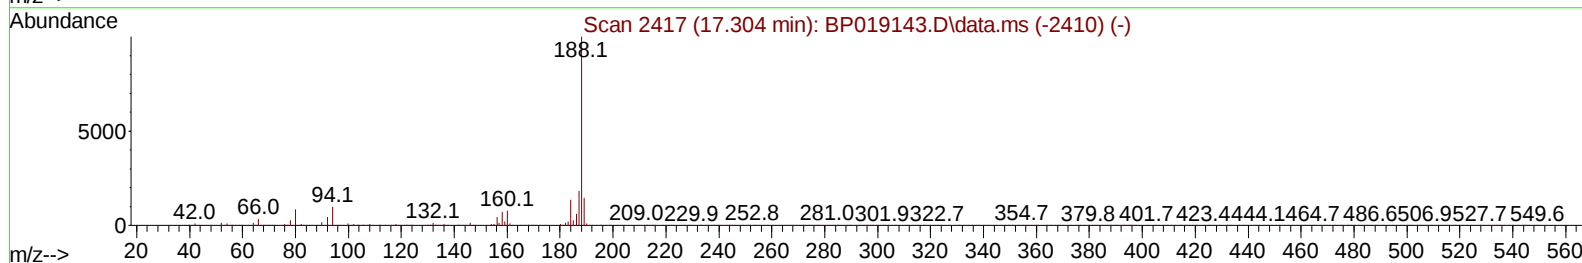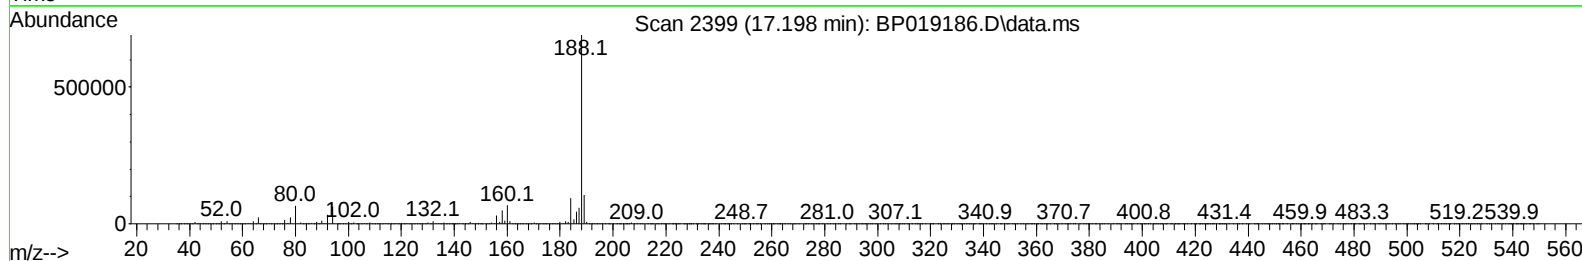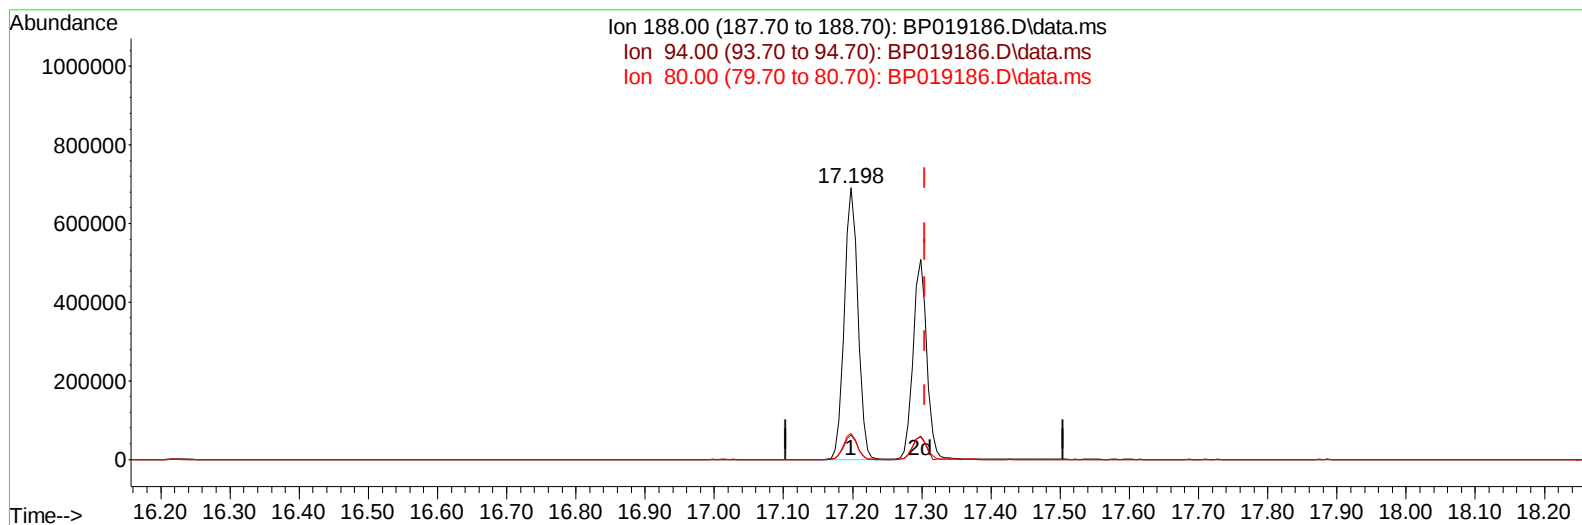

TIC: BP019186.D\data.ms

(73) Anthracene-d10 (S)

17.198min (-0.106) 19.15 ng/u1

response 941855

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.50	9.00
80.00	9.10	9.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019186.D
Acq On : 30 Dec 2023 03:13
Operator : MA/JU
Sample : 06020-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:48:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

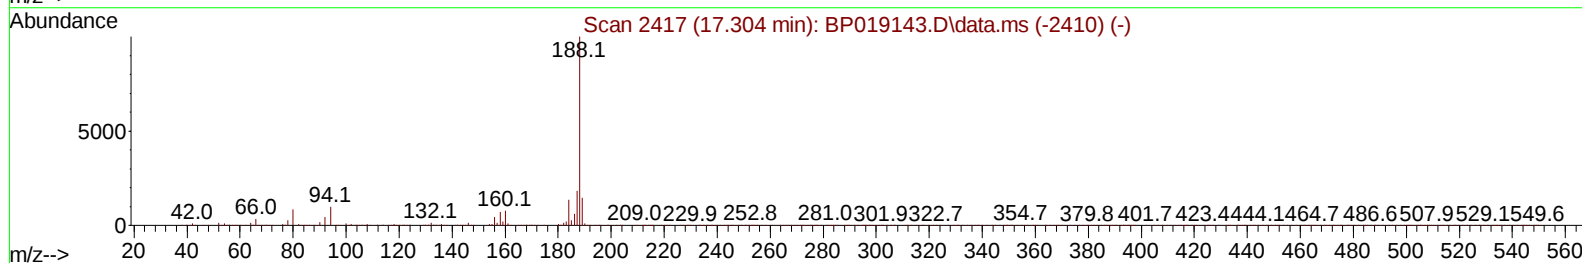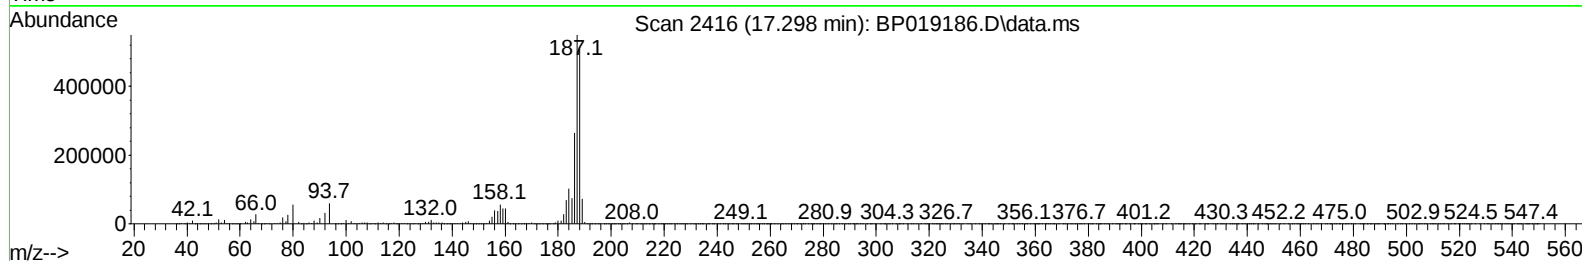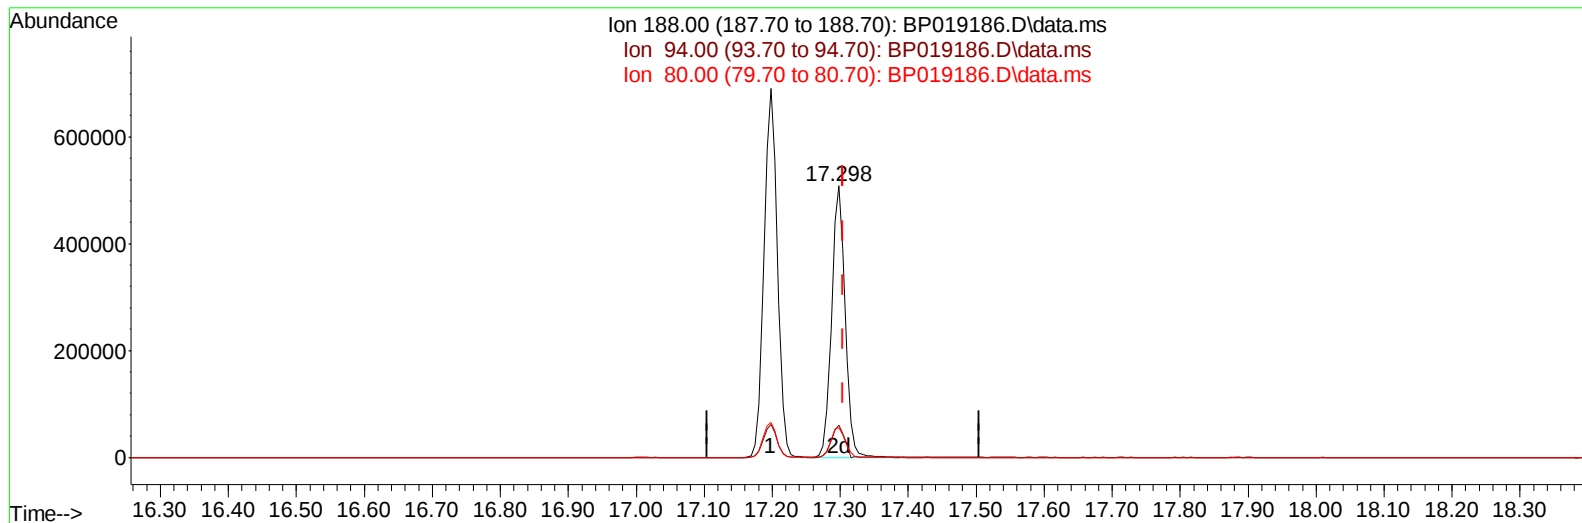

TIC: BP019186.D\data.ms

(73) Anthracene-d10 (S)

17.298min (-0.006) 14.26 ng/ul m

response 701568

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.50	11.84
80.00	9.10	11.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019186.D
 Acq On : 30 Dec 2023 03:13
 Operator : MA/JU
 Sample : 06020-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

Quant Time: Dec 30 03:50:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	178003	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	680200	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	409057	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	941855	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1008690	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1013793	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	26231	5.033	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.975	99	64593	4.046	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	376304	40.749	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	375648	29.190	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	130169	10.474	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	222503	37.841	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	232235	36.545	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	433045	33.747	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	4420m	0.280	ng/ul	0.01
46) Dimethylphthalate-d6	13.863	166	1247785	34.535	ng/ul	0.00
49) Acenaphthylene-d8	14.139	160	4207m	0.107	ng/ul	0.00
54) 4-Nitrophenol-d4	14.663	143	35638	5.841	ng/ul	0.00
60) Fluorene-d10	15.439	176	982114	31.464	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	187275	30.330	ng/ul	0.00
73) Anthracene-d10	17.298	188	701568m	14.263	ng/ul	0.00
81) Pyrene-d10	19.545	212	1364167	22.191	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	378182	6.490	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019186.D
Acq On : 30 Dec 2023 03:13
Operator : MA/JU
Sample : 06020-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P1

Manual IntegrationsAPPROVED

Quant Time: Dec 30 03:50:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

