




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019190.D
Acq On : 30 Dec 2023 05:30
Operator : MA/JU
Sample : 06020-12
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X7

Manual IntegrationsAPPROVED

Quant Time: Jan 01 00:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

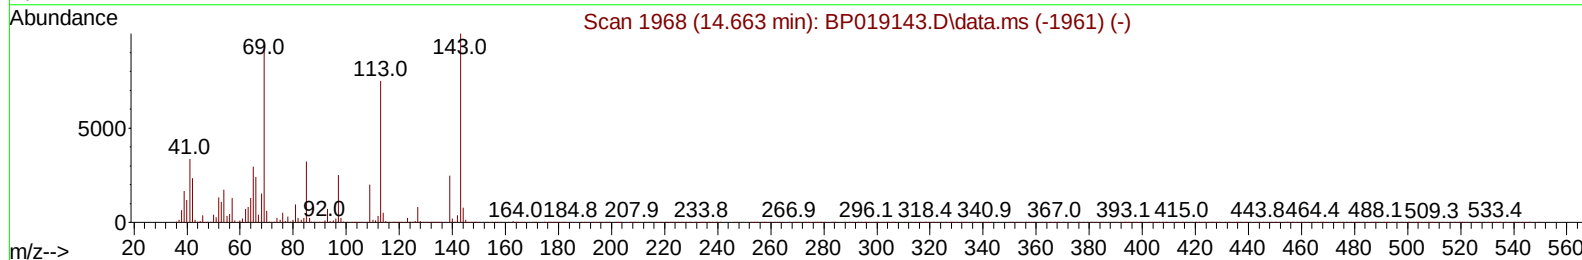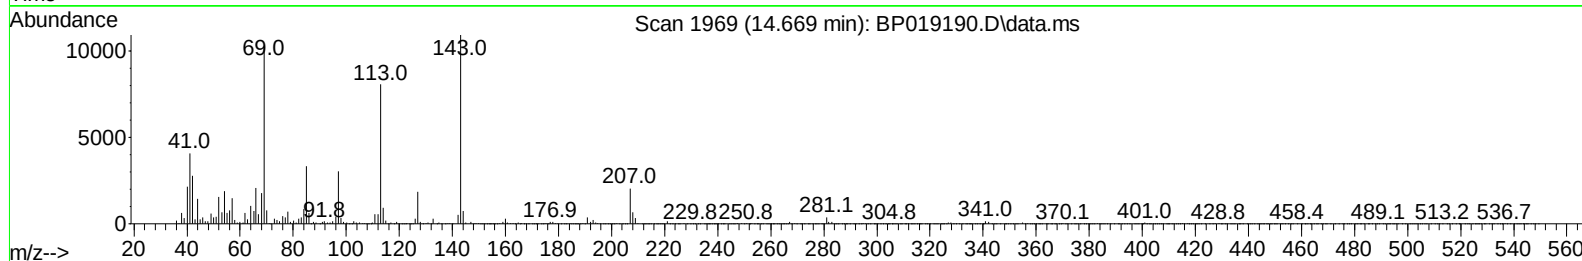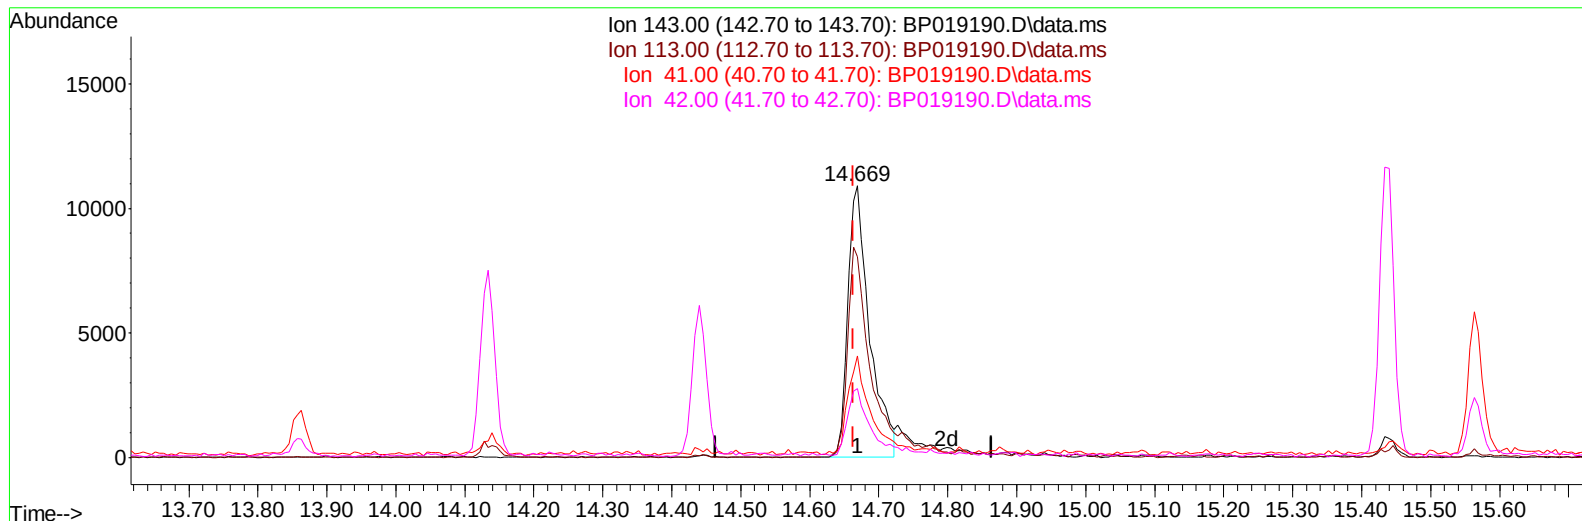

TIC: BP019190.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (+ 0.006) 4.68 ng/ul

response 23812

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	73.50	73.89
41.00	33.40	37.31
42.00	23.00	25.42




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019190.D
 Acq On : 30 Dec 2023 05:30
 Operator : MA/JU
 Sample : 06020-12
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X7

Manual IntegrationsAPPROVED

Quant Time: Jan 01 00:19:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

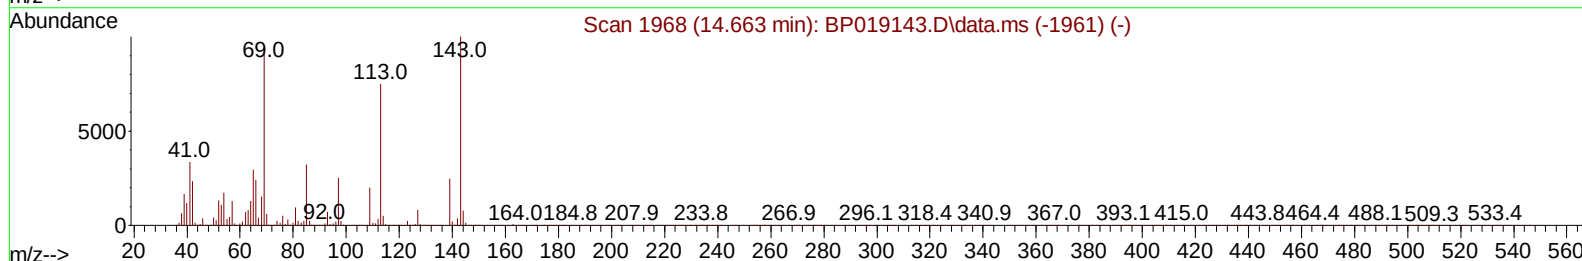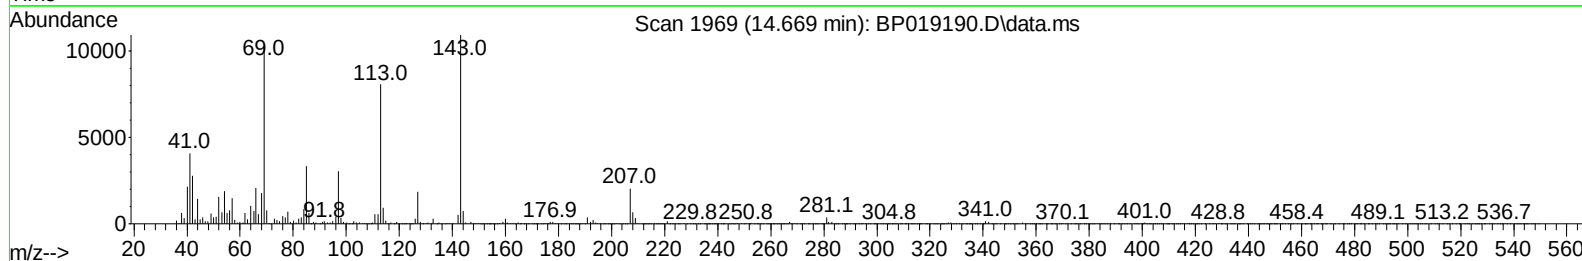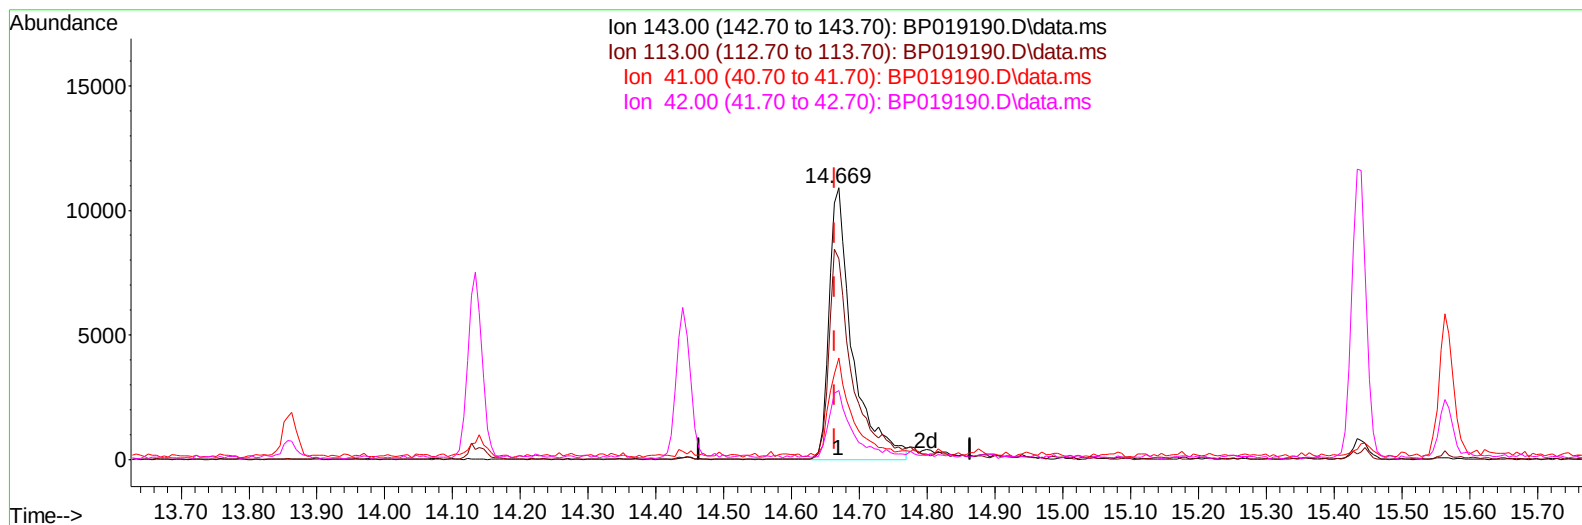

TIC: BP019190.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (+ 0.006) 5.11 ng/ul m

response 25980

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	73.50	73.89
41.00	33.40	37.31
42.00	23.00	25.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019190.D
 Acq On : 30 Dec 2023 05:30
 Operator : MA/JU
 Sample : 06020-12
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/01/2024
 Supervised By :mohammad ahmed 01/01/2024

Quant Time: Jan 01 00:26:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	166493	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	605846	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.440	164	341030	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	766416	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	844752	20.000	ng/ul	0.00
88) Perylene-d12	23.663	264	1027951	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	21571	4.425	ng/uL	0.00
4) Pyridine-d5	3.658	84	116469	9.519	ng/ul	0.00
7) Phenol-d5	6.975	99	114086	7.641	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	284159	32.898	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	295636	24.561	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	188403	16.208	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	164943	31.495	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	162801	28.763	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	312339	27.328	ng/ul	0.00
31) 4-Chloroaniline-d4	10.740	131	385638	27.431	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	930139	30.879	ng/ul	0.00
49) Acenaphthylene-d8	14.134	160	1045678	31.993	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	25980m	5.108	ng/ul	0.00
60) Fluorene-d10	15.440	176	835018	32.087	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	127292	25.335	ng/ul	-0.01
73) Anthracene-d10	17.298	188	1421490	35.515	ng/ul	0.00
81) Pyrene-d10	19.539	212	1839541	35.731	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	2121733	35.909	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019190.D
Acq On : 30 Dec 2023 05:30
Operator : MA/JU
Sample : 06020-12
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X7

Manual IntegrationsAPPROVED

Quant Time: Jan 01 00:26:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 01/01/2024
Supervised By :mohammad ahmed 01/01/2024

