

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019148.D
 Acq On : 29 Dec 2023 05:01
 Operator : MA/JU
 Sample : 05986-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK7

Quant Time: Dec 29 05:30:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	166858	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	624429	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.446	164	390965	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	873670	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	922338	20.000	ng/ul	0.00
88) Perylene-d12	23.674	264	1113787	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	18912	3.871	ng/uL	0.00
4) Pyridine-d5	3.658	84	107519	8.768	ng/ul	0.00
7) Phenol-d5	6.981	99	94203	6.296	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	299824	34.635	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	291656	24.177	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	182342	15.652	ng/ul	0.00
21) Nitrobenzene-d5	8.969	128	184831	34.242	ng/ul	0.00
24) 2-Nitrophenol-d4	9.687	143	190962	32.735	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	342964	29.114	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	391641	27.029	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	1211982	35.096	ng/ul	0.00
49) Acenaphthylene-d8	14.140	160	1303168	34.779	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	28345	4.861	ng/ul	0.00
60) Fluorene-d10	15.445	176	1083010	36.302	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	174947	30.545	ng/ul	0.00
73) Anthracene-d10	17.304	188	1854174	40.639	ng/ul	0.00
81) Pyrene-d10	19.545	212	2314617	41.177	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.522	264	2695896	42.110	ng/ul	0.00
Target Compounds						
59) Diethylphthalate	15.275	149	40120	1.214	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019148.D
Acq On : 29 Dec 2023 05:01
Operator : MA/JU
Sample : 05986-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAK7

Quant Time: Dec 29 05:30:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

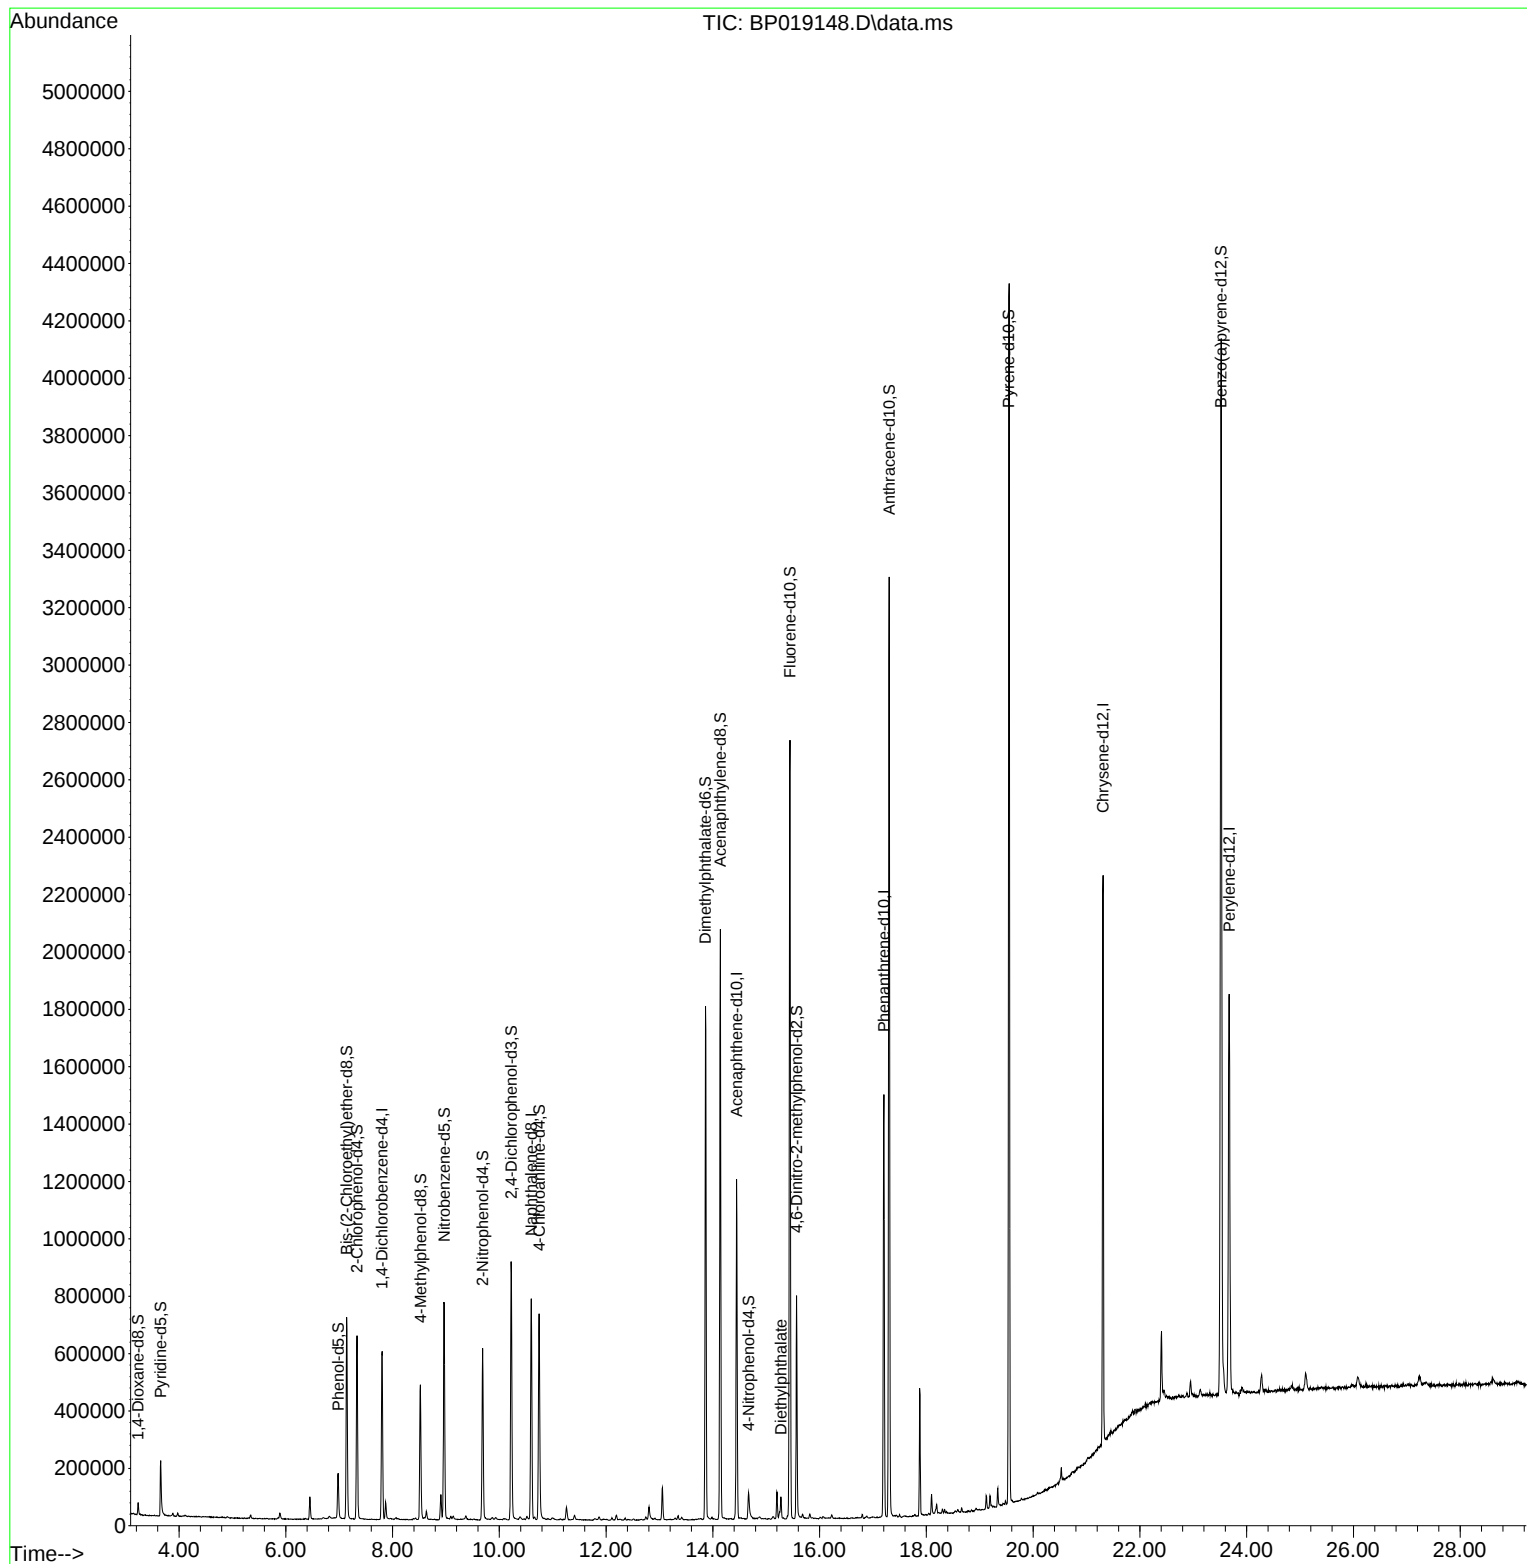

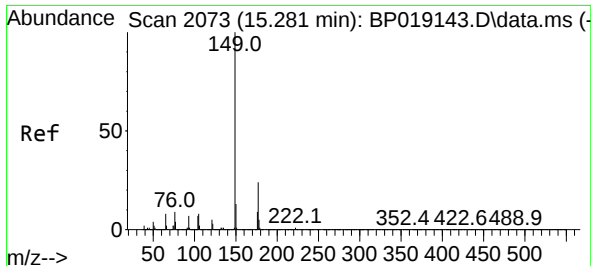

#59

Diethylphthalate

Concen: 1.214 ng/ul

RT: 15.275 min Scan# 2072

Delta R.T. -0.006 min

Lab File: BP019148.D


Acq: 29 Dec 2023 05:01

Instrument :

BNA_P

ClientSampleId :

C0AK7

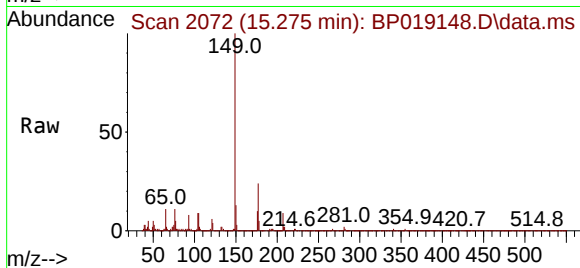

Tgt Ion:149 Resp: 40120

Ion Ratio Lower Upper

149 100

177 24.4 18.7 28.1

150 12.8 9.8 14.8

