

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019151.D
 Acq On : 29 Dec 2023 06:43
 Operator : MA/JU
 Sample : 06021-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z3

Quant Time: Dec 29 07:17:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	180300	20.000	ng/u1	0.00
20) Naphthalene-d8	10.599	136	702756	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.446	164	441007	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	1003278	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1115406	20.000	ng/u1	0.00
88) Perylene-d12	23.669	264	1310530	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	21657	4.102	ng/uL	0.00
4) Pyridine-d5	3.658	84	77095	5.818	ng/u1	0.00
7) Phenol-d5	6.981	99	131171	8.113	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	328308	35.098	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	345497	26.505	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	229376	18.222	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	208122	34.259	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	226659	34.523	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	408632	30.822	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	417998	25.633	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1336982	34.323	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1465864	34.682	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	43195	6.567	ng/u1	0.00
60) Fluorene-d10	15.440	176	1168106	34.711	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	212588	32.322	ng/u1	0.00
73) Anthracene-d10	17.304	188	1986023	37.905	ng/u1	0.00
81) Pyrene-d10	19.545	212	2535972	37.306	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	2891530	38.385	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.270	88	7288	1.256	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019151.D
Acq On : 29 Dec 2023 06:43
Operator : MA/JU
Sample : 06021-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z3

Quant Time: Dec 29 07:17:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

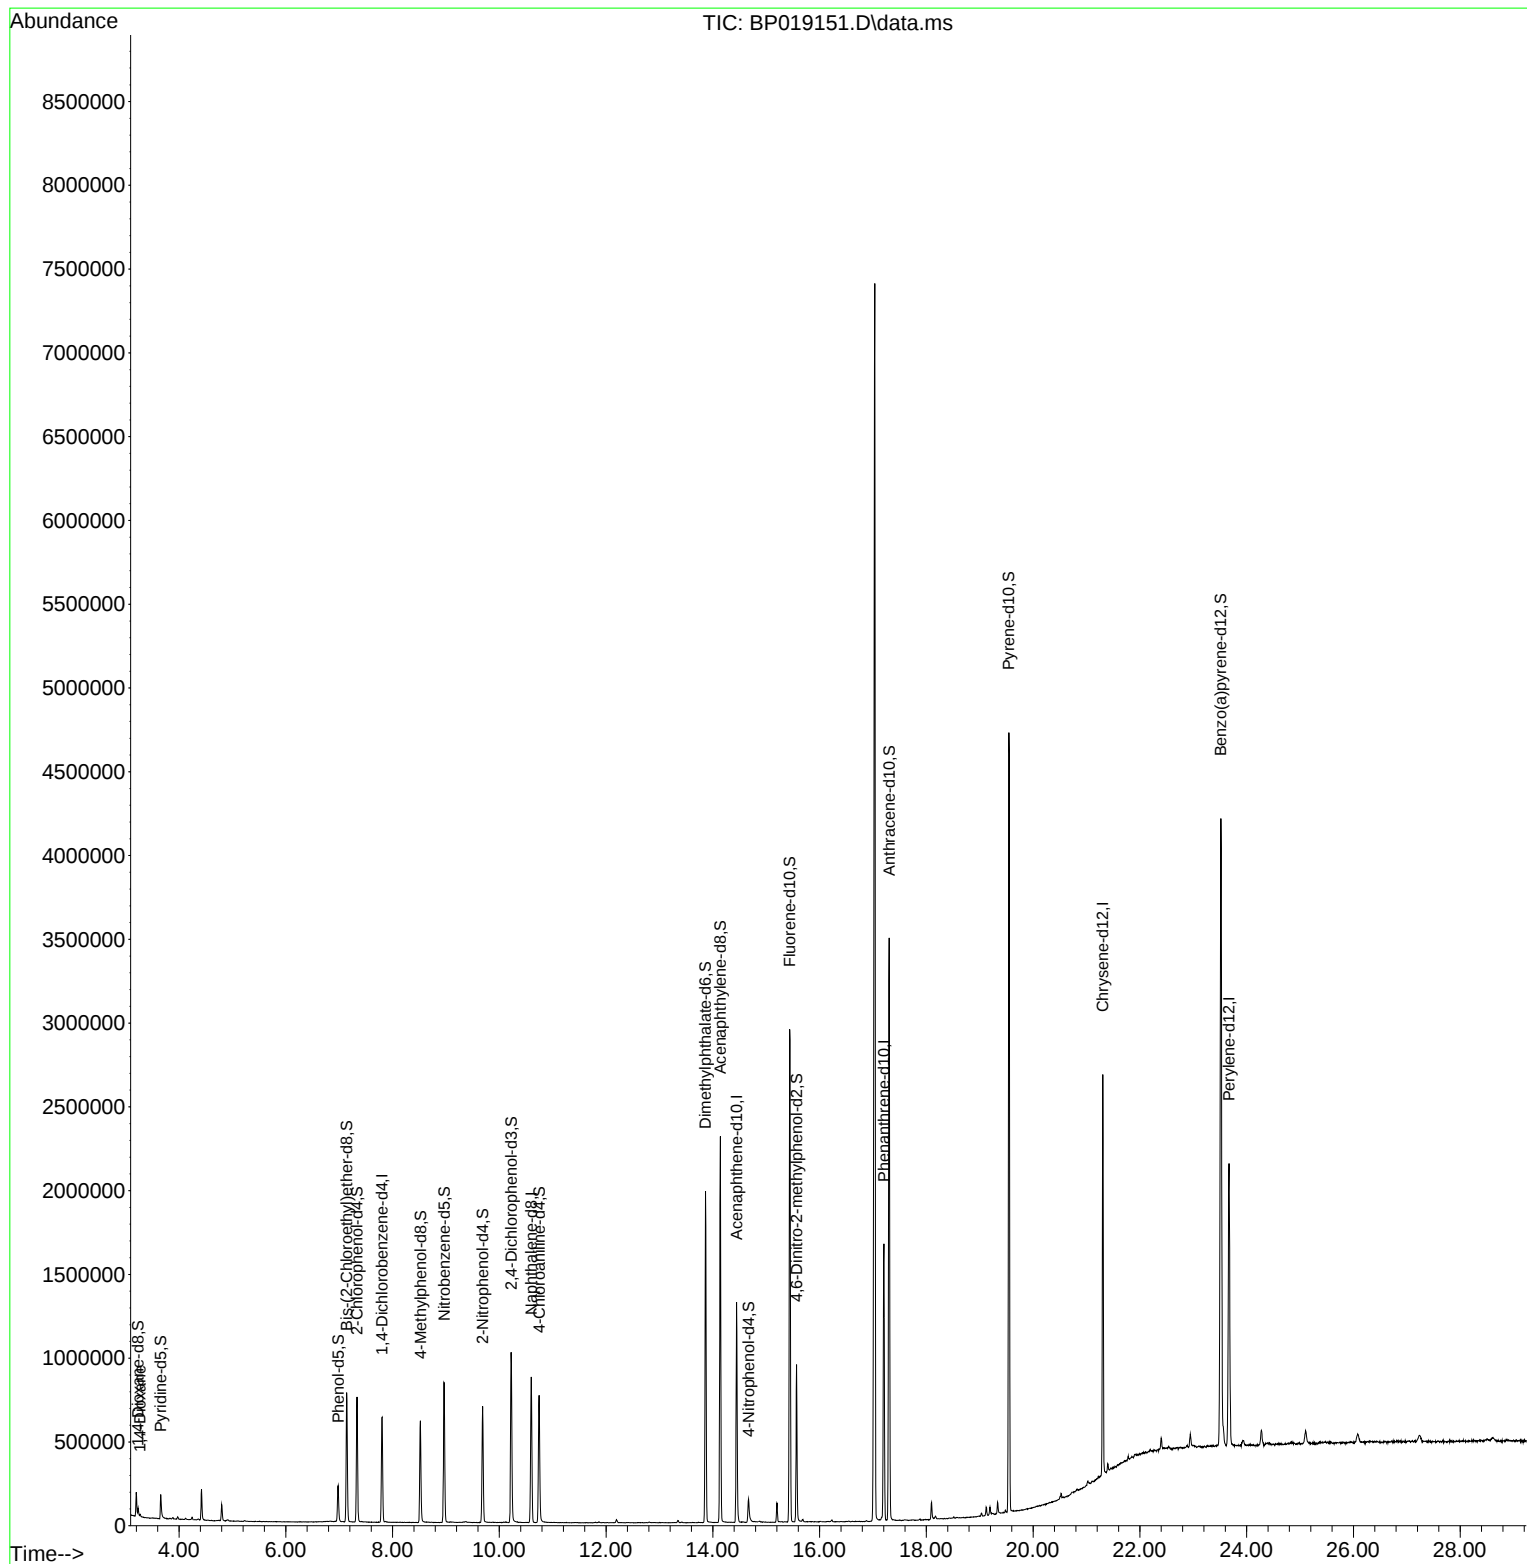

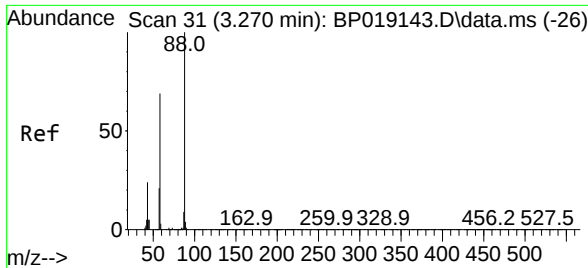

#2
 1,4-Dioxane
 Concen: 1.256 ng/uL
 RT: 3.270 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BP019151.D
 Acq: 29 Dec 2023 06:43

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z3

Tgt Ion:	88	Resp:	7288
Ion	Ratio	Lower	Upper
88	100		
43	24.6	21.0	31.4
58	59.8	56.6	84.8

