

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019152.D
 Acq On : 29 Dec 2023 07:17
 Operator : MA/JU
 Sample : 06021-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z4

Quant Time: Dec 29 07:45:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	201480	20.000	ng/u1	0.00
20) Naphthalene-d8	10.599	136	765235	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	448718	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	916179	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1022800	20.000	ng/u1	0.00
88) Perylene-d12	23.668	264	1226995	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	26147	4.432	ng/uL	0.00
4) Pyridine-d5	3.652	84	187343	12.652	ng/u1	0.00
7) Phenol-d5	6.981	99	156196	8.645	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	387741	37.095	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	404472	27.768	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	268843	19.112	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	240444	36.348	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	258639	36.178	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	466847	32.338	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	587453	33.083	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1458474	36.798	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1591328	37.003	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	43084	6.437	ng/u1	0.00
60) Fluorene-d10	15.445	176	1259991	36.798	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	195341	32.523	ng/u1	0.00
73) Anthracene-d10	17.310	188	1891901	39.542	ng/u1	0.00
81) Pyrene-d10	19.545	212	2411754	38.691	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	2736234	38.797	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.270	88	7656	1.180	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019152.D
Acq On : 29 Dec 2023 07:17
Operator : MA/JU
Sample : 06021-12
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z4

Quant Time: Dec 29 07:45:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

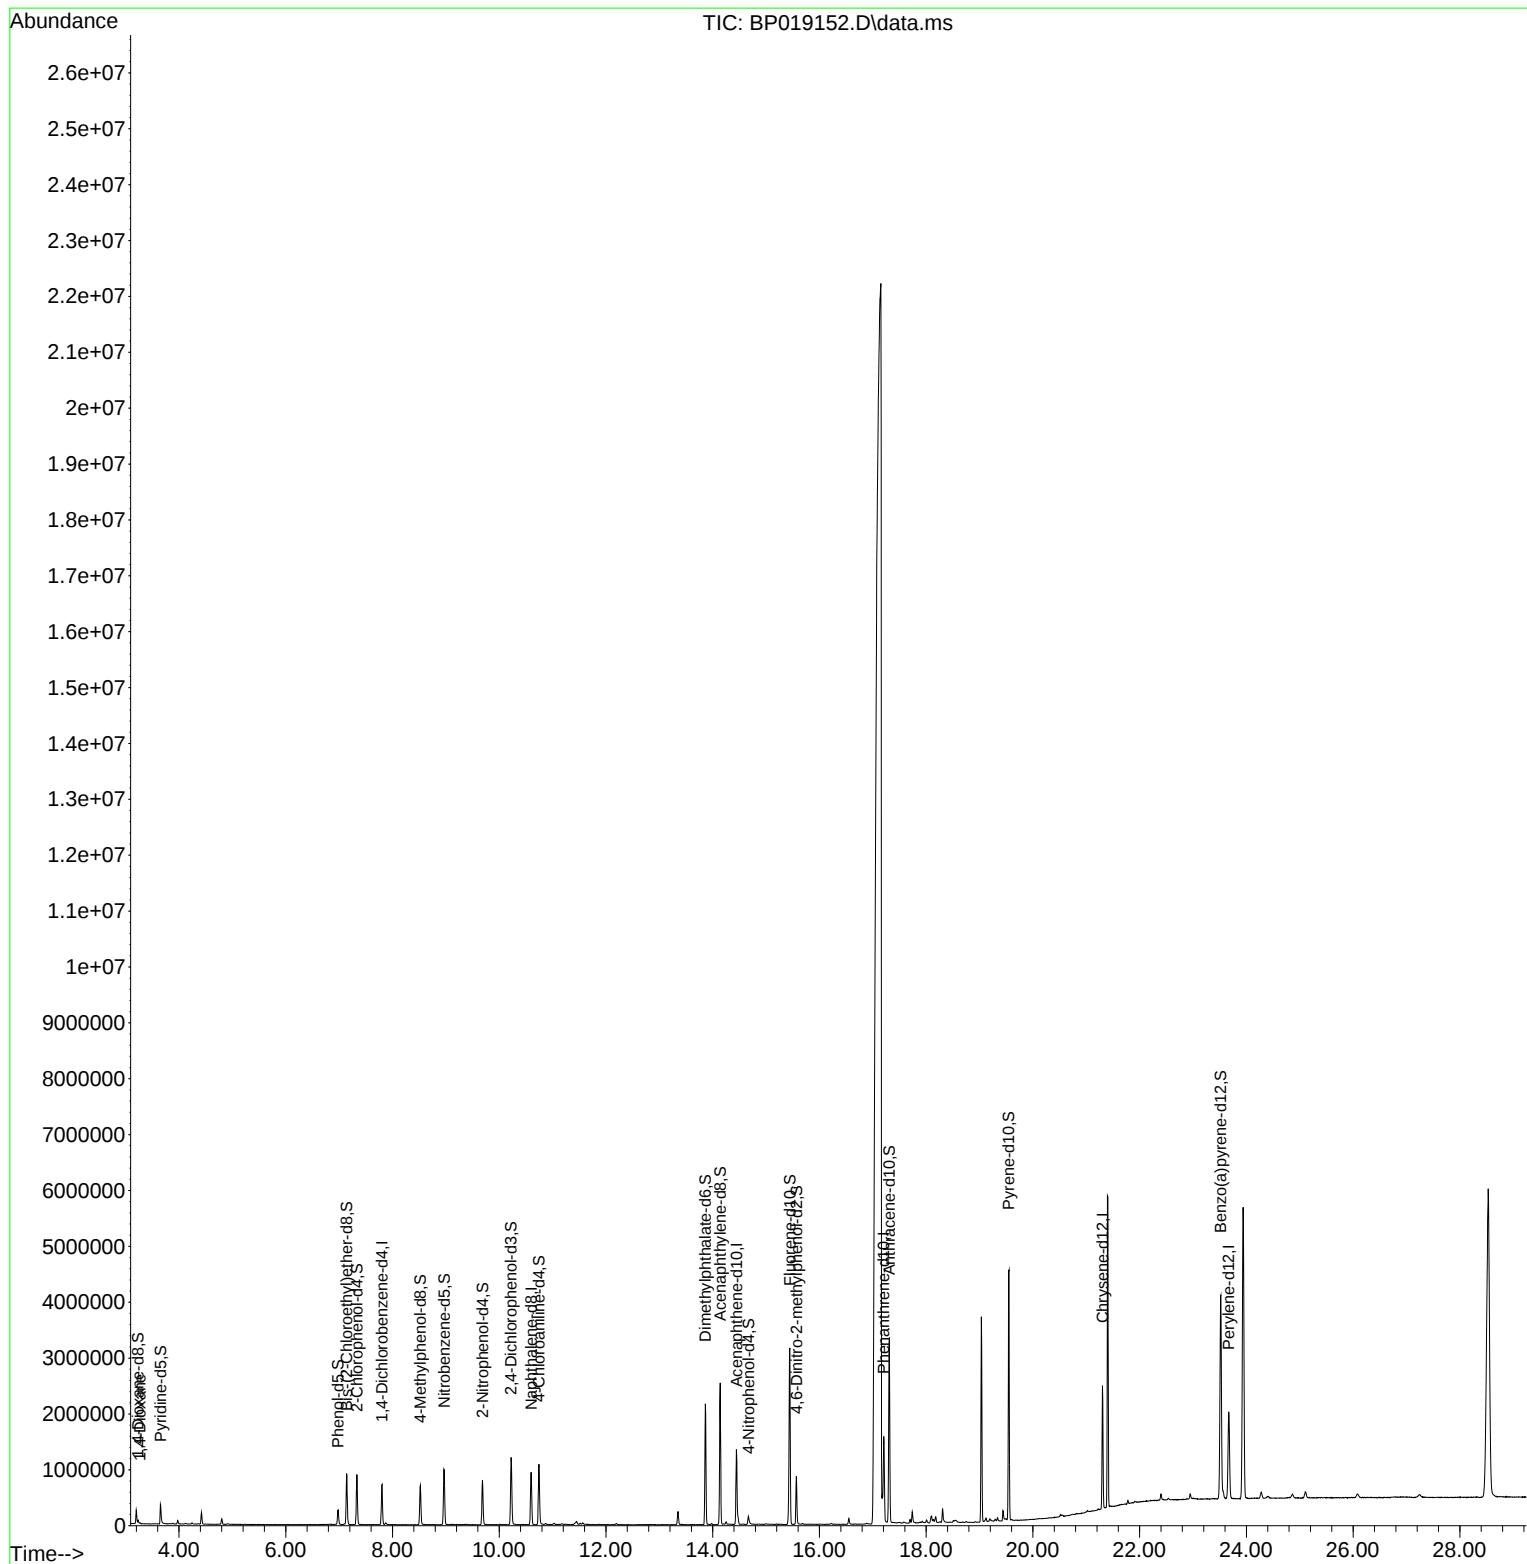

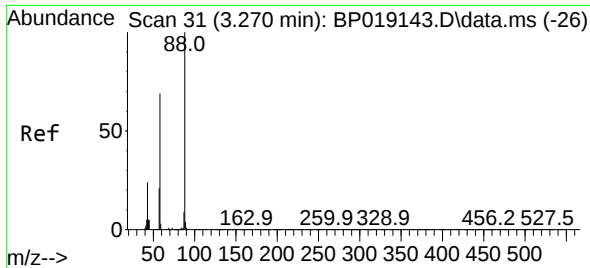

#2
 1,4-Dioxane
 Concen: 1.180 ng/uL
 RT: 3.270 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BP019152.D
 Acq: 29 Dec 2023 07:17

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z4

Tgt Ion:	88	Resp:	7656
Ion	Ratio	Lower	Upper
88	100		
43	26.0	21.0	31.4
58	64.7	56.6	84.8

