

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019193.D
 Acq On : 30 Dec 2023 07:11
 Operator : MA/JU
 Sample : 06020-15
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Y1

Quant Time: Jan 01 00:20:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	197826	20.000	ng/ul	0.00
20) Naphthalene-d8	10.593	136	730178	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	446597	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	1040558	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1151824	20.000	ng/ul	0.00
88) Perylene-d12	23.668	264	1359749	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	25243	4.358	ng/uL	0.00
4) Pyridine-d5	3.658	84	102724	7.066	ng/ul	0.00
7) Phenol-d5	6.975	99	125352	7.066	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	325368	31.702	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	335366	23.449	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	218203	15.798	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	195437	30.963	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	198716	29.130	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	379437	27.545	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.740	131	428699	25.302	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	1318059	33.413	ng/ul	0.00
49) Acenaphthylene-d8	14.134	160	1397165	32.642	ng/ul	0.00
54) 4-Nitrophenol-d4	14.663	143	39179	5.882	ng/ul	0.00
60) Fluorene-d10	15.439	176	1182791	34.708	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	196535	28.811	ng/ul	-0.01
73) Anthracene-d10	17.298	188	2059007	37.890	ng/ul	0.00
81) Pyrene-d10	19.539	212	2645139	37.682	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	3004402	38.440	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.898	107	22486	1.702	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019193.D
Acq On : 30 Dec 2023 07:11
Operator : MA/JU
Sample : 06020-15
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Y1

Quant Time: Jan 01 00:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

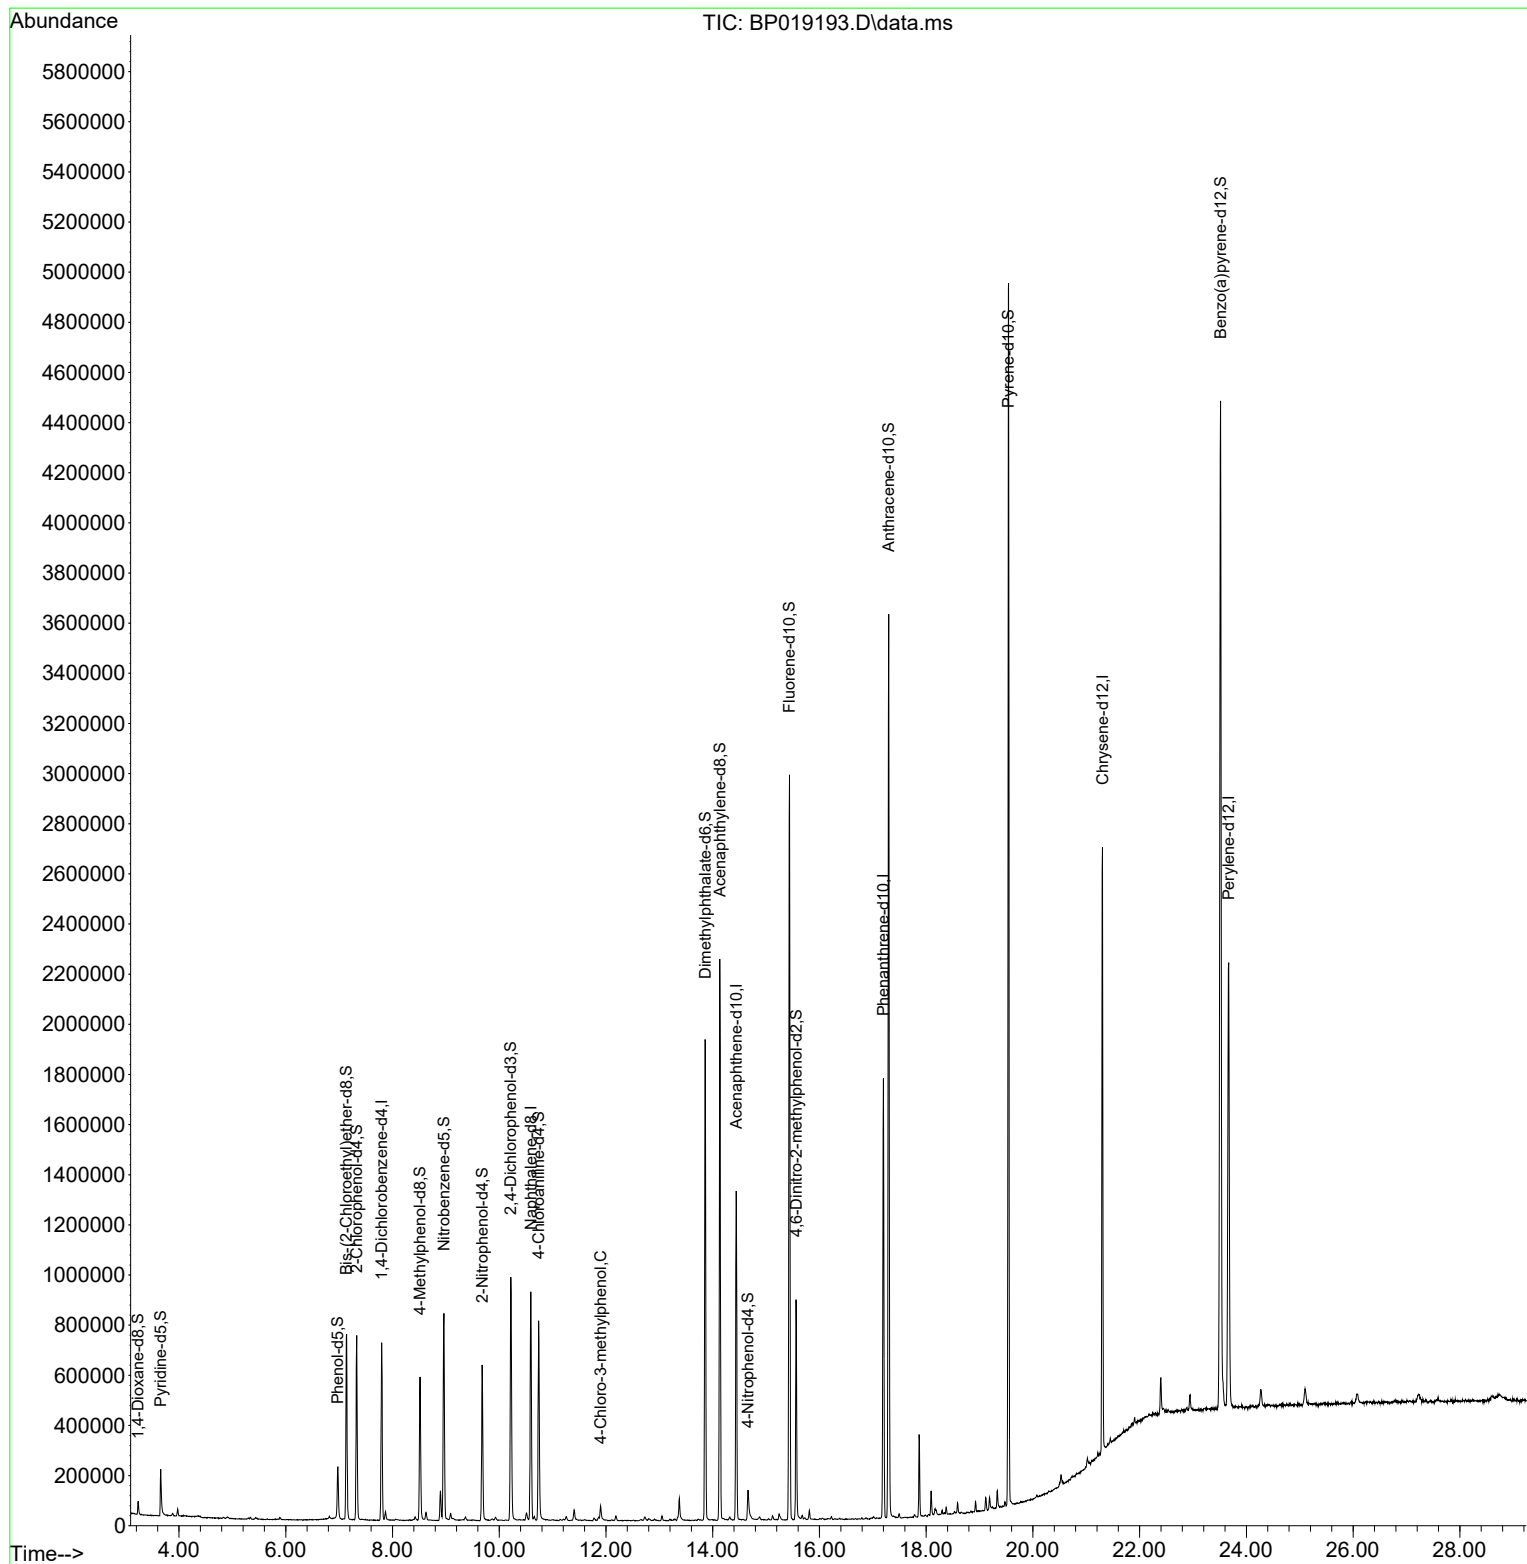

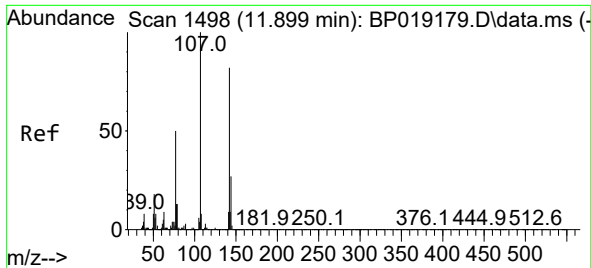

#35
 4-Chloro-3-methylphenol
 Concen: 1.702 ng/ul
 RT: 11.898 min Scan# 1498
 Delta R.T. -0.000 min
 Lab File: BP019193.D
 Acq: 30 Dec 2023 07:11

Instrument :
 BNA_P
 ClientSampleId :
 BH7Y1

Tgt Ion:107 Resp: 22486
 Ion Ratio Lower Upper
 107 100
 144 23.9 21.0 31.6
 142 85.2 64.8 97.2

