

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019125.D
 Acq On : 28 Dec 2023 11:26
 Operator : MA/JU
 Sample : PB158024BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	31	rBV	52086	62268	1.35%	0.160%
2	3.652	92	96	110	rBV	578847	842346	18.31%	2.163%
3	3.981	148	152	155	rVB2	10863	14345	0.31%	0.037%
4	4.446	227	231	235	rBV4	5233	10392	0.23%	0.027%
5	6.981	654	662	674	rVV	617331	981651	21.34%	2.521%
6	7.146	681	690	700	rBV	532824	815914	17.74%	2.095%
7	7.340	716	723	731	rBV	624430	989099	21.50%	2.540%
8	7.804	795	802	810	rBV	539038	849613	18.47%	2.182%
9	8.522	918	924	933	rBV	718690	1186217	25.79%	3.046%
10	8.969	993	1000	1013	rBV	568564	935384	20.33%	2.402%
11	9.381	1065	1070	1072	rBV5	3186	5825	0.13%	0.015%
12	9.692	1115	1123	1133	rBV	449070	729201	15.85%	1.872%
13	10.228	1207	1214	1227	rBV	719053	1212909	26.37%	3.115%
14	10.604	1270	1278	1291	rVB	678278	1131625	24.60%	2.906%
15	10.751	1295	1303	1321	rBV	697450	1218728	26.49%	3.129%
16	11.804	1476	1482	1486	rBV9	3550	8597	0.19%	0.022%
17	12.204	1544	1550	1559	rBV4	11449	24485	0.53%	0.063%
18	12.822	1650	1655	1660	rBV8	4083	7730	0.17%	0.020%
19	13.357	1740	1746	1750	rBV4	8980	15169	0.33%	0.039%
20	13.428	1753	1758	1765	rVB9	2649	5788	0.13%	0.015%
21	13.733	1806	1810	1815	rBV7	3472	5748	0.12%	0.015%
22	13.869	1827	1833	1844	rBV	1303653	1776206	38.61%	4.561%
23	14.145	1873	1880	1888	rBV	1434748	2087357	45.37%	5.360%
24	14.451	1925	1932	1941	rBV	1034531	1508879	32.80%	3.875%
25	14.669	1962	1969	1984	rBV	446149	771067	16.76%	1.980%
26	14.880	2003	2005	2016	rVB	4542	8911	0.19%	0.023%
27	15.251	2065	2068	2072	rVB6	4218	4990	0.11%	0.013%
28	15.451	2093	2102	2110	rBV	1876840	2736112	59.48%	7.026%
29	15.575	2117	2123	2133	rBV	491997	679282	14.77%	1.744%
30	15.692	2139	2143	2147	rVB6	9011	13203	0.29%	0.034%
31	16.239	2232	2236	2242	rVB5	7893	12285	0.27%	0.032%
32	16.510	2278	2282	2288	rBV9	4677	7221	0.16%	0.019%
33	16.892	2341	2347	2349	rVB7	5141	7658	0.17%	0.020%
34	16.998	2362	2365	2369	rBV6	3342	5398	0.12%	0.014%
35	17.210	2394	2401	2407	rBV	1332919	1851788	40.25%	4.755%
36	17.310	2411	2418	2430	rBV	2160819	2971835	64.60%	7.631%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019125.D
Acq On : 28 Dec 2023 11:26
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	18.104	2548	2553	2561	rBV7	20115	40237	0.87%	0.103%
38	19.127	2724	2727	2731	rVB2	27545	34481	0.75%	0.089%
39	19.198	2736	2739	2745	rVV	23358	33128	0.72%	0.085%
40	19.345	2760	2764	2767	rBV5	24216	36802	0.80%	0.095%
41	19.551	2794	2799	2807	rBV	2846904	3743510	81.37%	9.613%
42	20.533	2963	2966	2971	rVB	73681	80503	1.75%	0.207%
43	21.315	3094	3099	3106	rBV	1747920	2299523	49.99%	5.905%
44	23.527	3468	3475	3492	rVB2	2317085	4600402	100.00%	11.813%
45	23.680	3495	3501	3511	rVB	1292221	2579445	56.07%	6.624%




Sum of corrected areas: 38943257

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019125.D
Acq On : 28 Dec 2023 11:26
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

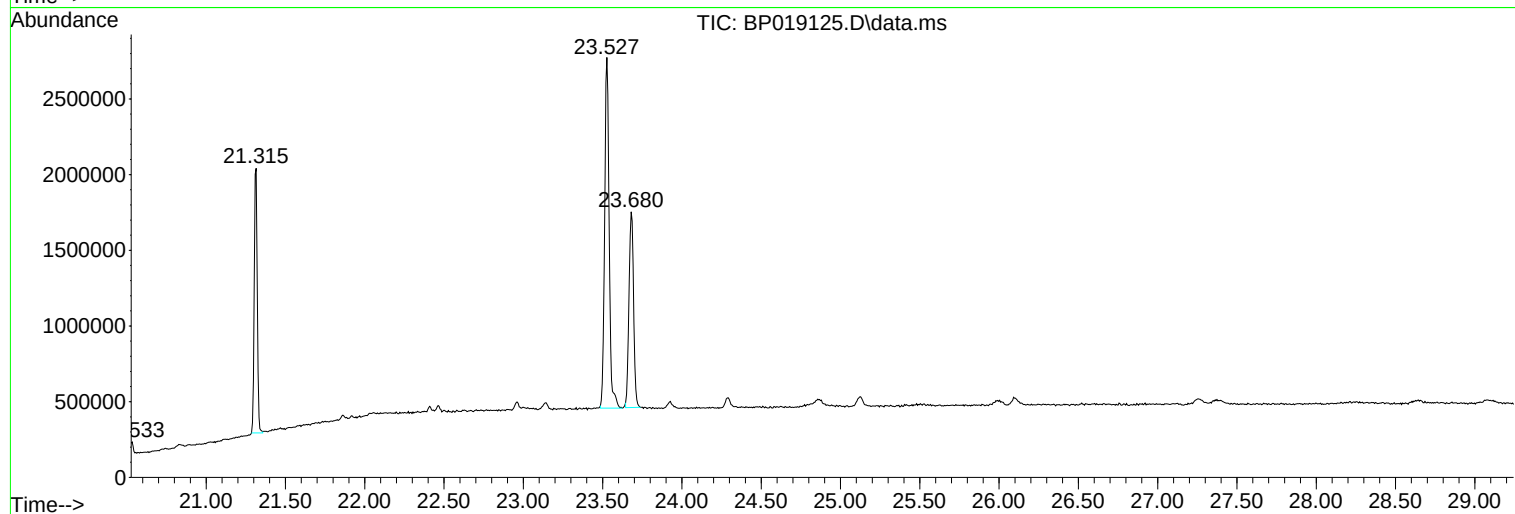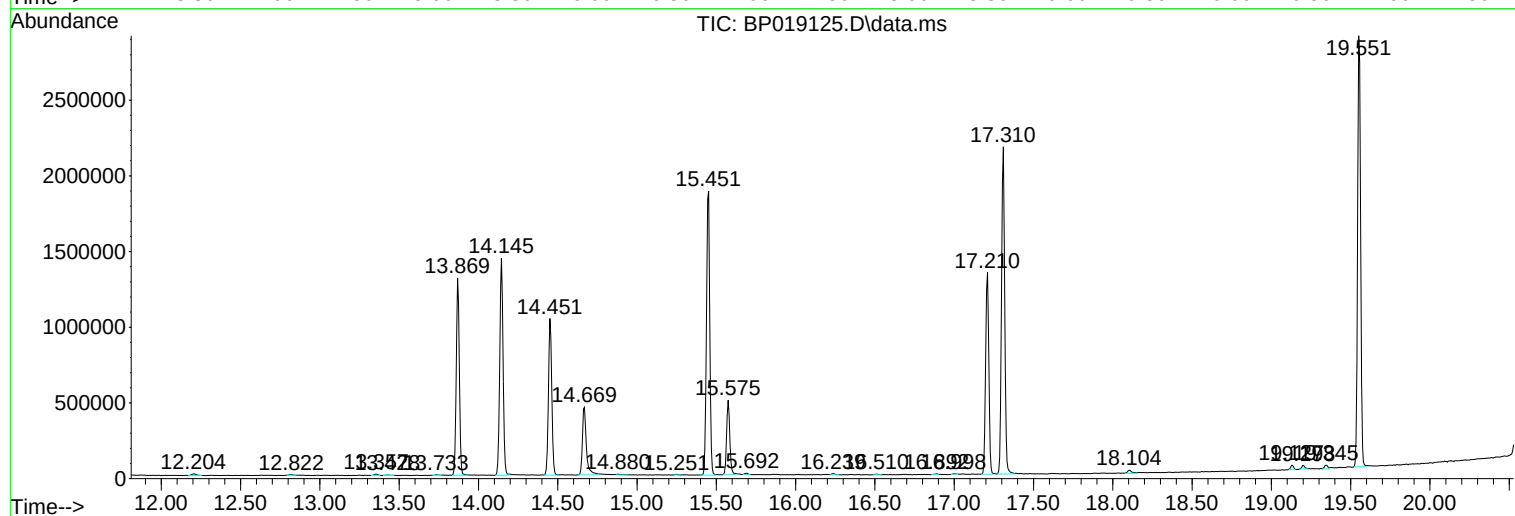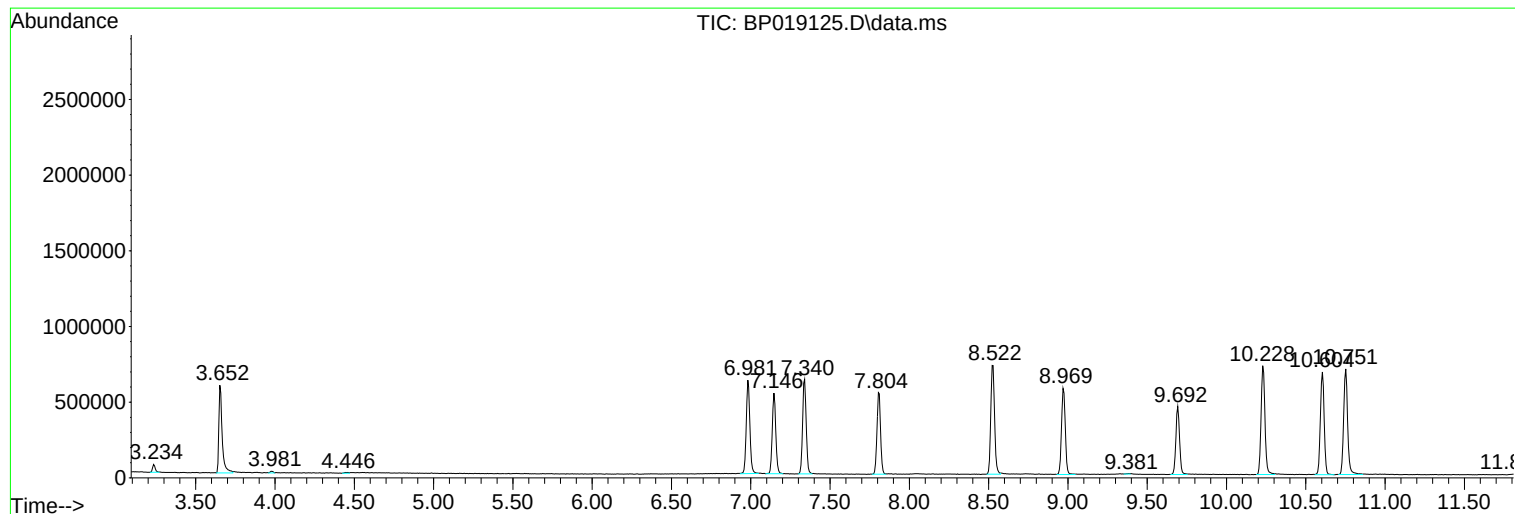

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019125.D
Acq On : 28 Dec 2023 11:26
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019125.D
Acq On : 28 Dec 2023 11:26
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------