

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019129.D
 Acq On : 28 Dec 2023 17:40
 Operator : MA/JU
 Sample : PB158118BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	30	rBV	51323	62780	1.43%	0.166%
2	3.652	92	96	113	rBV	574263	820948	18.74%	2.172%
3	3.975	147	151	156	rBV	11398	17322	0.40%	0.046%
4	6.981	655	662	673	rVB	600412	933449	21.31%	2.470%
5	7.146	683	690	699	rVB	512630	779969	17.80%	2.063%
6	7.334	716	722	732	rBV	616344	951670	21.72%	2.518%
7	7.805	795	802	810	rBV	537594	842091	19.22%	2.228%
8	8.522	917	924	937	rBV	714527	1142961	26.09%	3.024%
9	8.969	993	1000	1010	rBV	549457	878398	20.05%	2.324%
10	9.328	1055	1061	1064	rBV8	2394	4384	0.10%	0.012%
11	9.687	1114	1122	1134	rBV	415838	694979	15.86%	1.839%
12	10.228	1206	1214	1232	rBV	686073	1170891	26.73%	3.098%
13	10.599	1270	1277	1286	rVB	667101	1115999	25.47%	2.952%
14	10.746	1295	1302	1318	rBV	655225	1142558	26.08%	3.023%
15	12.204	1544	1550	1562	rBV4	9971	25361	0.58%	0.067%
16	12.816	1647	1654	1655	rBV7	2943	5171	0.12%	0.014%
17	13.351	1741	1745	1750	rBV3	10435	15578	0.36%	0.041%
18	13.416	1754	1756	1760	rBV5	2867	4515	0.10%	0.012%
19	13.869	1825	1833	1846	rBV	1237227	1706414	38.95%	4.514%
20	14.140	1872	1879	1896	rBV	1332906	1980961	45.21%	5.241%
21	14.451	1925	1932	1941	rBV	1025388	1486274	33.92%	3.932%
22	14.663	1961	1968	1986	rBV	421409	729866	16.66%	1.931%
23	15.245	2060	2067	2072	rBV8	3840	7247	0.17%	0.019%
24	15.445	2094	2101	2108	rBV	1885445	2598847	59.32%	6.876%
25	15.575	2116	2123	2133	rBV	456487	669923	15.29%	1.772%
26	15.687	2139	2142	2147	rVB4	7224	9958	0.23%	0.026%
27	16.239	2231	2236	2237	rBV5	8160	11599	0.26%	0.031%
28	16.516	2277	2283	2286	rBV8	2655	5774	0.13%	0.015%
29	16.886	2340	2346	2348	rBV7	4354	7820	0.18%	0.021%
30	16.998	2361	2365	2368	rBV5	4027	6569	0.15%	0.017%
31	17.204	2394	2400	2410	rBV	1323209	1868508	42.65%	4.943%
32	17.304	2411	2417	2430	rBV2	2046184	2874567	65.61%	7.605%
33	18.110	2551	2554	2559	rBV7	5120	6412	0.15%	0.017%
34	19.128	2724	2727	2733	rVB3	28419	36388	0.83%	0.096%
35	19.198	2735	2739	2746	rBV2	24372	40175	0.92%	0.106%
36	19.551	2793	2799	2812	rBV	2914711	3668762	83.74%	9.706%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019129.D
Acq On : 28 Dec 2023 17:40
Operator : MA/JU
Sample : PB158118BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	21.310	3093	3098	3106	rBV	1929333	2389956	54.55%	6.323%
38	23.521	3468	3474	3491	rVB	2206852	4381214	100.00%	11.591%
39	23.674	3494	3500	3514	rVB	1313558	2702307	61.68%	7.149%




Sum of corrected areas: 37798565

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019129.D
Acq On : 28 Dec 2023 17:40
Operator : MA/JU
Sample : PB158118BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

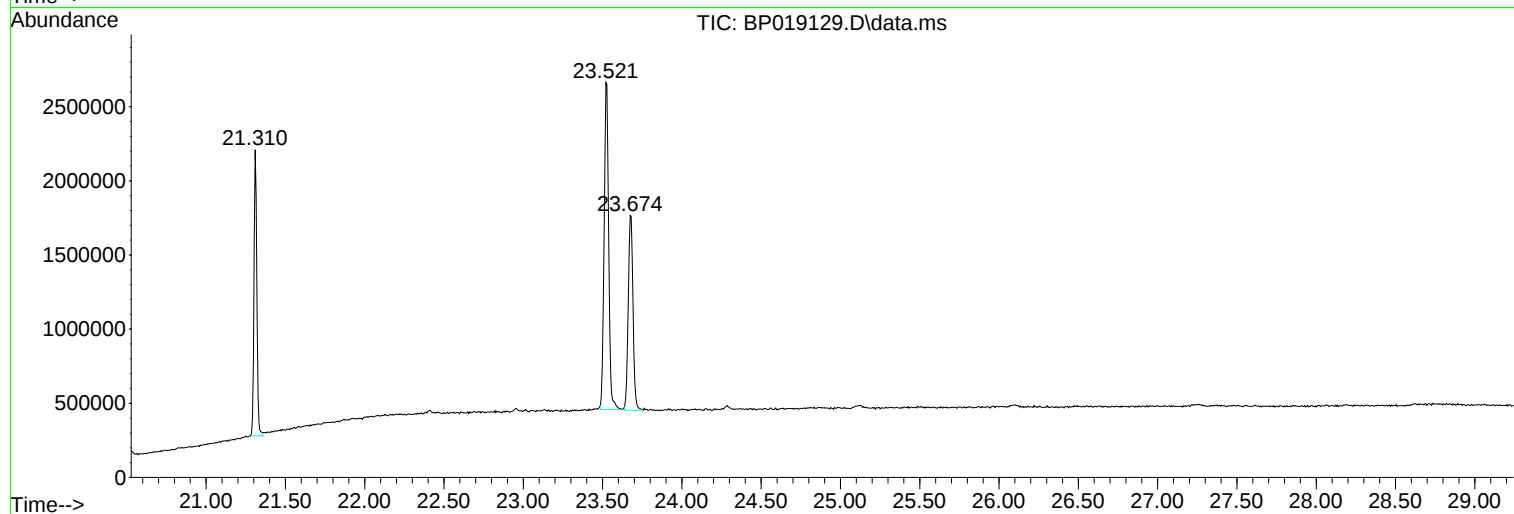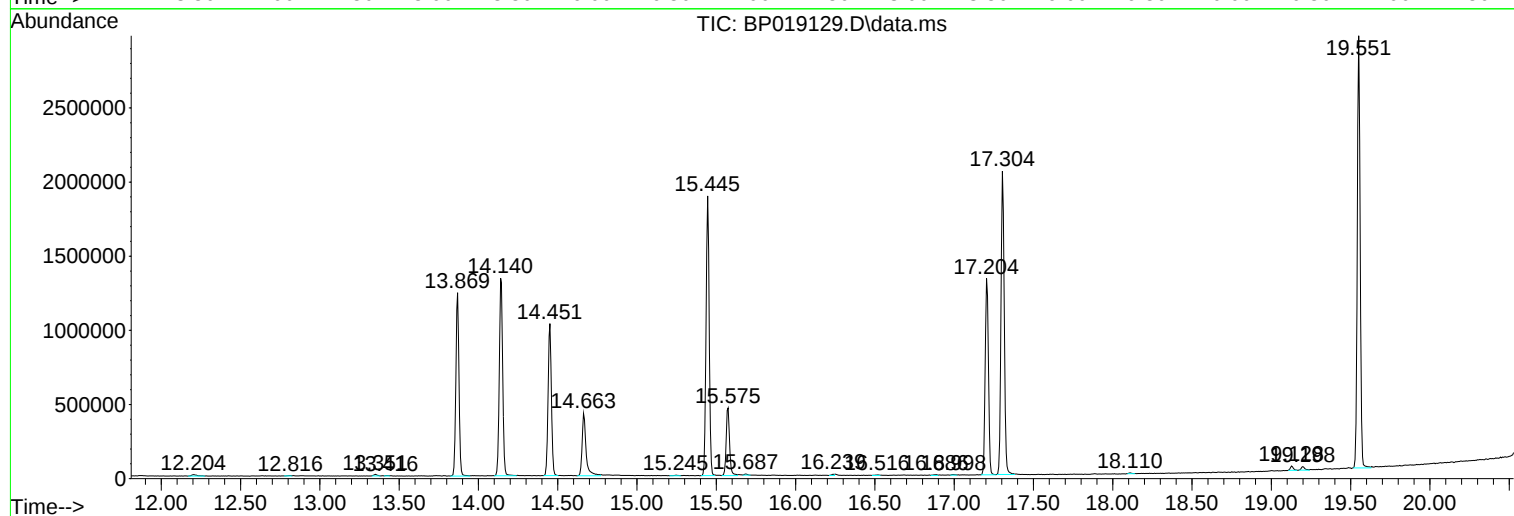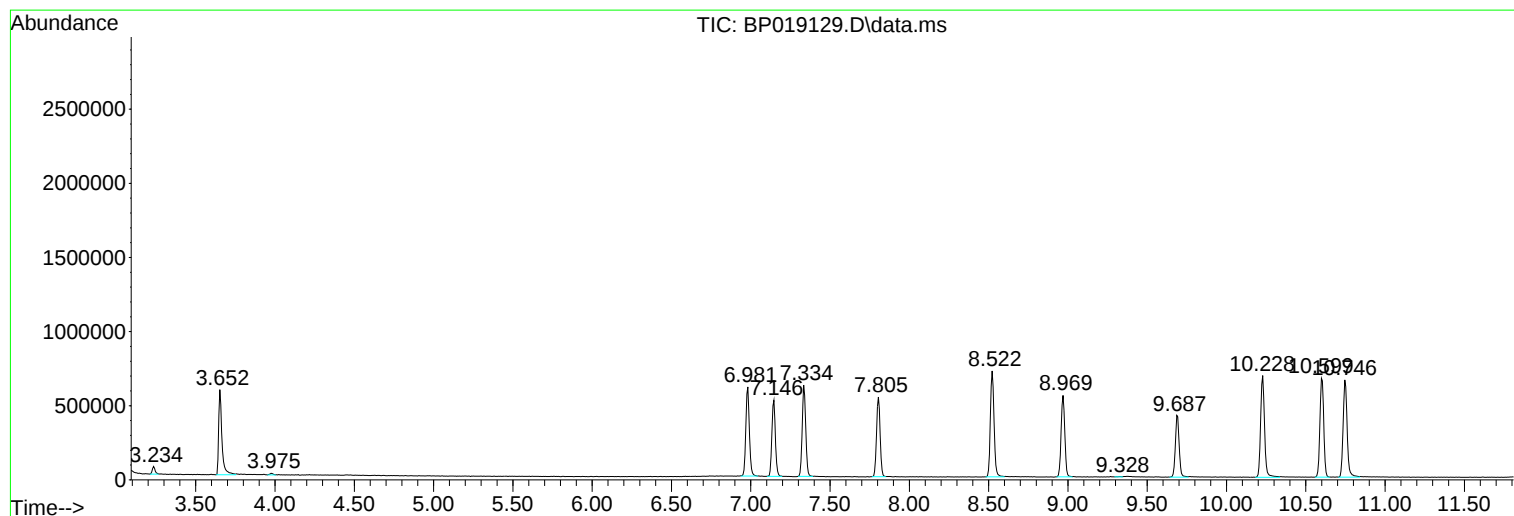

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019129.D
Acq On : 28 Dec 2023 17:40
Operator : MA/JU
Sample : PB158118BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019129.D
Acq On : 28 Dec 2023 17:40
Operator : MA/JU
Sample : PB158118BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------