

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019136.D
 Acq On : 28 Dec 2023 21:39
 Operator : MA/JU
 Sample : 05986-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	30	rVB	37727	42843	0.50%	0.077%
2	3.658	93	97	115	rBV	163547	243241	2.85%	0.438%
3	3.975	148	151	156	rVB	10248	14009	0.16%	0.025%
4	6.981	657	662	671	rVB	147056	232073	2.72%	0.418%
5	7.146	683	690	702	rVB	608085	937999	11.00%	1.689%
6	7.334	715	722	731	rBV	563581	887348	10.40%	1.598%
7	7.805	795	802	810	rVB	658145	1014301	11.89%	1.826%
8	8.522	917	924	933	rBV	419534	672848	7.89%	1.211%
9	8.969	993	1000	1011	rBV	678868	1094282	12.83%	1.970%
10	9.375	1063	1069	1077	rVB8	7797	14381	0.17%	0.026%
11	9.687	1114	1122	1131	rBV	528564	873124	10.24%	1.572%
12	10.228	1205	1214	1230	rBV	822465	1370264	16.06%	2.467%
13	10.599	1270	1277	1286	rVB	811551	1364829	16.00%	2.457%
14	10.746	1295	1302	1322	rBV	583103	1029975	12.07%	1.854%
15	11.869	1487	1493	1501	rVB10	5791	11977	0.14%	0.022%
16	12.193	1543	1548	1554	rVV2	14873	25016	0.29%	0.045%
17	12.728	1634	1639	1645	rVB9	5144	10162	0.12%	0.018%
18	12.810	1645	1653	1656	rBV10	5223	11105	0.13%	0.020%
19	13.193	1713	1718	1721	rBV7	5144	8886	0.10%	0.016%
20	13.351	1739	1745	1752	rBV2	23602	40439	0.47%	0.073%
21	13.869	1825	1833	1844	rBV	1693018	2308081	27.06%	4.156%
22	14.140	1872	1879	1889	rBV	1803601	2635170	30.89%	4.744%
23	14.451	1922	1932	1940	rBV	1231018	1872082	21.95%	3.371%
24	14.669	1964	1969	1987	rBV	101255	200721	2.35%	0.361%
25	15.445	2094	2101	2113	rVB	2490683	3560423	41.74%	6.410%
26	15.569	2116	2122	2135	rVV	774628	1104227	12.94%	1.988%
27	15.687	2138	2142	2147	rVB4	12733	19264	0.23%	0.035%
28	15.816	2159	2164	2169	rBV	73558	97410	1.14%	0.175%
29	16.181	2221	2226	2232	rBV	26343	42200	0.49%	0.076%
30	16.234	2232	2235	2239	rVB5	10602	12301	0.14%	0.022%
31	16.292	2241	2245	2251	rBV2	17062	29346	0.34%	0.053%
32	16.863	2338	2342	2345	rBV6	8401	14711	0.17%	0.026%
33	17.016	2365	2368	2370	rBV3	8673	10260	0.12%	0.018%
34	17.086	2376	2380	2383	rVB5	9595	13412	0.16%	0.024%
35	17.204	2394	2400	2409	rBV	1612520	2326169	27.27%	4.188%
36	17.304	2411	2417	2429	rVB2	3013501	4254843	49.88%	7.661%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019136.D
Acq On : 28 Dec 2023 21:39
Operator : MA/JU
Sample : 05986-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	18.098	2548	2552	2560	rBV	139055	202612	2.38%	0.365%
38	18.169	2562	2564	2568	rVB	10056	13353	0.16%	0.024%
39	19.128	2722	2727	2732	rBV3	49752	85742	1.01%	0.154%
40	19.192	2735	2738	2742	rBV	54160	75538	0.89%	0.136%
41	19.339	2759	2763	2769	rBV	89339	119071	1.40%	0.214%
42	19.551	2793	2799	2805	rBV	4377304	5556376	65.14%	10.004%
43	20.916	3012	3031	3046	rVB2	2175449	8530184	100.00%	15.358%
44	21.310	3093	3098	3105	rBV	2280907	2894270	33.93%	5.211%
45	23.521	3467	3474	3489	rVB2	3372984	6479226	75.96%	11.665%
46	23.674	3493	3500	3509	rVB	1635150	3185959	37.35%	5.736%




Sum of corrected areas: 55542053

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019136.D
Acq On : 28 Dec 2023 21:39
Operator : MA/JU
Sample : 05986-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

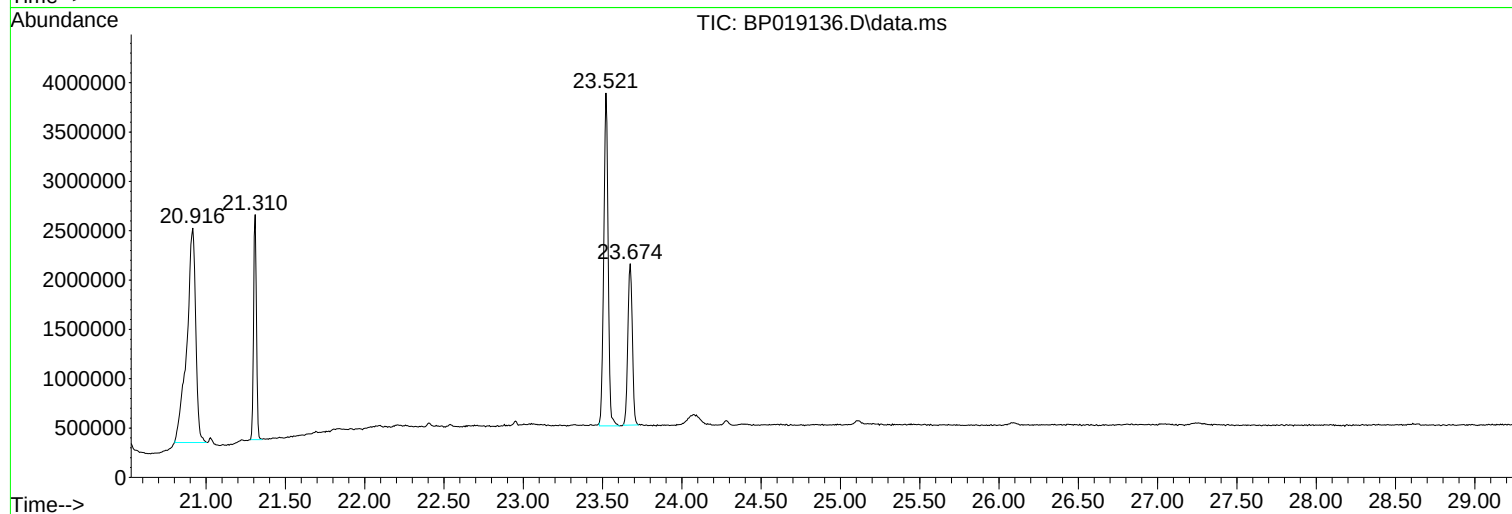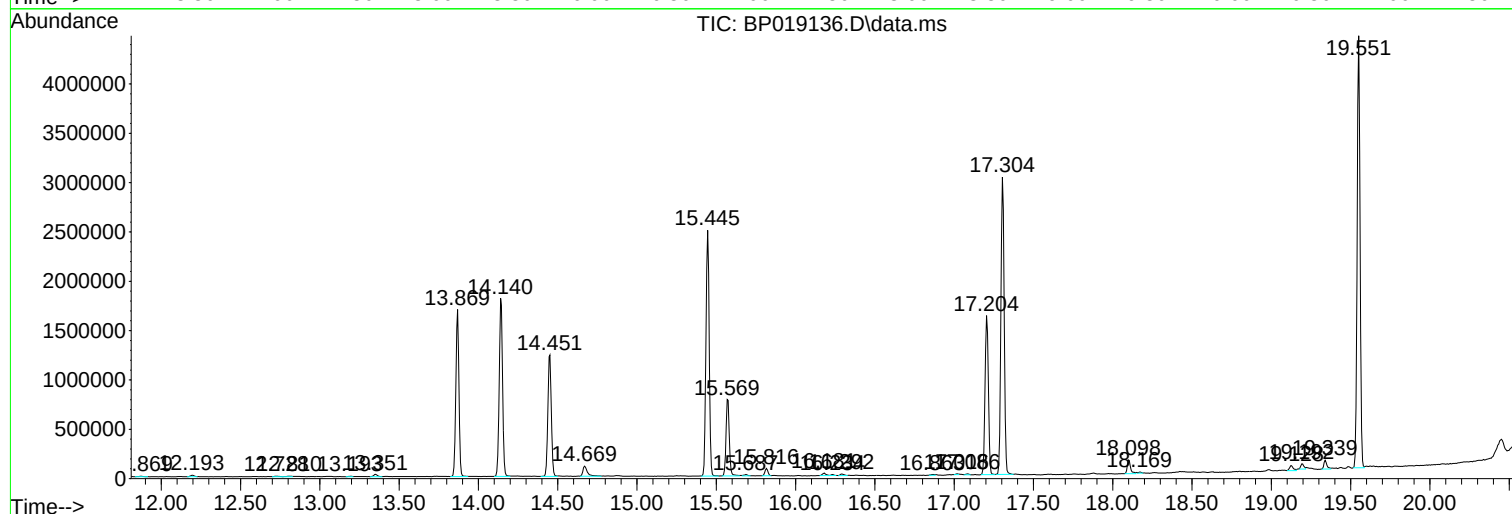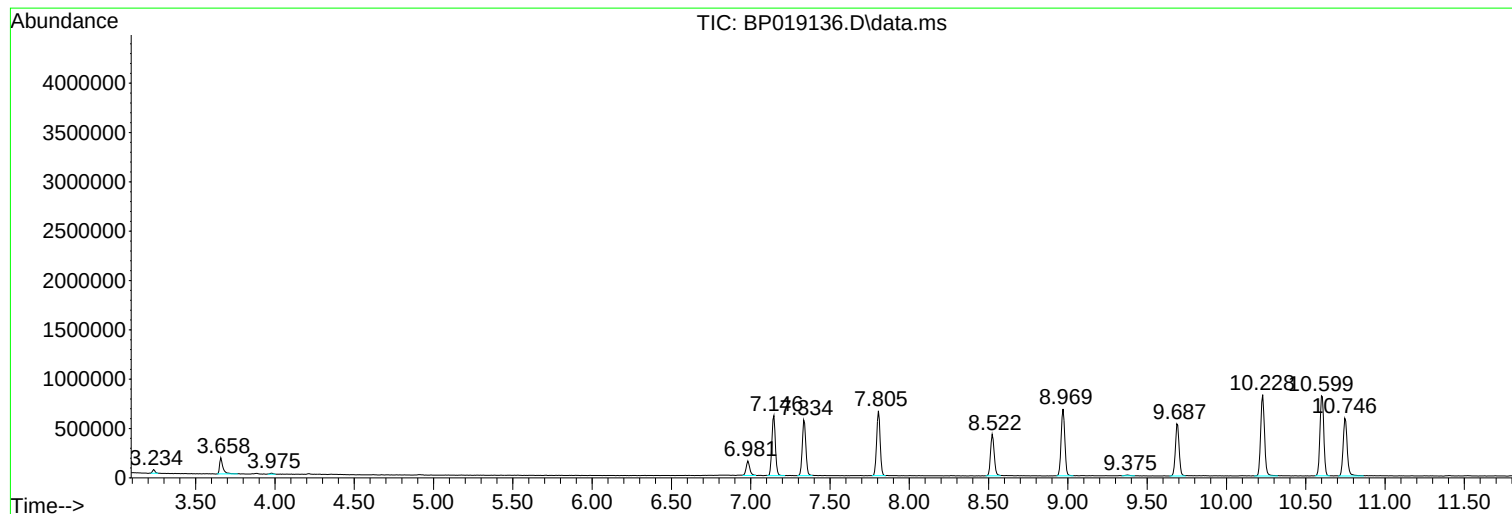

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019136.D
Acq On : 28 Dec 2023 21:39
Operator : MA/JU
Sample : 05986-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 D:A-Friedoursan-3-one Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.916	58.95 ng/ul	8530180	Chrysene-d12	21.310

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Friedelan-3-one	426	C30H50O	000559-74-0	99
2			Friedelan-3-one	426	C30H50O	000559-74-0	95
3			Friedelan-3-one	426	C30H50O	000559-74-0	95
4			D:A-Friedoursan-3-one	426	C30H50O	089950-00-5	70
5			5-Bromo-4-oxo-4,5,6,7-tetrahydro...	216	C6H5BrN2O2	300574-36-1	59

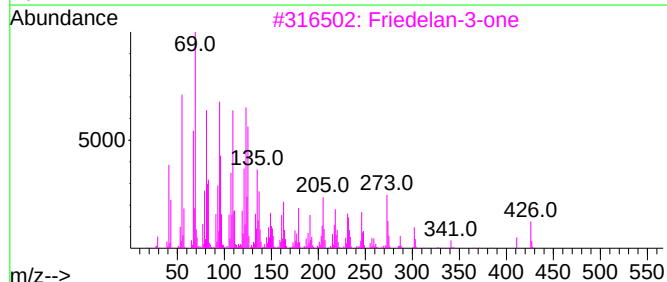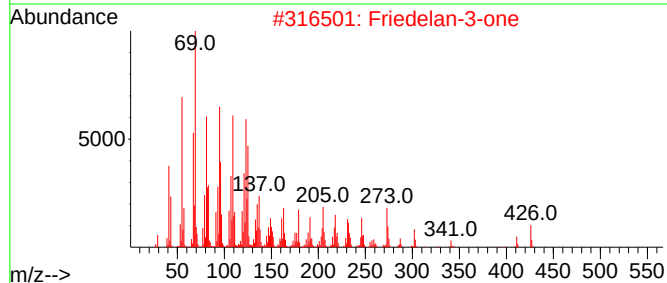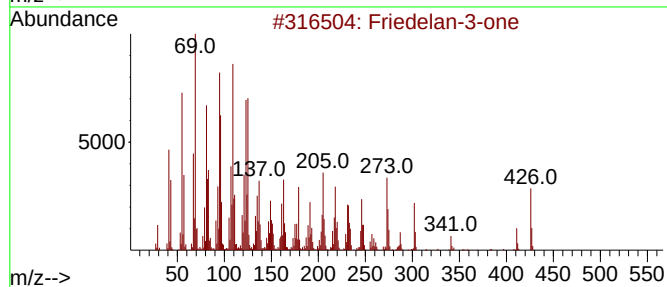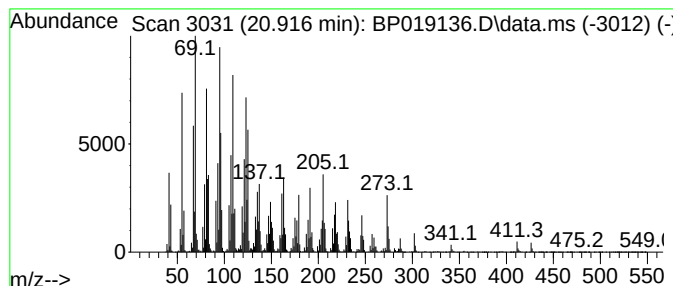

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019136.D
Acq On : 28 Dec 2023 21:39
Operator : MA/JU
Sample : 05986-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
D:A-Friedoursan...	20.916	59.0	ng/ul	8530180	5	21.310	2894270	20.0