

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019137.D
 Acq On : 28 Dec 2023 22:13
 Operator : MA/JU
 Sample : 05986-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	32	rVB	36991	47848	0.63%	0.092%
2	3.658	94	97	113	rBV	110011	175188	2.30%	0.336%
3	3.881	132	135	142	rVB4	6671	12029	0.16%	0.023%
4	3.975	148	151	156	rVB	9477	12743	0.17%	0.024%
5	6.946	651	656	657	rBV3	8580	12321	0.16%	0.024%
6	6.981	657	662	673	rVB	148113	238835	3.14%	0.458%
7	7.146	683	690	703	rVB	621619	967034	12.72%	1.856%
8	7.334	715	722	732	rBV	558294	907112	11.93%	1.741%
9	7.805	795	802	811	rBV	596397	932448	12.26%	1.789%
10	8.522	917	924	936	rBV	424658	688691	9.06%	1.322%
11	8.969	992	1000	1011	rBV	705561	1143653	15.04%	2.195%
12	9.375	1061	1069	1080	rVB3	13396	31248	0.41%	0.060%
13	9.687	1114	1122	1135	rBV	540669	913250	12.01%	1.753%
14	10.228	1205	1214	1224	rBV	839200	1401236	18.43%	2.689%
15	10.599	1269	1277	1287	rBV	763287	1295453	17.04%	2.486%
16	10.746	1294	1302	1318	rBV	673667	1182901	15.56%	2.270%
17	11.804	1476	1482	1486	rBV8	4002	8730	0.11%	0.017%
18	11.875	1489	1494	1499	rVB8	4875	9843	0.13%	0.019%
19	12.198	1542	1549	1556	rBV2	16216	30306	0.40%	0.058%
20	12.810	1648	1653	1656	rBV5	5484	8074	0.11%	0.015%
21	13.351	1741	1745	1751	rVB3	17414	27762	0.37%	0.053%
22	13.869	1826	1833	1844	rBV	1870283	2535010	33.34%	4.865%
23	14.140	1871	1879	1888	rBV	2016445	2910578	38.28%	5.586%
24	14.451	1923	1932	1939	rBV	1273613	1885928	24.80%	3.619%
25	14.557	1948	1950	1957	rVB8	4644	8655	0.11%	0.017%
26	14.669	1963	1969	1987	rBV	118449	235030	3.09%	0.451%
27	14.875	1999	2004	2011	rVB10	7292	17444	0.23%	0.033%
28	15.245	2062	2067	2070	rBV6	5091	8987	0.12%	0.017%
29	15.445	2094	2101	2116	rBV	2838697	4024267	52.92%	7.723%
30	15.575	2116	2123	2138	rBV	946318	1354340	17.81%	2.599%
31	15.686	2138	2142	2145	rVB3	11614	16951	0.22%	0.033%
32	15.816	2159	2164	2169	rBV	69195	94698	1.25%	0.182%
33	16.234	2231	2235	2240	rVB3	11704	18099	0.24%	0.035%
34	16.881	2340	2345	2350	rVB8	6364	11155	0.15%	0.021%
35	17.016	2362	2368	2374	rBV5	11869	20568	0.27%	0.039%
36	17.204	2393	2400	2410	rBV	1729328	2446160	32.17%	4.694%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019137.D
 Acq On : 28 Dec 2023 22:13
 Operator : MA/JU
 Sample : 05986-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	17.304	2411	2417	2429	rVV2	3604501	5115237	67.27%	9.817%
38	17.392	2429	2432	2439	rVB9	10525	20789	0.27%	0.040%
39	17.598	2464	2467	2474	rBV9	3937	8873	0.12%	0.017%
40	18.098	2548	2552	2558	rBV	111920	149500	1.97%	0.287%
41	19.127	2722	2727	2732	rBV2	54549	75410	0.99%	0.145%
42	19.192	2735	2738	2742	rBV	51955	68200	0.90%	0.131%
43	19.339	2759	2763	2768	rBV	68203	91342	1.20%	0.175%
44	19.486	2785	2788	2793	rBV5	16270	22237	0.29%	0.043%
45	19.551	2793	2799	2806	rBV	5066932	6612687	86.96%	12.690%
46	19.780	2835	2838	2843	rVB2	23191	29085	0.38%	0.056%
47	20.527	2962	2965	2969	rVB	116470	120356	1.58%	0.231%
48	21.027	3047	3050	3057	rVB5	74124	123811	1.63%	0.238%
49	21.310	3093	3098	3108	rBV	2500114	3084856	40.57%	5.920%
50	23.521	3467	3474	3487	rVB2	3894035	7604200	100.00%	14.593%
51	23.674	3493	3500	3510	rVB	1652205	3346789	44.01%	6.423%




Sum of corrected areas: 52107947

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019137.D
Acq On : 28 Dec 2023 22:13
Operator : MA/JU
Sample : 05986-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

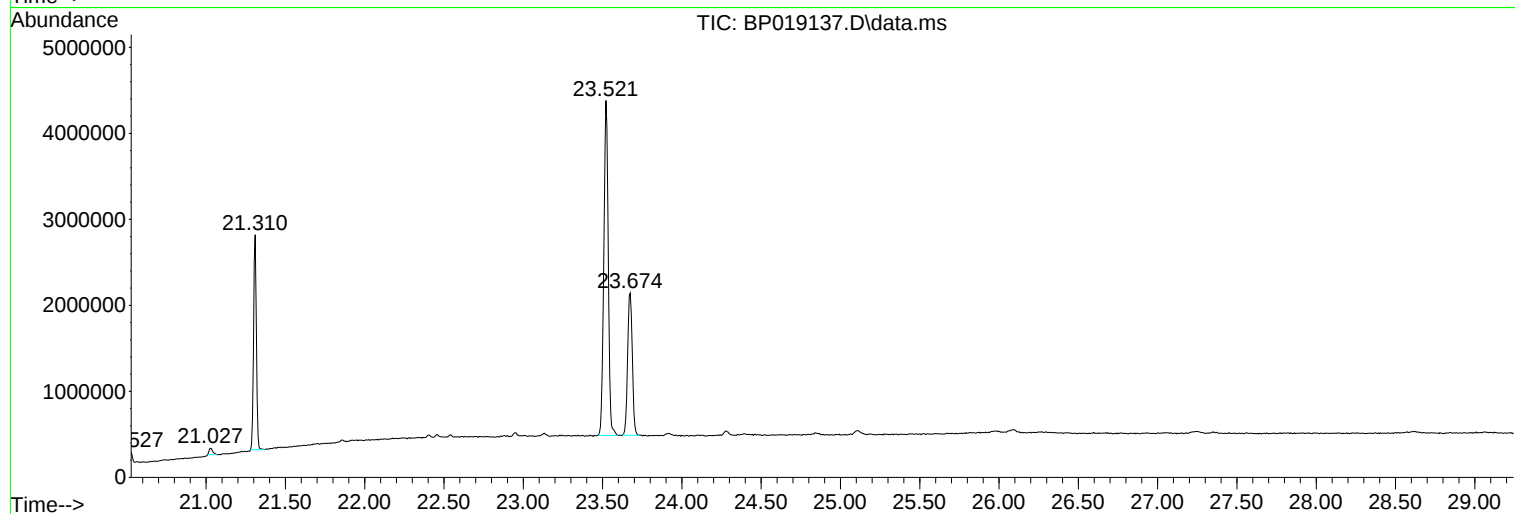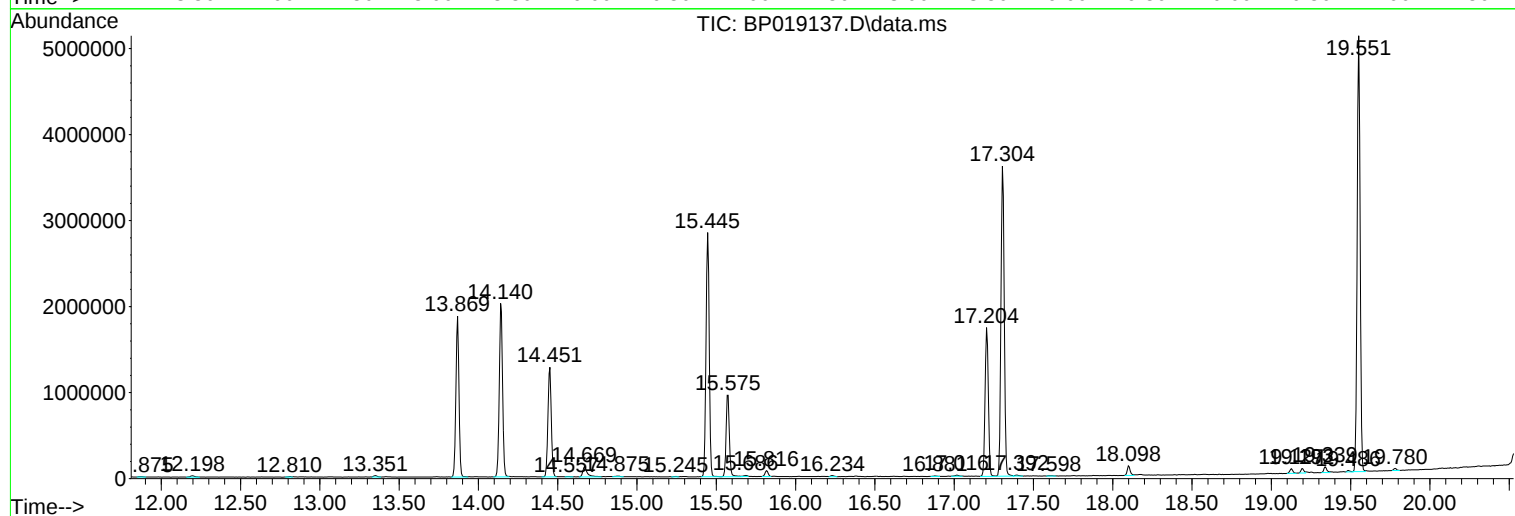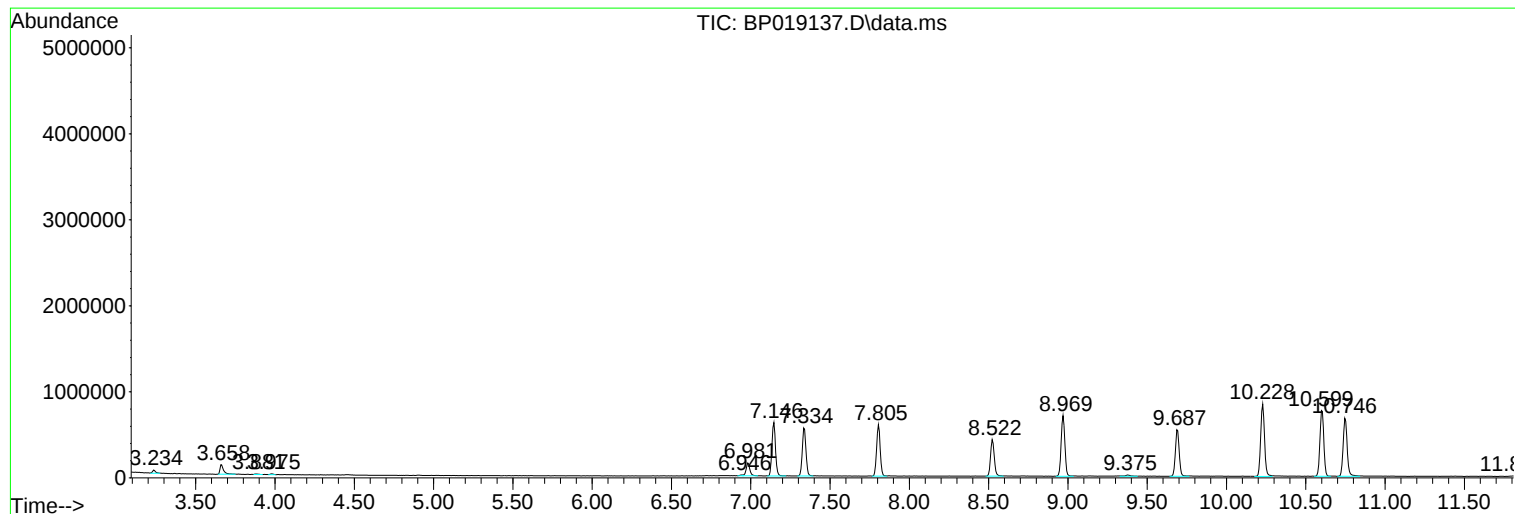

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019137.D
Acq On : 28 Dec 2023 22:13
Operator : MA/JU
Sample : 05986-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019137.D
Acq On : 28 Dec 2023 22:13
Operator : MA/JU
Sample : 05986-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
