

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019138.D
 Acq On : 28 Dec 2023 22:47
 Operator : MA/JU
 Sample : 06021-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	35	rVB	36385	50477	1.60%	0.185%
2	3.657	93	97	112	rBV	213644	301998	9.58%	1.105%
3	3.981	148	152	156	rVB2	9083	12739	0.40%	0.047%
4	6.981	649	662	676	rVB	203969	336385	10.67%	1.230%
5	7.145	682	690	700	rVB	264637	418130	13.26%	1.529%
6	7.334	715	722	732	rBV	284018	460497	14.60%	1.684%
7	7.804	794	802	810	rBV	624029	982021	31.14%	3.592%
8	8.522	916	924	937	rBV	290479	482165	15.29%	1.763%
9	8.969	992	1000	1010	rBV	282387	470057	14.91%	1.719%
10	9.251	1039	1048	1049	rBV9	1957	3546	0.11%	0.013%
11	9.381	1066	1070	1076	rVB6	5070	9155	0.29%	0.033%
12	9.686	1115	1122	1132	rBV	203334	349551	11.09%	1.278%
13	10.228	1206	1214	1223	rBV	343747	583840	18.52%	2.135%
14	10.598	1270	1277	1286	rVB	781839	1313495	41.66%	4.804%
15	10.745	1295	1302	1316	rBV	315397	592224	18.78%	2.166%
16	11.798	1479	1481	1487	rVB6	2466	4948	0.16%	0.018%
17	11.869	1491	1493	1497	rVB5	4298	6012	0.19%	0.022%
18	12.198	1544	1549	1556	rBV8	5675	13499	0.43%	0.049%
19	12.416	1583	1586	1591	rBV6	2158	3746	0.12%	0.014%
20	12.816	1648	1654	1658	rBV7	3512	7024	0.22%	0.026%
21	13.345	1741	1744	1752	rVB6	9925	16241	0.52%	0.059%
22	13.733	1805	1810	1812	rBV5	3285	4239	0.13%	0.016%
23	13.869	1825	1833	1841	rBV	672461	951955	30.19%	3.482%
24	14.139	1872	1879	1888	rBV	710662	1084679	34.40%	3.967%
25	14.204	1888	1890	1892	rVB3	4237	3194	0.10%	0.012%
26	14.269	1899	1901	1908	rBV7	1919	3332	0.11%	0.012%
27	14.451	1924	1932	1939	rBV	1209291	1773271	56.24%	6.485%
28	14.669	1961	1969	1991	rBV	118138	265644	8.42%	0.972%
29	14.821	1991	1995	1997	rVB4	2698	3298	0.10%	0.012%
30	14.886	2004	2006	2013	rVB8	3463	6475	0.21%	0.024%
31	15.245	2065	2067	2072	rBV5	3330	3869	0.12%	0.014%
32	15.445	2094	2101	2111	rBV	1071398	1489560	47.24%	5.448%
33	15.574	2117	2123	2131	rBV	234597	349816	11.09%	1.279%
34	15.686	2139	2142	2145	rVB5	3829	4321	0.14%	0.016%
35	15.869	2171	2173	2178	rVB6	3906	6473	0.21%	0.024%
36	16.233	2230	2235	2241	rBV8	4579	7804	0.25%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019138.D
 Acq On : 28 Dec 2023 22:47
 Operator : MA/JU
 Sample : 06021-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	16.680	2307	2311	2313	rVB5	3203	4126	0.13%	0.015%
38	16.992	2361	2364	2368	rVB4	4174	6070	0.19%	0.022%
39	17.204	2394	2400	2409	rBV	1579576	2202219	69.84%	8.054%
40	17.304	2411	2417	2429	rVV	1214583	1738386	55.13%	6.358%
41	17.874	2511	2514	2516	rBV4	3341	4705	0.15%	0.017%
42	18.098	2548	2552	2560	rBV4	27804	45034	1.43%	0.165%
43	19.121	2723	2726	2731	rBV6	17267	25836	0.82%	0.094%
44	19.198	2735	2739	2741	rBV2	18385	24160	0.77%	0.088%
45	19.339	2759	2763	2770	rBV9	19185	37688	1.20%	0.138%
46	19.551	2793	2799	2806	rBV	1683836	2262377	71.75%	8.274%
47	21.309	3093	3098	3106	rBV	2293118	2900113	91.97%	10.607%
48	23.515	3467	3473	3480	rBV	1355905	2562742	81.27%	9.373%
49	23.674	3493	3500	3512	rVB	1587105	3153193	100.00%	11.532%




Sum of corrected areas: 27342329

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019138.D
Acq On : 28 Dec 2023 22:47
Operator : MA/JU
Sample : 06021-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

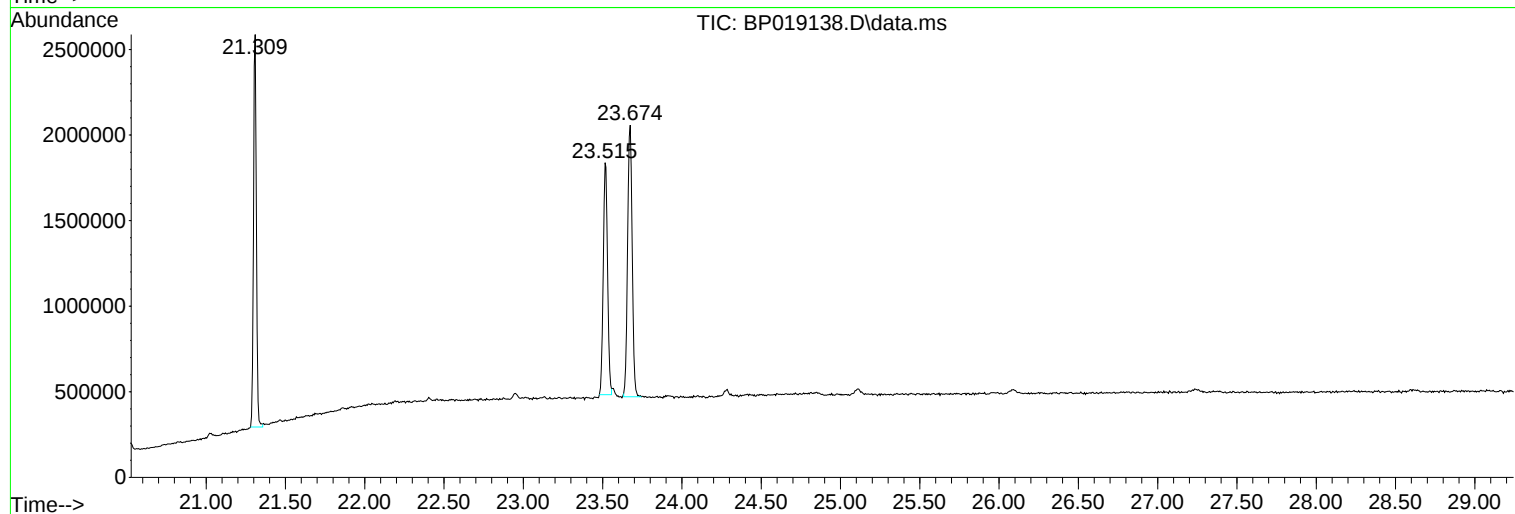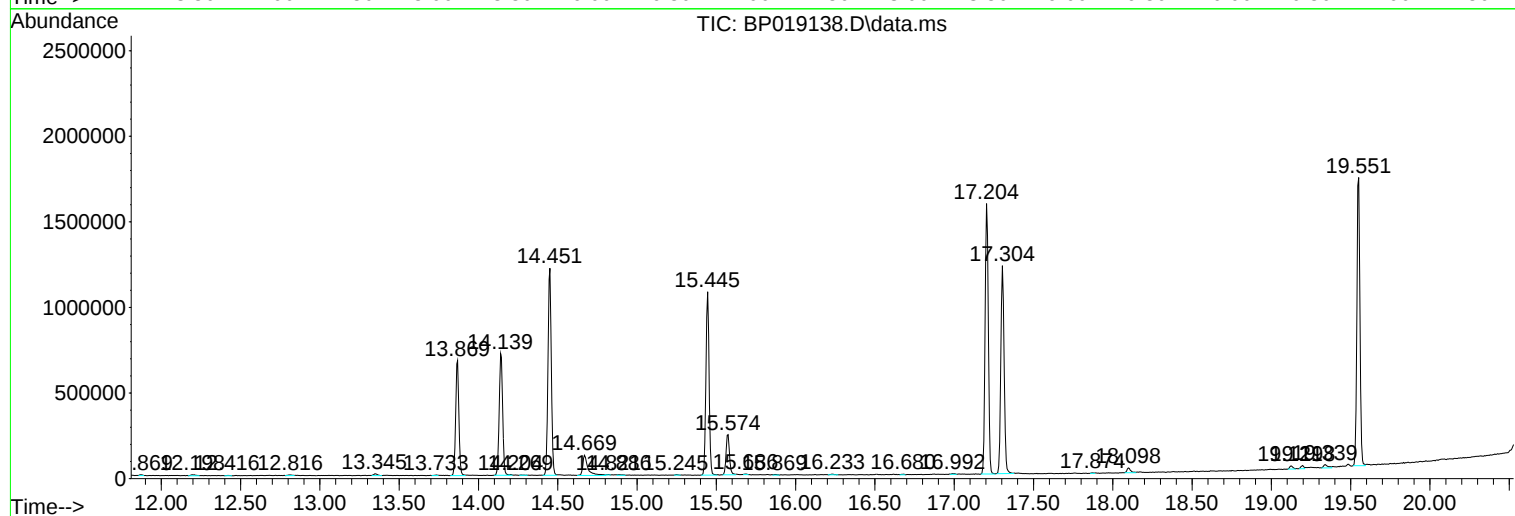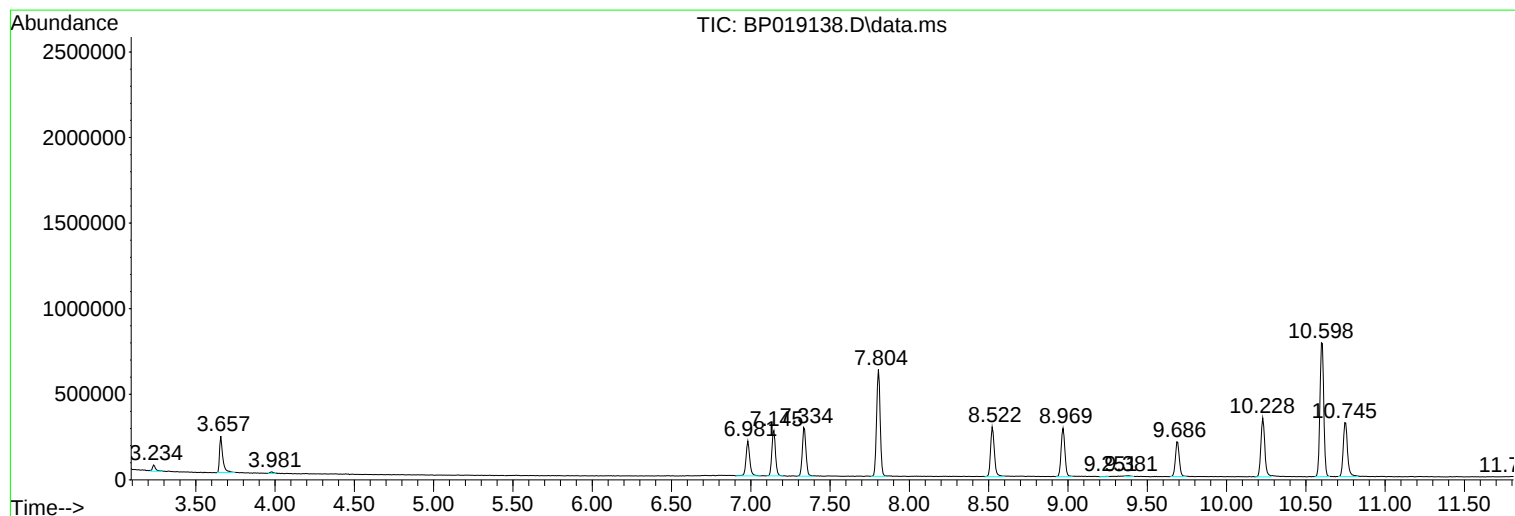

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019138.D
Acq On : 28 Dec 2023 22:47
Operator : MA/JU
Sample : 06021-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019138.D
Acq On : 28 Dec 2023 22:47
Operator : MA/JU
Sample : 06021-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc