

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019140.D
 Acq On : 28 Dec 2023 23:55
 Operator : MA/JU
 Sample : 06021-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH800

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	34	rVB	51514	66948	0.91%	0.123%
2	3.658	94	97	109	rBV	146040	216017	2.95%	0.396%
3	3.881	132	135	140	rVB3	10321	14373	0.20%	0.026%
4	3.975	147	151	159	rBV	27503	39363	0.54%	0.072%
5	4.905	305	309	310	rBV2	7171	8665	0.12%	0.016%
6	5.346	380	384	388	rVB2	7606	10066	0.14%	0.018%
7	5.893	473	477	481	rBV3	6379	8816	0.12%	0.016%
8	6.816	630	634	639	rVB4	6912	9414	0.13%	0.017%
9	6.981	652	662	675	rVB	237663	399129	5.44%	0.731%
10	7.146	683	690	699	rVB	847171	1305848	17.81%	2.392%
11	7.334	716	722	736	rVB	831416	1275392	17.39%	2.337%
12	7.805	793	802	810	rBV	657378	1004150	13.69%	1.840%
13	7.875	810	814	820	rVB	23634	36896	0.50%	0.068%
14	8.428	905	908	914	rVB4	10299	15934	0.22%	0.029%
15	8.522	916	924	933	rBV	632110	1009028	13.76%	1.849%
16	8.634	938	943	949	rVB	24961	40104	0.55%	0.073%
17	8.904	984	989	994	rBV	82573	135192	1.84%	0.248%
18	8.969	994	1000	1015	rVV	972258	1552560	21.17%	2.844%
19	9.093	1018	1021	1024	rVV4	6958	10616	0.14%	0.019%
20	9.140	1024	1029	1038	rVB4	6072	14539	0.20%	0.027%
21	9.375	1063	1069	1075	rVB	27703	44944	0.61%	0.082%
22	9.687	1115	1122	1134	rBV	728250	1217541	16.60%	2.231%
23	9.863	1144	1152	1158	rBV9	6799	16972	0.23%	0.031%
24	9.934	1160	1164	1176	rVB6	9772	20367	0.28%	0.037%
25	10.228	1205	1214	1224	rBV	1116445	1883103	25.68%	3.450%
26	10.516	1256	1263	1271	rBV7	18962	41961	0.57%	0.077%
27	10.598	1271	1277	1284	rVV	792680	1343355	18.32%	2.461%
28	10.663	1284	1288	1293	rVB5	11161	18402	0.25%	0.034%
29	10.746	1293	1302	1314	rBV	622943	1083975	14.78%	1.986%
30	11.263	1385	1390	1398	rVB	13011	26207	0.36%	0.048%
31	11.410	1407	1415	1427	rBV2	34002	64425	0.88%	0.118%
32	11.781	1473	1478	1483	rBV2	8108	17329	0.24%	0.032%
33	11.869	1488	1493	1496	rBV	29959	48066	0.66%	0.088%
34	11.904	1496	1499	1505	rVB	38165	60115	0.82%	0.110%
35	12.193	1541	1548	1556	rVB	22326	40013	0.55%	0.073%
36	12.734	1634	1640	1648	rBV7	10190	19138	0.26%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019140.D
 Acq On : 28 Dec 2023 23:55
 Operator : MA/JU
 Sample : 06021-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH800

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	12.804	1648	1652	1660	rVB7	7552	16917	0.23%	0.031%
38	13.057	1690	1695	1705	rVB5	12012	25124	0.34%	0.046%
39	13.381	1741	1750	1763	rVB2	62443	134758	1.84%	0.247%
40	13.734	1806	1810	1815	rBV6	6372	10113	0.14%	0.019%
41	13.869	1825	1833	1839	rBV	2068739	2858770	38.99%	5.237%
42	14.139	1871	1879	1888	rBV	2272818	3366078	45.91%	6.167%
43	14.322	1905	1910	1915	rBV2	8051	12565	0.17%	0.023%
44	14.451	1925	1932	1941	rBV	1225463	1830791	24.97%	3.354%
45	14.669	1960	1969	1983	rBV	138663	274357	3.74%	0.503%
46	14.875	1996	2004	2011	rVB	8612	21109	0.29%	0.039%
47	15.134	2038	2048	2053	rBV2	12198	22032	0.30%	0.040%
48	15.257	2064	2069	2077	rBV4	15909	35319	0.48%	0.065%
49	15.445	2094	2101	2108	rBV	3057275	4418731	60.26%	8.095%
50	15.569	2116	2122	2136	rBV	913515	1261838	17.21%	2.312%
51	15.681	2138	2141	2147	rVV3	16116	27963	0.38%	0.051%
52	15.816	2160	2164	2170	rVV	12287	19261	0.26%	0.035%
53	16.228	2230	2234	2239	rBV5	10658	16259	0.22%	0.030%
54	16.798	2328	2331	2337	rBV5	6381	11334	0.15%	0.021%
55	16.881	2342	2345	2351	rVB8	6233	9557	0.13%	0.018%
56	17.204	2390	2400	2410	rBV	1550197	2199064	29.99%	4.029%
57	17.304	2410	2417	2429	rBV	3534106	4901506	66.85%	8.980%
58	17.498	2447	2450	2456	rVB	10468	12472	0.17%	0.023%
59	17.786	2496	2499	2502	rBV3	9031	9432	0.13%	0.017%
60	17.880	2510	2515	2525	rBV	154766	208564	2.84%	0.382%
61	18.057	2540	2545	2548	rBV7	6062	12395	0.17%	0.023%
62	18.098	2548	2552	2558	rBV	55978	73674	1.00%	0.135%
63	18.175	2562	2565	2566	rBV	8903	8683	0.12%	0.016%
64	18.298	2584	2586	2590	rVB4	8943	10639	0.15%	0.019%
65	18.386	2597	2601	2604	rVB4	19262	24180	0.33%	0.044%
66	18.592	2632	2636	2641	rVB5	28577	38180	0.52%	0.070%
67	18.933	2690	2694	2698	rBV	30254	37742	0.51%	0.069%
68	19.122	2722	2726	2731	rBV2	51229	76045	1.04%	0.139%
69	19.192	2734	2738	2745	rBV	49305	73581	1.00%	0.135%
70	19.339	2759	2763	2772	rBV3	48418	73971	1.01%	0.136%
71	19.551	2793	2799	2810	rBV	4702798	6236380	85.05%	11.425%
72	21.310	3093	3098	3104	rBV	2086556	2718997	37.08%	4.981%
73	23.521	3466	3474	3487	rVB2	3876552	7332475	100.00%	13.433%
74	23.674	3493	3500	3509	rVB	1548437	3045151	41.53%	5.579%

Sum of corrected areas: 54584970




Instrument :
BNA_P
ClientSampleId :
BH800

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019140.D
Acq On : 28 Dec 2023 23:55
Operator : MA/JU
Sample : 06021-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

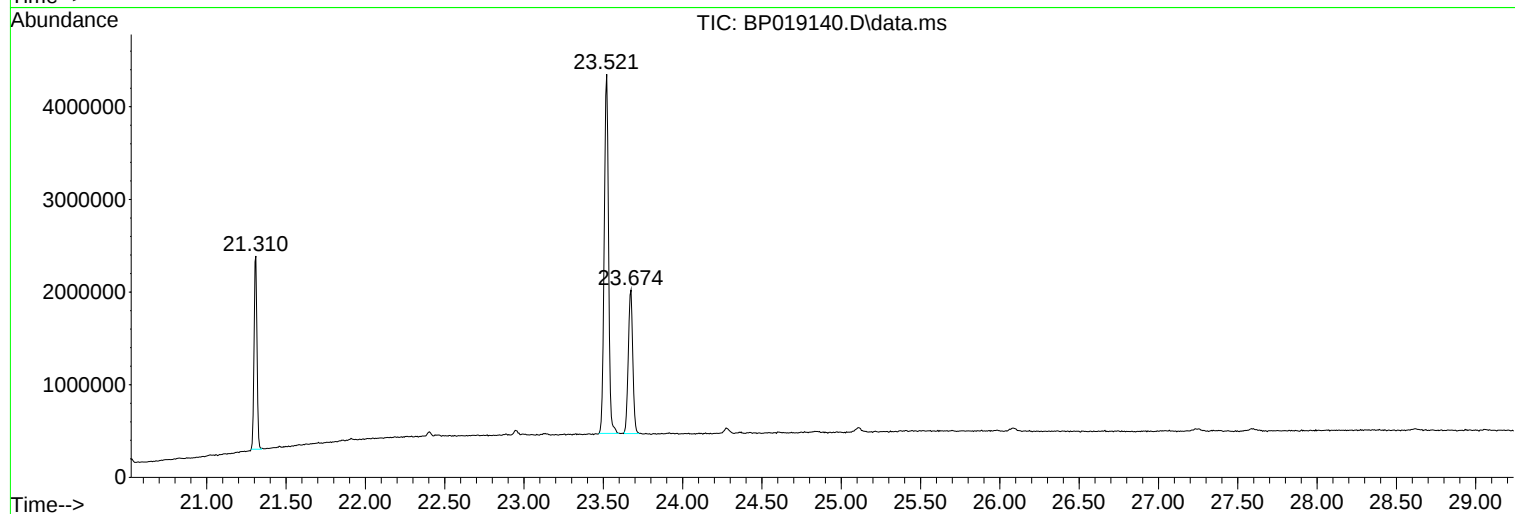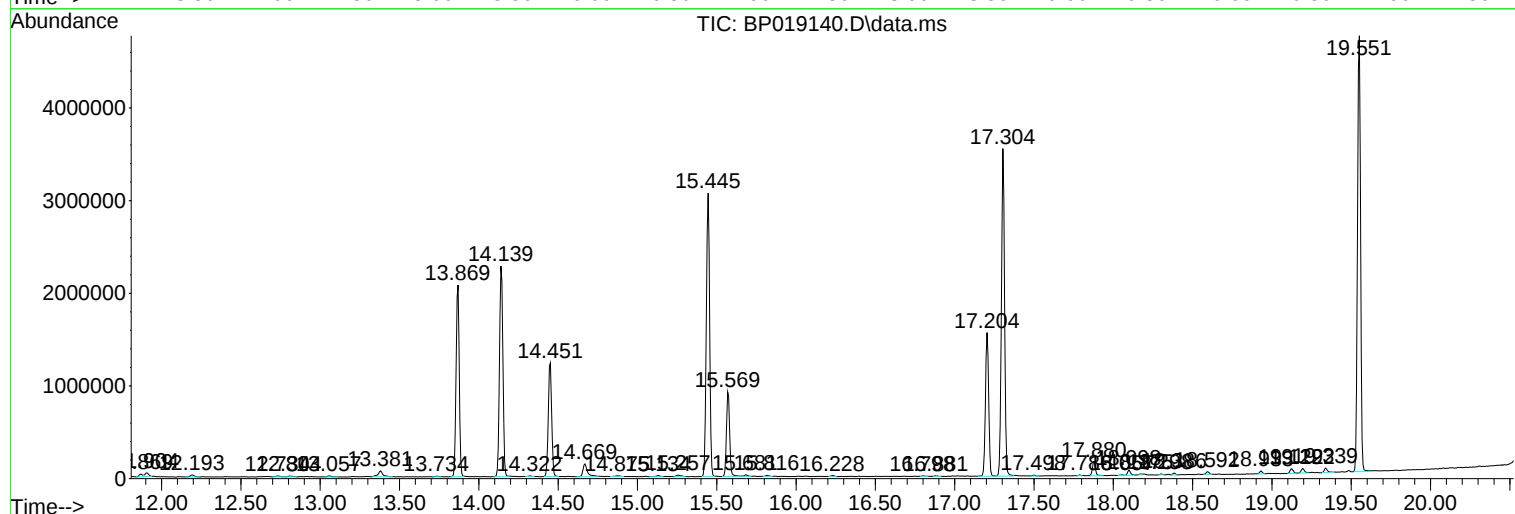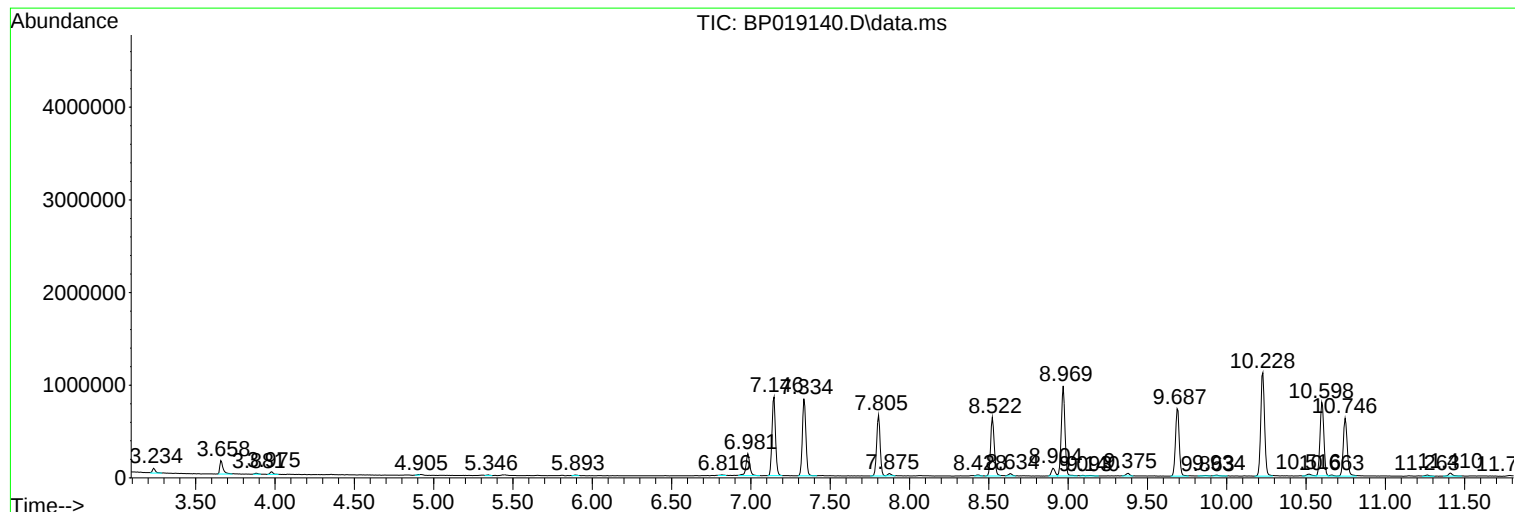

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019140.D
Acq On : 28 Dec 2023 23:55
Operator : MA/JU
Sample : 06021-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH800










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phenol, 2-methoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.904	2.69 ng/ul	135192	1,4-Dichlorobenzene-d4	7.805

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	96
2			Mequinol	124	C7H8O2	000150-76-5	90
3			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	90
4			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	90
5			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	64

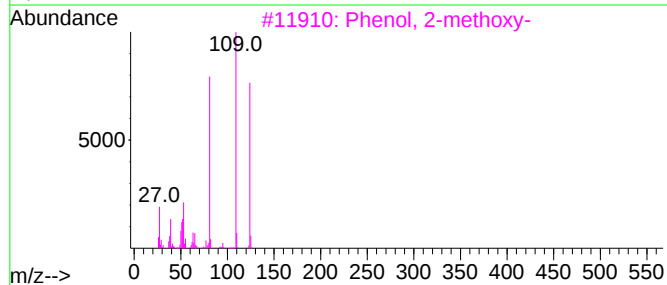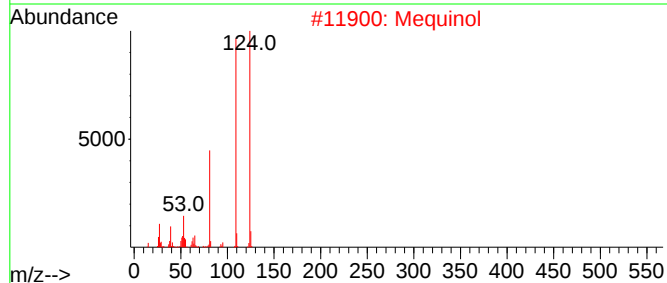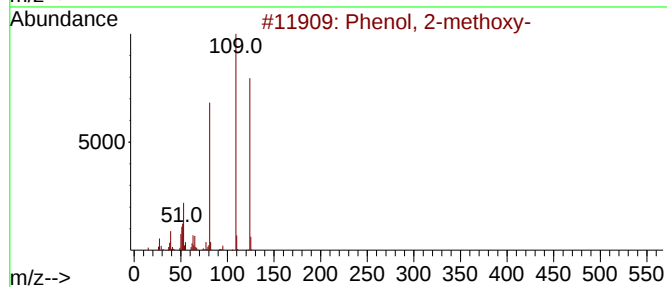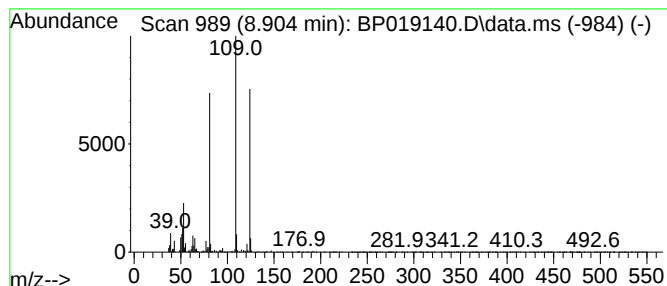

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019140.D
Acq On : 28 Dec 2023 23:55
Operator : MA/JU
Sample : 06021-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH800

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 2-methoxy-	8.904	2.7	ng/u1	135192	1	7.805	1004150	20.0