

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019144.D
 Acq On : 29 Dec 2023 02:45
 Operator : MA/JU
 Sample : PB158024BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	30	rBV	59136	67360	1.27%	0.155%
2	3.652	92	96	118	rBV	667660	940265	17.76%	2.164%
3	3.975	148	151	156	rVB	11150	14240	0.27%	0.033%
4	6.981	654	662	676	rVB	694573	1090916	20.61%	2.511%
5	7.146	683	690	698	rBV	575585	895827	16.92%	2.062%
6	7.334	715	722	734	rBV	721650	1116454	21.09%	2.570%
7	7.805	795	802	811	rBV	599389	941452	17.79%	2.167%
8	8.522	912	924	937	rBV	839080	1340968	25.33%	3.086%
9	8.969	993	1000	1009	rBV	636293	1030441	19.47%	2.372%
10	9.687	1112	1122	1131	rBV	517963	827992	15.64%	1.906%
11	10.228	1206	1214	1226	rBV	794467	1380210	26.08%	3.177%
12	10.599	1269	1277	1288	rVB	765155	1275124	24.09%	2.935%
13	10.746	1293	1302	1320	rBV	785600	1373710	25.95%	3.162%
14	11.875	1486	1494	1496	rBV9	3331	5828	0.11%	0.013%
15	12.204	1543	1550	1558	rVB3	10525	22408	0.42%	0.052%
16	13.346	1738	1744	1749	rBV6	9289	14948	0.28%	0.034%
17	13.422	1752	1757	1764	rBV6	3090	7050	0.13%	0.016%
18	13.863	1825	1832	1844	rBV	1361468	1916769	36.21%	4.412%
19	14.140	1872	1879	1892	rBV2	1583860	2315740	43.75%	5.330%
20	14.445	1924	1931	1942	rBV	1127812	1663878	31.44%	3.830%
21	14.663	1961	1968	1992	rBV	520587	887649	16.77%	2.043%
22	15.245	2060	2067	2070	rBV9	3711	7463	0.14%	0.017%
23	15.445	2093	2101	2111	rBV	2086772	2979433	56.29%	6.858%
24	15.569	2116	2122	2133	rVV	551346	777043	14.68%	1.788%
25	15.681	2137	2141	2146	rVB5	8881	14172	0.27%	0.033%
26	16.228	2230	2234	2239	rBV7	6798	10295	0.19%	0.024%
27	16.875	2342	2344	2351	rVB7	3582	5834	0.11%	0.013%
28	17.204	2393	2400	2409	rBV	1469979	2024651	38.25%	4.660%
29	17.304	2410	2417	2430	rVV	2265733	3245746	61.32%	7.471%
30	18.098	2546	2552	2557	rBV9	9379	18636	0.35%	0.043%
31	19.122	2723	2726	2731	rBV3	35319	43167	0.82%	0.099%
32	19.192	2735	2738	2744	rBV	28472	41043	0.78%	0.094%
33	19.545	2793	2798	2805	rBV	3203899	4212484	79.59%	9.696%
34	21.304	3092	3097	3104	rBV	2080644	2676338	50.56%	6.160%
35	23.516	3467	3473	3489	rVB2	2561726	5292966	100.00%	12.183%
36	23.669	3493	3499	3512	rVB	1454101	2968322	56.08%	6.832%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019144.D
Acq On : 29 Dec 2023 02:45
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 43446822

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019144.D
Acq On : 29 Dec 2023 02:45
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

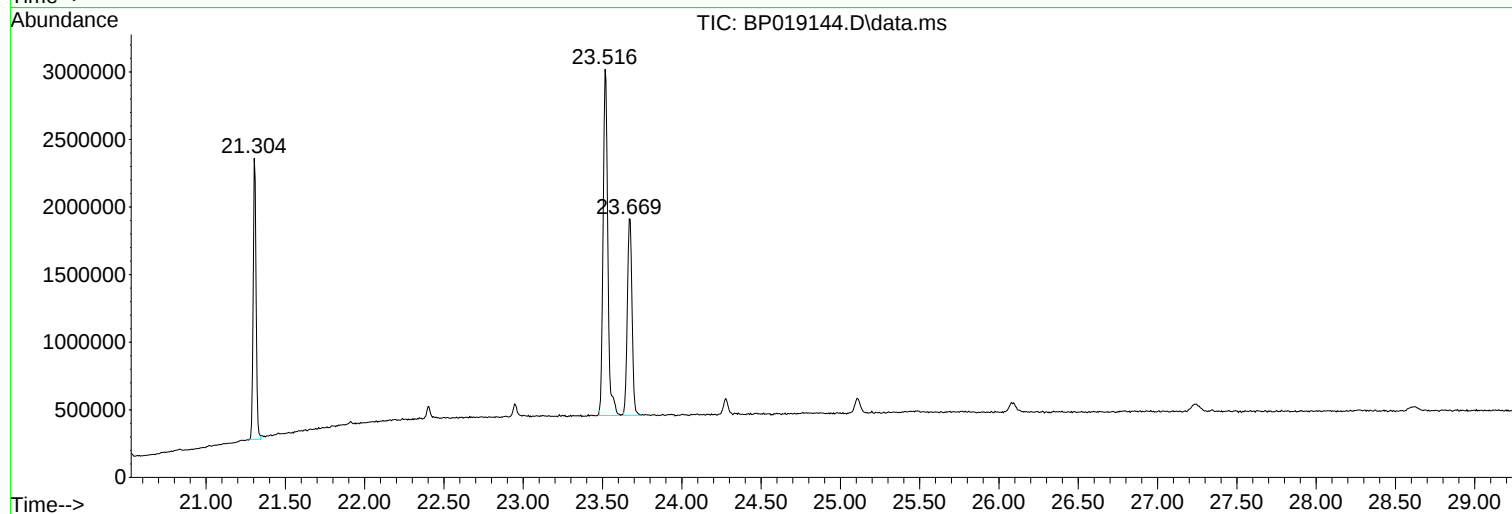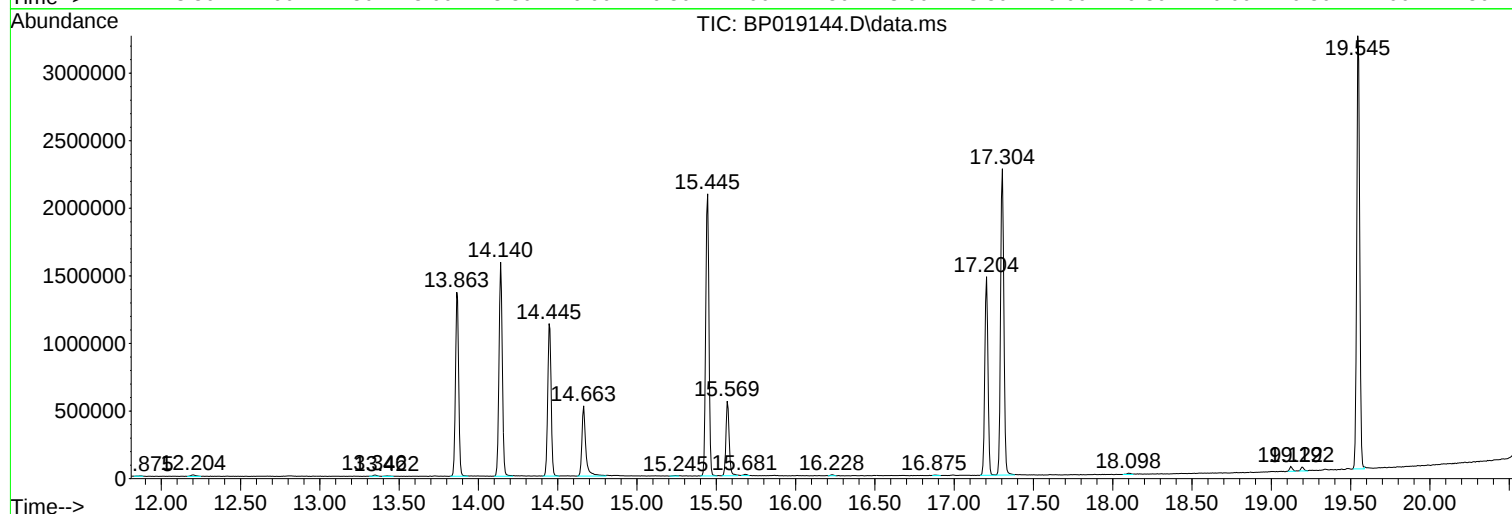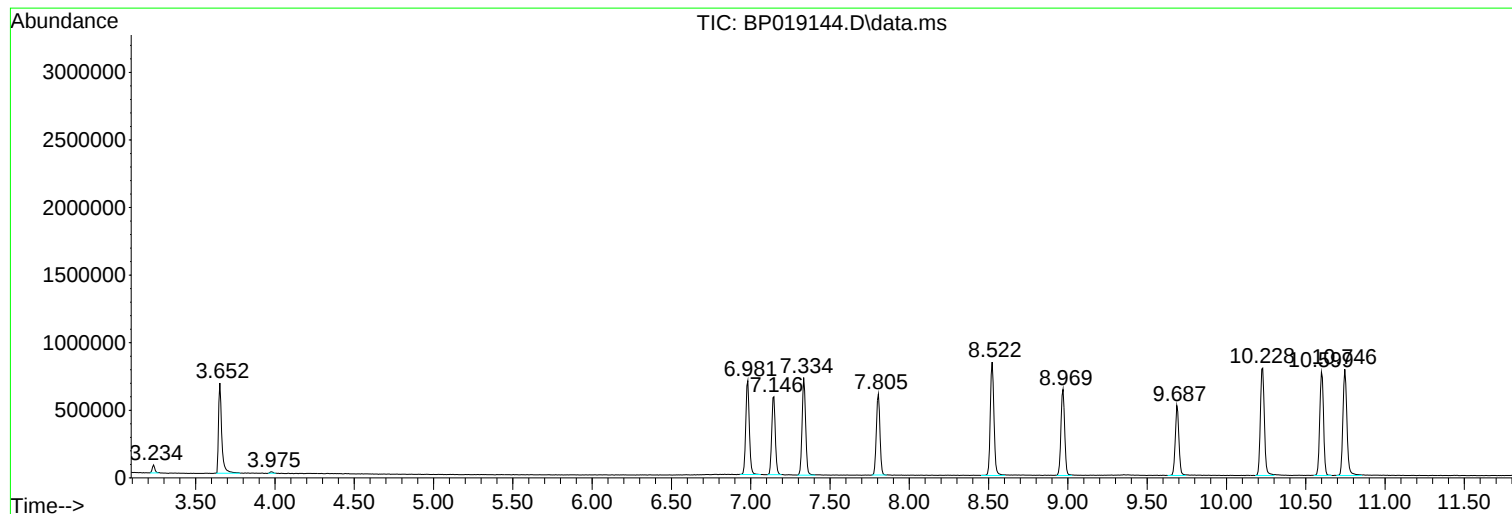

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019144.D
Acq On : 29 Dec 2023 02:45
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019144.D
Acq On : 29 Dec 2023 02:45
Operator : MA/JU
Sample : PB158024BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------